

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025755.D
 Acq On : 25 Mar 2020 07:31
 Operator : CG/JU
 Sample : L1161-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.763	145	149	153	rBV3	13747	20583	0.57%	0.121%
2	3.846	159	163	169	rBV4	12082	17975	0.50%	0.106%
3	4.063	198	200	202	rBV3	3886	4156	0.12%	0.024%
4	4.151	213	215	218	rBV3	2404	3607	0.10%	0.021%
5	4.387	251	255	258	rVB4	4550	6469	0.18%	0.038%
6	4.740	310	315	322	rBV	35060	59001	1.65%	0.347%
7	6.739	650	655	657	rVB4	3504	4979	0.14%	0.029%
8	7.569	789	796	804	rBV	779240	1182197	32.99%	6.944%
9	8.775	998	1001	1004	rBV3	2292	3721	0.10%	0.022%
10	10.333	1259	1266	1275	rVV	1034520	1643593	45.86%	9.655%
11	10.910	1359	1364	1367	rVB5	2589	4437	0.12%	0.026%
12	12.727	1671	1673	1680	rVB3	3221	6831	0.19%	0.040%
13	13.633	1825	1827	1832	rVB2	6248	6138	0.17%	0.036%
14	13.892	1868	1871	1876	rVB5	2820	4154	0.12%	0.024%
15	14.204	1918	1924	1934	rBV	1539786	2274275	63.46%	13.359%
16	15.051	2065	2068	2071	rVB3	3620	4180	0.12%	0.025%
17	15.210	2090	2095	2101	rVB5	5494	8372	0.23%	0.049%
18	15.262	2101	2104	2109	rVB5	3603	5102	0.14%	0.030%
19	15.586	2155	2159	2162	rBV3	2768	3646	0.10%	0.021%
20	15.686	2174	2176	2180	rBV3	3089	4161	0.12%	0.024%
21	15.968	2222	2224	2227	rVB4	3103	3720	0.10%	0.022%
22	16.739	2351	2355	2361	rVB3	9224	14767	0.41%	0.087%
23	16.951	2385	2391	2403	rVV	2042983	2781806	77.63%	16.341%
24	17.051	2403	2408	2414	rVB	13185	19632	0.55%	0.115%
25	17.651	2504	2510	2512	rBV4	2958	4668	0.13%	0.027%
26	17.703	2516	2519	2522	rBV4	2505	3609	0.10%	0.021%
27	17.874	2545	2548	2551	rVB3	3888	4118	0.11%	0.024%
28	17.939	2557	2559	2561	rBV3	4252	3638	0.10%	0.021%
29	19.080	2749	2753	2755	rBV3	18743	21036	0.59%	0.124%
30	19.315	2787	2793	2797	rBV3	34553	50411	1.41%	0.296%
31	19.345	2797	2798	2802	rVV4	13824	15268	0.43%	0.090%
32	19.380	2802	2804	2805	rVV	4516	3895	0.11%	0.023%
33	19.403	2805	2808	2810	rVV2	10227	12630	0.35%	0.074%
34	19.439	2810	2814	2818	rVB3	26189	32421	0.90%	0.190%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025755.D
 Acq On : 25 Mar 2020 07:31
 Operator : CG/JU
 Sample : L1161-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	19.939	2896	2899	2903	rVB5	13719	14921	0.42%	0.088%
36	20.162	2935	2937	2939	rVB3	7715	4823	0.13%	0.028%
37	20.368	2969	2972	2974	rBV3	21240	17559	0.49%	0.103%
38	20.439	2981	2984	2986	rVB	21154	21245	0.59%	0.125%
39	20.468	2986	2989	2992	rVB4	15553	16747	0.47%	0.098%
40	20.897	3059	3062	3065	rBV2	41987	48070	1.34%	0.282%
41	21.144	3099	3104	3112	rBV	2905191	3387350	94.52%	19.898%
42	21.333	3133	3136	3141	rBV2	91224	96630	2.70%	0.568%
43	21.756	3205	3208	3214	rVB	125467	136851	3.82%	0.804%
44	22.203	3280	3284	3290	rVB	181642	221609	6.18%	1.302%
45	22.686	3362	3366	3372	rVB	204803	287233	8.02%	1.687%
46	23.227	3454	3458	3463	rBV	224010	318455	8.89%	1.871%
47	23.291	3463	3469	3478	rVB2	1999807	3583619	100.00%	21.051%
48	23.844	3558	3563	3569	rVB	194592	341467	9.53%	2.006%
49	24.544	3678	3682	3690	rVB2	143056	287918	8.03%	1.691%


Sum of corrected areas: 17023693

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025755.D
Acq On : 25 Mar 2020 07:31
Operator : CG/JU
Sample : L1161-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

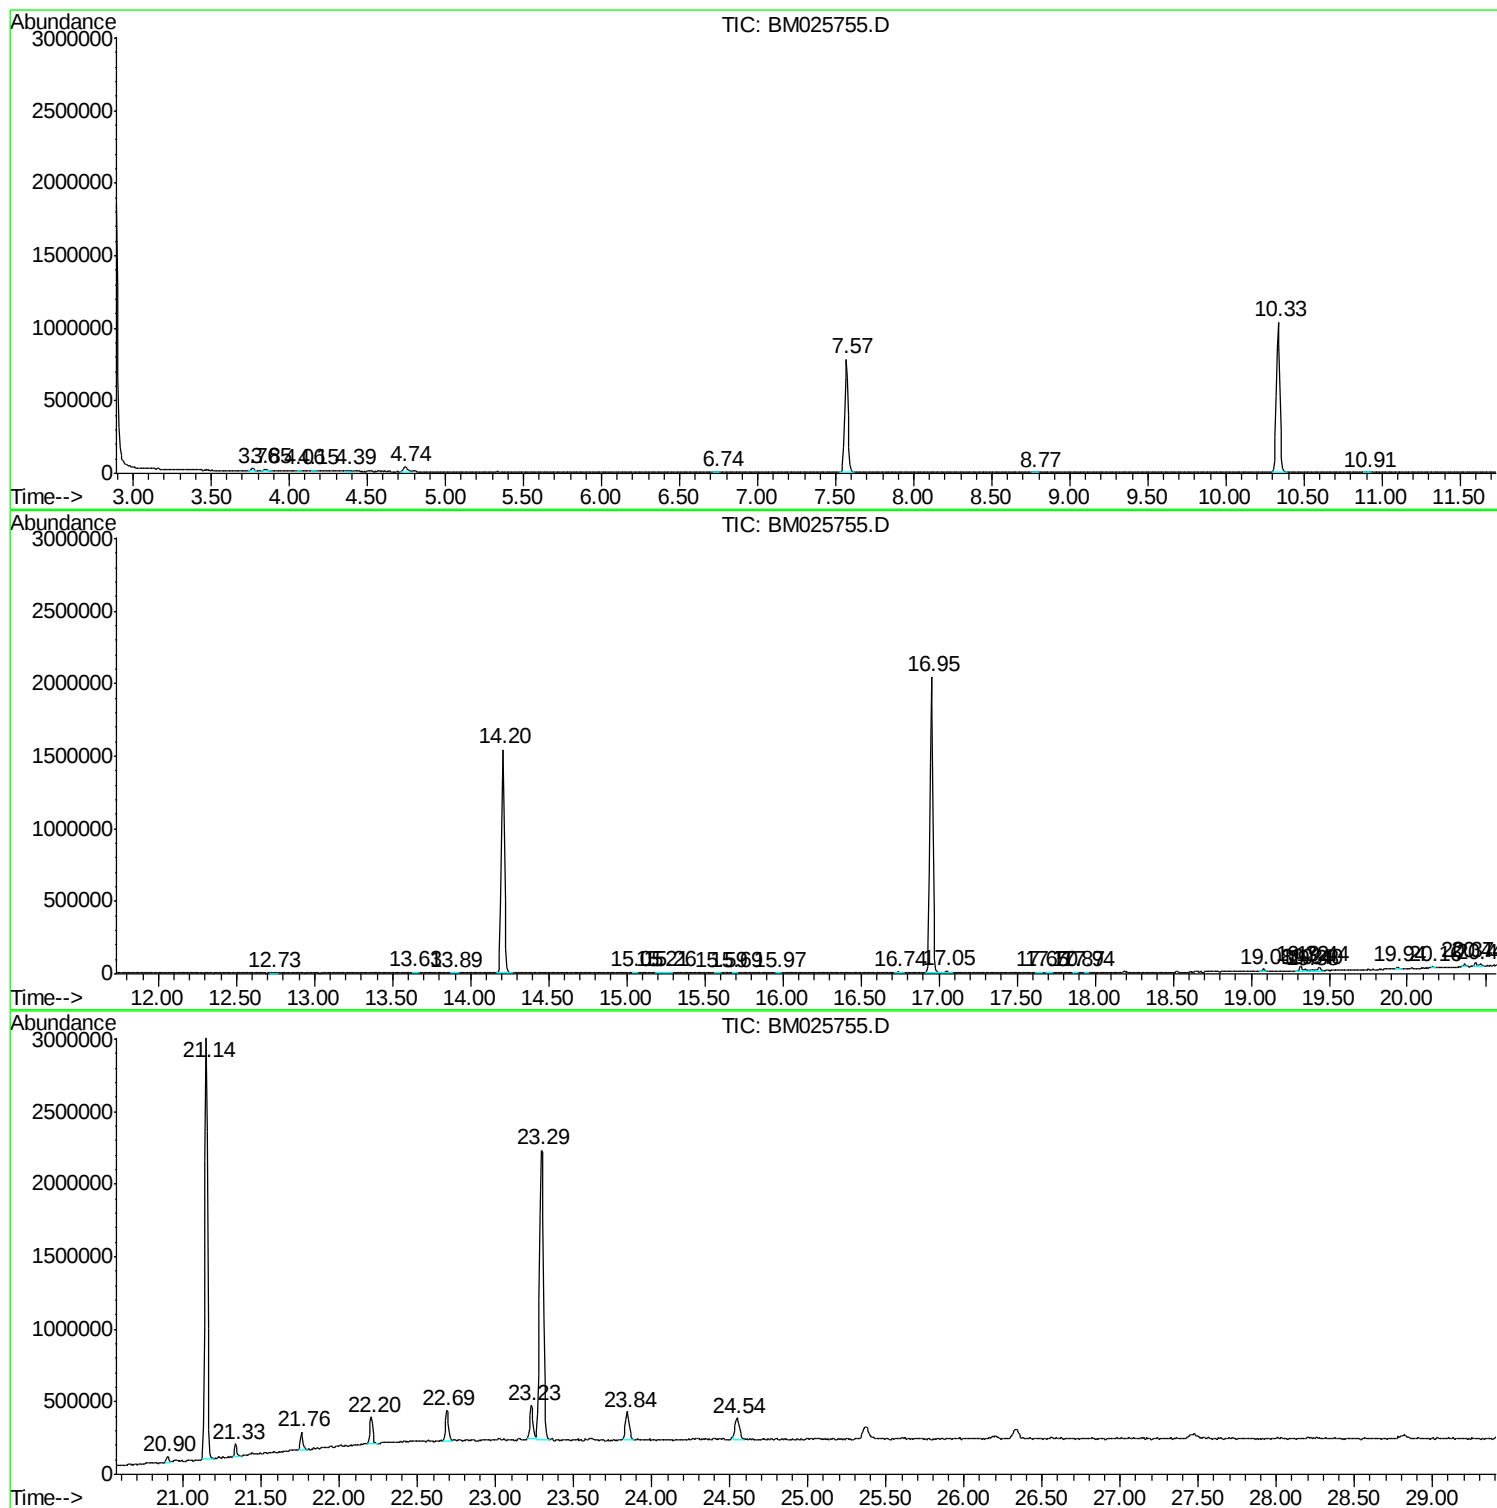

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025755.D
Acq On : 25 Mar 2020 07:31
Operator : CG/JU
Sample : L1161-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025755.D
Acq On : 25 Mar 2020 07:31
Operator : CG/JU
Sample : L1161-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc