

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034341.D
 Acq On : 23 Mar 2022 16:30
 Operator : CG/JU
 Sample : PB143412BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143412BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.495	377	384	397	rBV	4698649	6560838	47.44%	10.860%
2	7.101	649	657	672	rBV	4252546	6756461	48.85%	11.184%
3	7.937	792	799	808	rBV	775614	1222602	8.84%	2.024%
4	9.101	989	997	1020	rBV	2560264	4291199	31.03%	7.103%
5	10.748	1270	1277	1288	rBV	913660	1626538	11.76%	2.692%
6	13.207	1688	1695	1707	rBV	6653535	9782639	70.73%	16.193%
7	14.577	1922	1928	1942	rBV	1454869	2194160	15.86%	3.632%
8	16.065	2174	2181	2208	rBV	4896824	7534952	54.48%	12.473%
9	17.318	2388	2394	2410	rBV	1733824	2549430	18.43%	4.220%
10	19.936	2833	2839	2864	rBV	11047602	13830571	100.00%	22.894%
11	21.489	3098	3103	3120	rBV	1473875	2291921	16.57%	3.794%
12	23.906	3507	3514	3527	rBV2	756793	1771102	12.81%	2.932%




Sum of corrected areas: 60412413

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034341.D
Acq On : 23 Mar 2022 16:30
Operator : CG/JU
Sample : PB143412BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

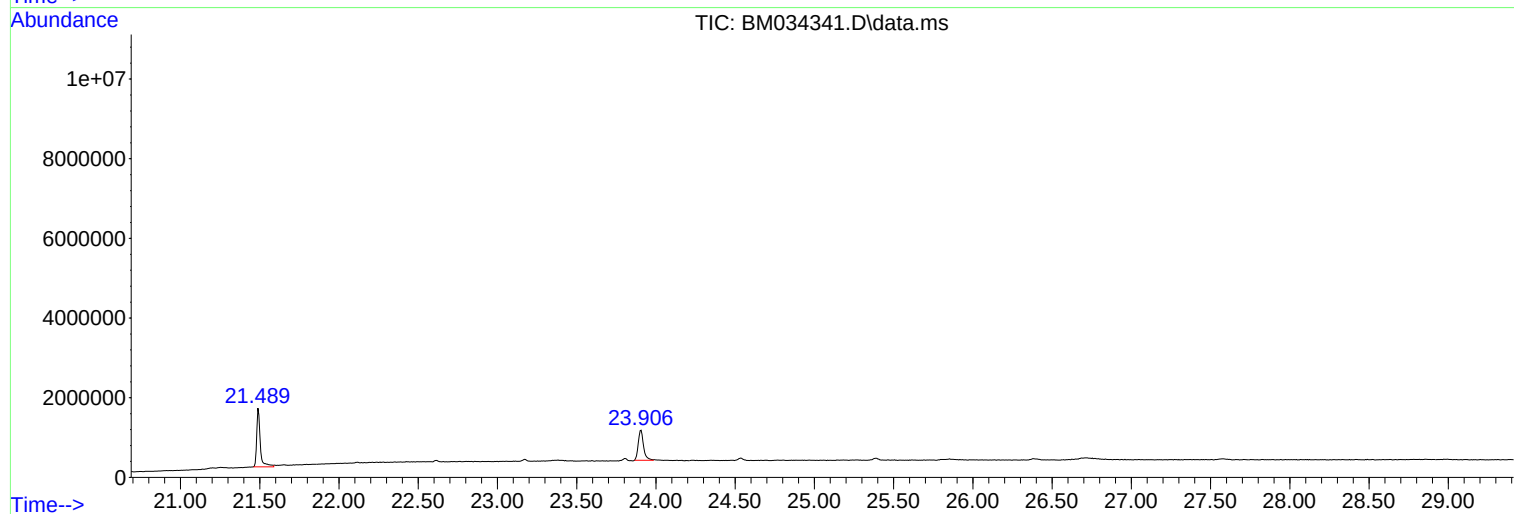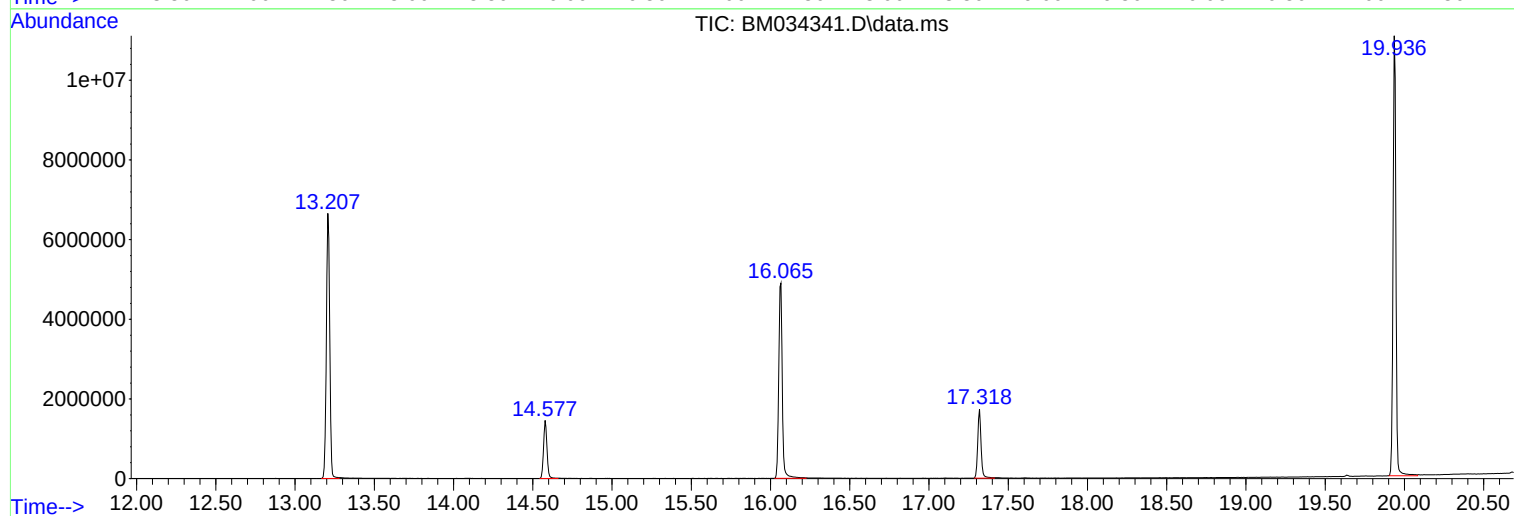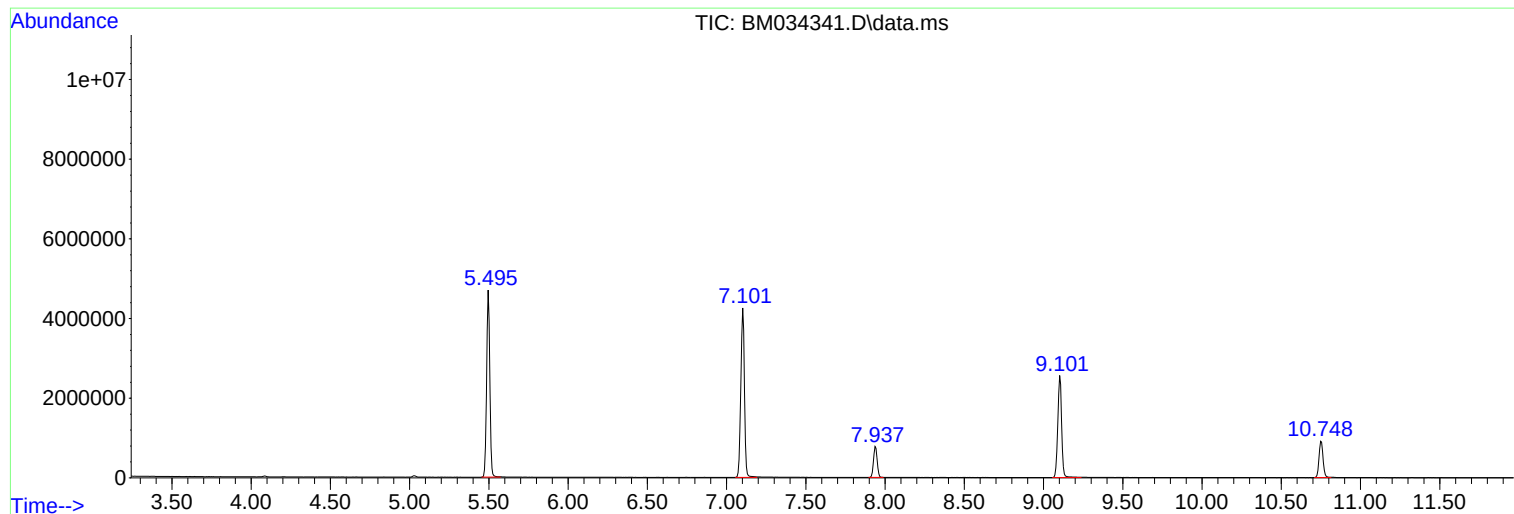

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034341.D
Acq On : 23 Mar 2022 16:30
Operator : CG/JU
Sample : PB143412BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034341.D
Acq On : 23 Mar 2022 16:30
Operator : CG/JU
Sample : PB143412BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143412BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------