

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034345.D
 Acq On : 23 Mar 2022 18:57
 Operator : CG/JU
 Sample : N2057-03 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 UST-7-NORTH-SIDEWALL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.490	377	383	393	rBV	632245	959850	44.07%	5.363%
2	7.095	649	656	669	rBV	615796	1000630	45.95%	5.591%
3	7.936	792	799	808	rBV	649527	1013637	46.54%	5.664%
4	9.095	989	996	1007	rBV	368673	635849	29.20%	3.553%
5	10.748	1267	1277	1286	rBV	857452	1424509	65.41%	7.960%
6	13.201	1687	1694	1704	rBV	947670	1398947	64.23%	7.817%
7	13.407	1721	1729	1737	rBV8	12391	27546	1.26%	0.154%
8	14.413	1893	1900	1908	rBV3	28502	74343	3.41%	0.415%
9	14.577	1921	1928	1936	rBV	1192890	1791658	82.27%	10.011%
10	16.059	2173	2180	2188	rBV	703041	1065337	48.92%	5.953%
11	17.130	2360	2362	2370	rVB7	15547	22278	1.02%	0.124%
12	17.312	2387	2393	2404	rBV	1330044	2000296	91.85%	11.177%
13	18.212	2541	2546	2555	rBV3	60495	104016	4.78%	0.581%
14	19.483	2760	2762	2767	rBV5	23786	38021	1.75%	0.212%
15	19.930	2833	2838	2850	rBV	1439687	1807090	82.98%	10.097%
16	21.194	3050	3053	3058	rBV2	133105	183110	8.41%	1.023%
17	21.489	3098	3103	3117	rBV	1504047	2171733	99.72%	12.135%
18	23.900	3507	3513	3528	rVB2	1031196	2177866	100.00%	12.169%




Sum of corrected areas: 17896716

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034345.D
Acq On : 23 Mar 2022 18:57
Operator : CG/JU
Sample : N2057-03 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
UST-7-NORTH-SIDEWALL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

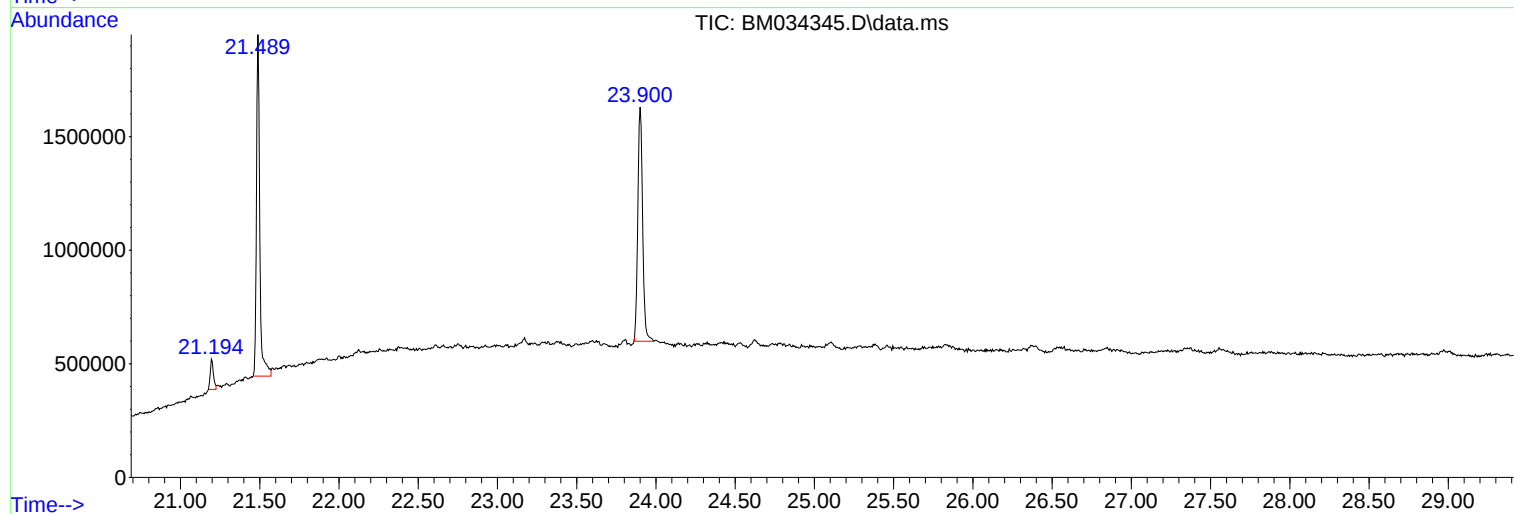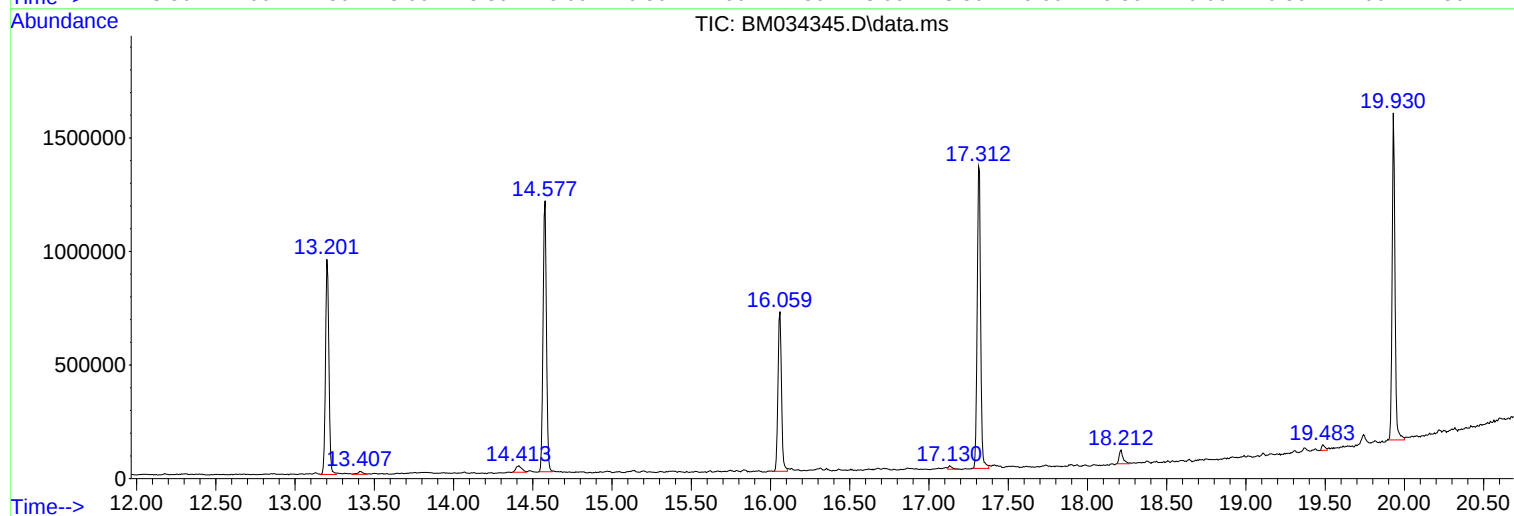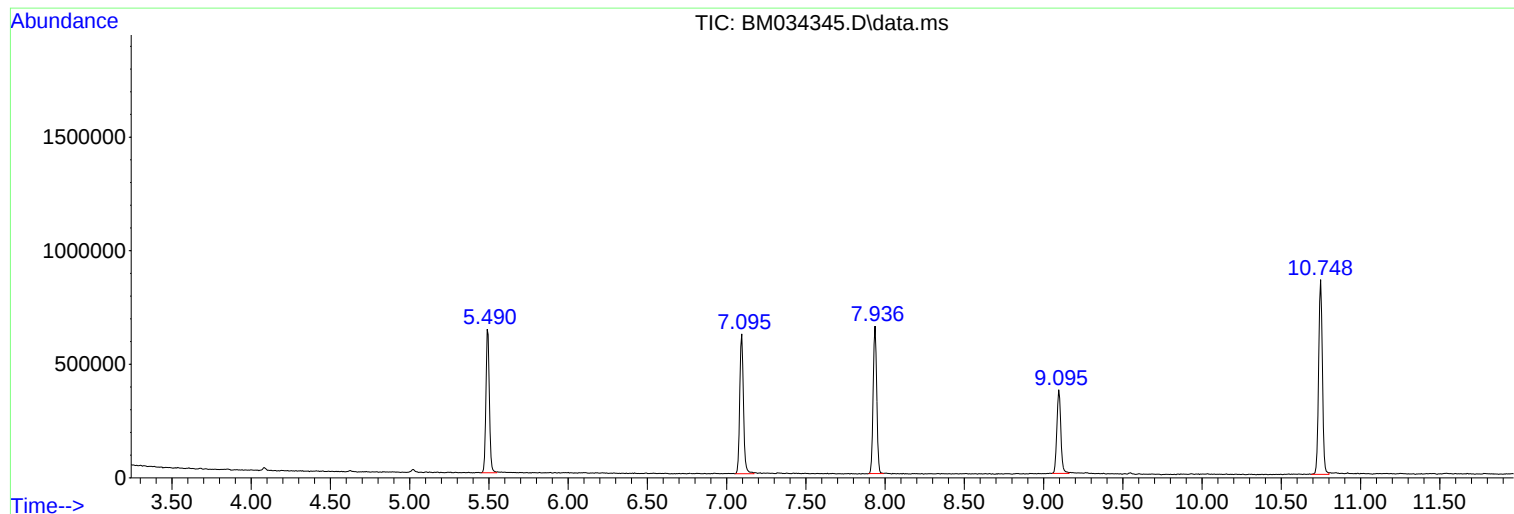

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034345.D
Acq On : 23 Mar 2022 18:57
Operator : CG/JU
Sample : N2057-03 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
UST-7-NORTH-SIDEWALL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034345.D
Acq On : 23 Mar 2022 18:57
Operator : CG/JU
Sample : N2057-03 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
UST-7-NORTH-SIDEWALL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------