

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034347.D
 Acq On : 23 Mar 2022 20:09
 Operator : CG/JU
 Sample : N1958-02 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C-2-1-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.084	140	144	150	rBV2	16927	25378	1.08%	0.136%
2	5.496	377	384	391	rBV	366203	573583	24.33%	3.065%
3	5.560	391	395	404	rVB2	16745	39492	1.67%	0.211%
4	5.931	451	458	463	rBV6	12953	34357	1.46%	0.184%
5	7.095	649	656	664	rBV	362711	597730	25.35%	3.194%
6	7.589	733	740	746	rBV3	17654	36204	1.54%	0.193%
7	7.937	792	799	807	rBV	677107	1069273	45.35%	5.713%
8	8.478	886	891	896	rBV	24368	41714	1.77%	0.223%
9	9.095	990	996	1009	rBV	216421	377574	16.01%	2.017%
10	10.748	1270	1277	1283	rBV	884694	1497340	63.50%	8.000%
11	10.795	1283	1285	1292	rVB	81076	118719	5.03%	0.634%
12	12.407	1555	1559	1566	rVB	19977	35623	1.51%	0.190%
13	13.201	1688	1694	1701	rBV	603581	886898	37.61%	4.739%
14	14.301	1876	1881	1889	rBV	25080	42759	1.81%	0.228%
15	14.407	1892	1899	1909	rBV3	30674	83620	3.55%	0.447%
16	14.577	1921	1928	1935	rBV	1285044	1875552	79.54%	10.021%
17	14.642	1935	1939	1949	rVB2	20803	40594	1.72%	0.217%
18	14.977	1992	1996	2004	rVB5	15516	31477	1.33%	0.168%
19	15.618	2101	2105	2111	rVB2	18100	23896	1.01%	0.128%
20	16.060	2174	2180	2188	rBV	423662	630159	26.73%	3.367%
21	17.136	2360	2363	2369	rVB	16889	25350	1.08%	0.135%
22	17.318	2387	2394	2398	rBV	1353402	2011671	85.32%	10.749%
23	17.359	2398	2401	2406	rVB	243328	326443	13.84%	1.744%
24	17.448	2412	2416	2421	rVB	63295	84729	3.59%	0.453%
25	17.718	2458	2462	2472	rBV4	15647	38320	1.63%	0.205%
26	18.206	2539	2545	2548	rBV3	65842	125950	5.34%	0.673%
27	18.242	2549	2551	2555	rVB	44620	51183	2.17%	0.273%
28	18.324	2561	2565	2571	rBV4	15329	23823	1.01%	0.127%
29	18.389	2571	2576	2580	rBV3	54378	101813	4.32%	0.544%
30	19.106	2695	2698	2701	rBV	29901	41181	1.75%	0.220%
31	19.371	2738	2743	2750	rBV	566622	778810	33.03%	4.161%
32	19.730	2796	2804	2814	rBV	483472	779128	33.04%	4.163%
33	19.930	2834	2838	2850	rVB	860929	1095626	46.47%	5.854%
34	21.400	3085	3088	3092	rVB	746285	804176	34.11%	4.297%
35	21.489	3097	3103	3107	rBV2	1568322	2357920	100.00%	12.599%
36	23.900	3507	3513	3520	rBV2	1011946	2007619	85.14%	10.727%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034347.D
Acq On : 23 Mar 2022 20:09
Operator : CG/JU
Sample : N1958-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-2-1-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 18715684

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034347.D
Acq On : 23 Mar 2022 20:09
Operator : CG/JU
Sample : N1958-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-2-1-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

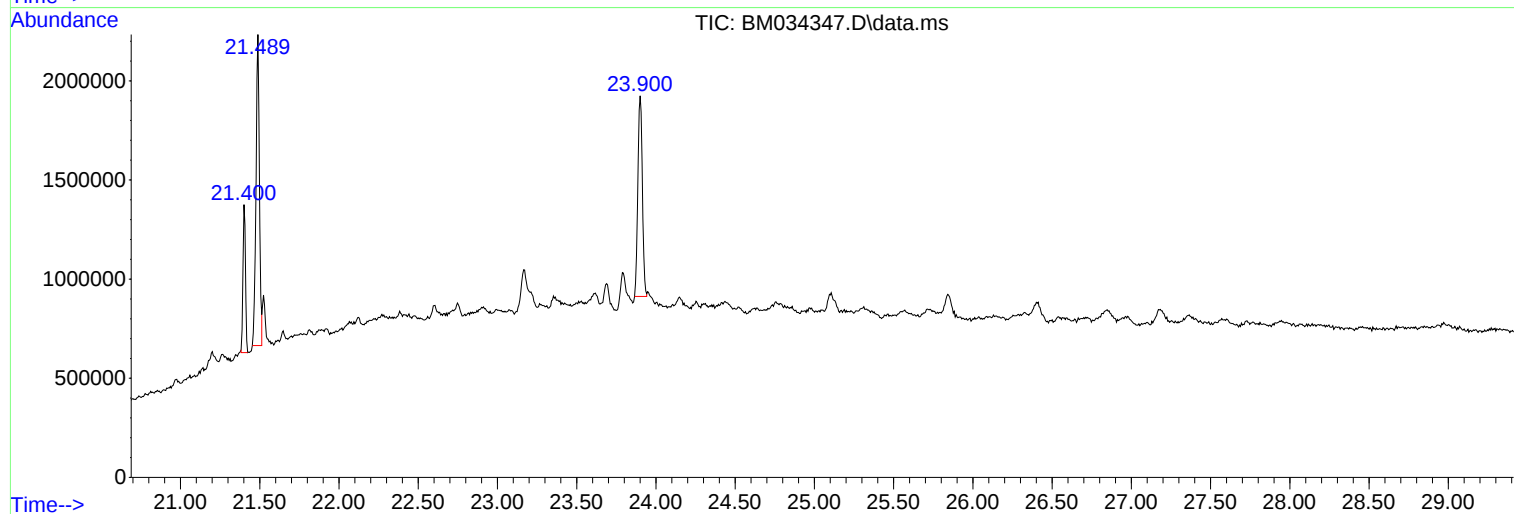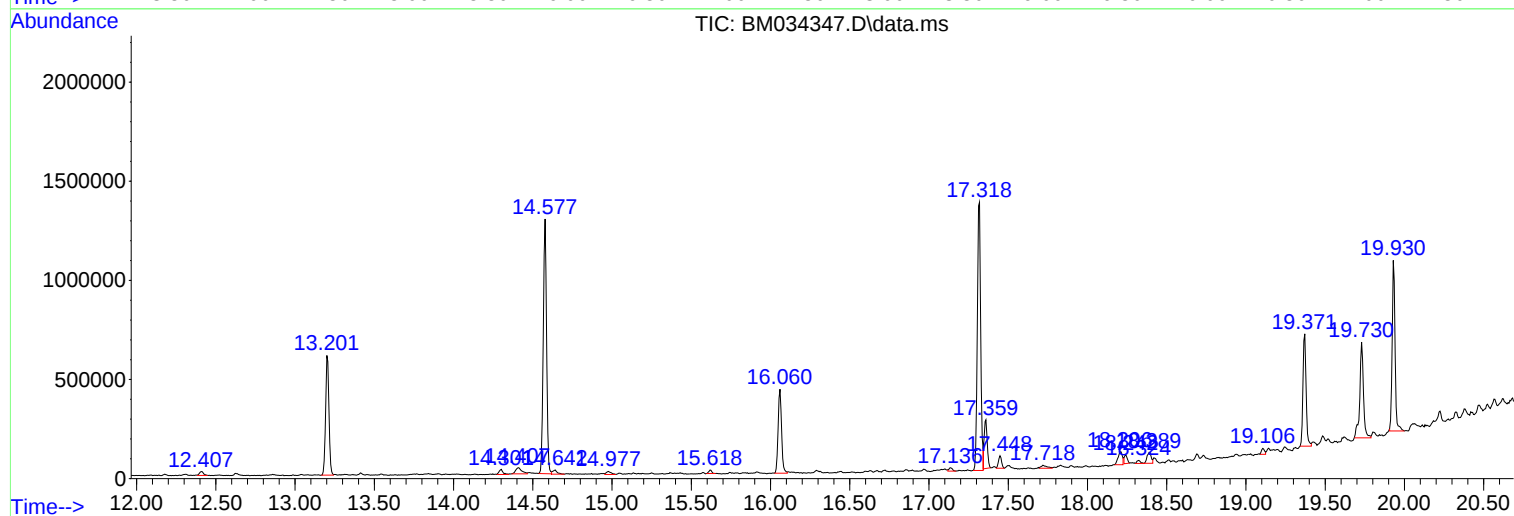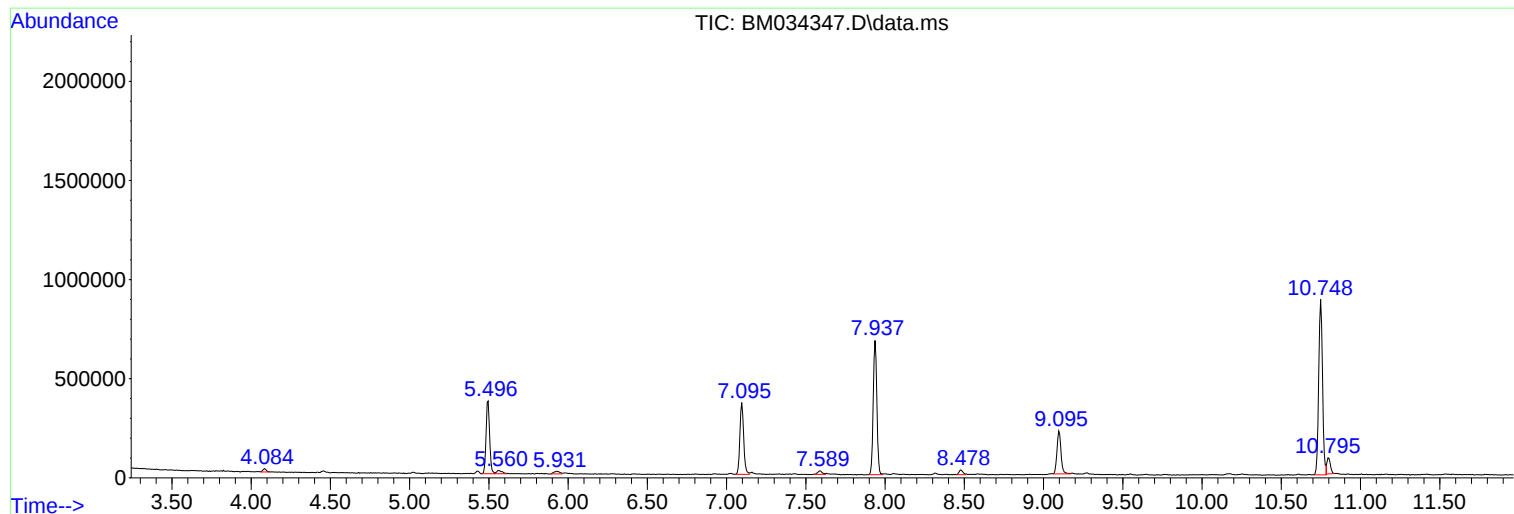

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034347.D
Acq On : 23 Mar 2022 20:09
Operator : CG/JU
Sample : N1958-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-2-1-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034347.D
Acq On : 23 Mar 2022 20:09
Operator : CG/JU
Sample : N1958-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-2-1-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------