

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034351.D
 Acq On : 23 Mar 2022 22:33
 Operator : CG/JU
 Sample : N1958-05 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C-5-4-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.078	140	143	149	rVB2	17665	23139	1.10%	0.141%
2	5.490	377	383	392	rBV	369269	551825	26.17%	3.361%
3	5.560	392	395	403	rVB2	15399	29241	1.39%	0.178%
4	5.937	450	459	463	rBV7	11854	31180	1.48%	0.190%
5	7.095	649	656	664	rBV	339168	553479	26.25%	3.371%
6	7.589	733	740	743	rBV4	19509	35632	1.69%	0.217%
7	7.936	792	799	807	rBV	693587	1080320	51.23%	6.579%
8	8.478	884	891	896	rBV2	19782	35904	1.70%	0.219%
9	9.095	990	996	1008	rBV	203533	358755	17.01%	2.185%
10	10.748	1269	1277	1283	rBV	868359	1457763	69.13%	8.878%
11	10.795	1283	1285	1292	rVB	74461	115437	5.47%	0.703%
12	12.407	1554	1559	1565	rVB3	18875	31601	1.50%	0.192%
13	12.630	1590	1597	1602	rBV3	13568	22341	1.06%	0.136%
14	13.201	1688	1694	1703	rVB	529367	801527	38.01%	4.882%
15	14.301	1875	1881	1887	rBV2	20880	39945	1.89%	0.243%
16	14.407	1891	1899	1908	rBV2	34051	99205	4.70%	0.604%
17	14.577	1921	1928	1935	rBV	1188804	1725451	81.82%	10.508%
18	14.977	1992	1996	2003	rVB4	10784	22815	1.08%	0.139%
19	16.059	2173	2180	2187	rBV	362950	558653	26.49%	3.402%
20	16.295	2216	2220	2226	rBV9	12796	25807	1.22%	0.157%
21	17.318	2388	2394	2398	rBV	1273962	1821181	86.36%	11.091%
22	17.359	2398	2401	2406	rVB	175130	243831	11.56%	1.485%
23	17.448	2413	2416	2421	rVB	34427	50610	2.40%	0.308%
24	18.212	2539	2546	2549	rBV2	69609	138243	6.56%	0.842%
25	18.389	2572	2576	2580	rBV3	34313	64730	3.07%	0.394%
26	19.148	2702	2705	2708	rBV5	26230	34557	1.64%	0.210%
27	19.371	2738	2743	2750	rBV	444361	630022	29.88%	3.837%
28	19.730	2800	2804	2814	rVB	343983	493055	23.38%	3.003%
29	19.930	2834	2838	2843	rBV	750256	952070	45.15%	5.798%
30	21.400	3086	3088	3093	rVB	233632	248189	11.77%	1.512%
31	21.489	3098	3103	3107	rBV	1456018	2034320	96.47%	12.390%
32	23.906	3508	3514	3530	rVB2	973178	2108858	100.00%	12.843%




Sum of corrected areas: 16419686

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034351.D
Acq On : 23 Mar 2022 22:33
Operator : CG/JU
Sample : N1958-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-5-4-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

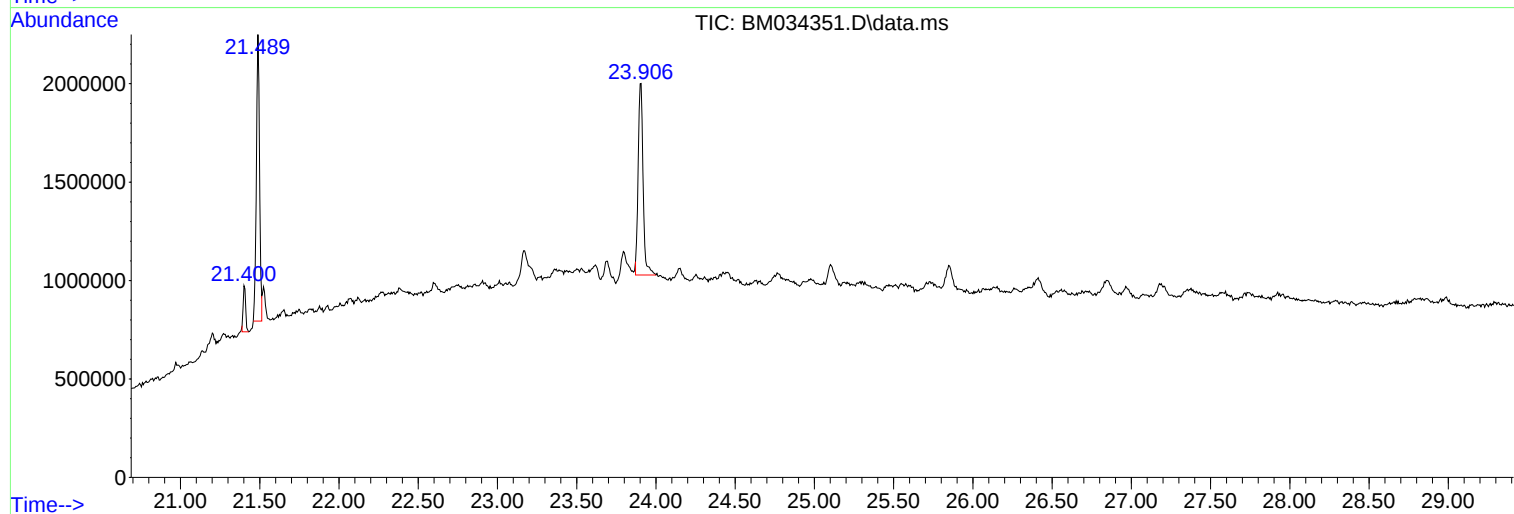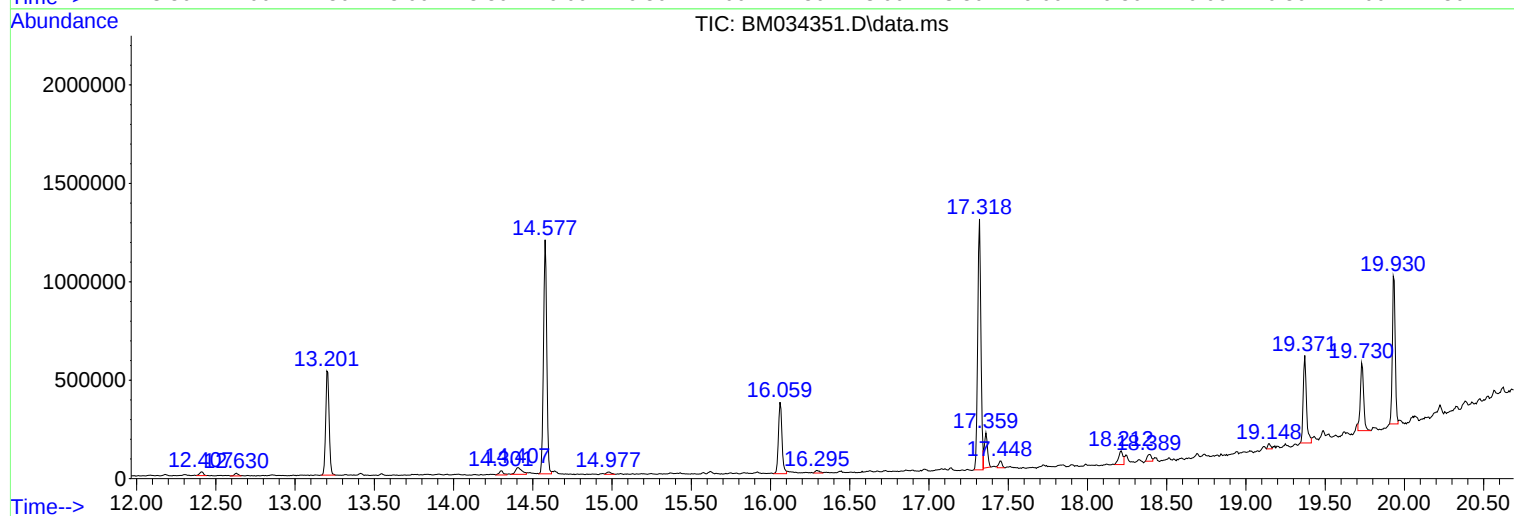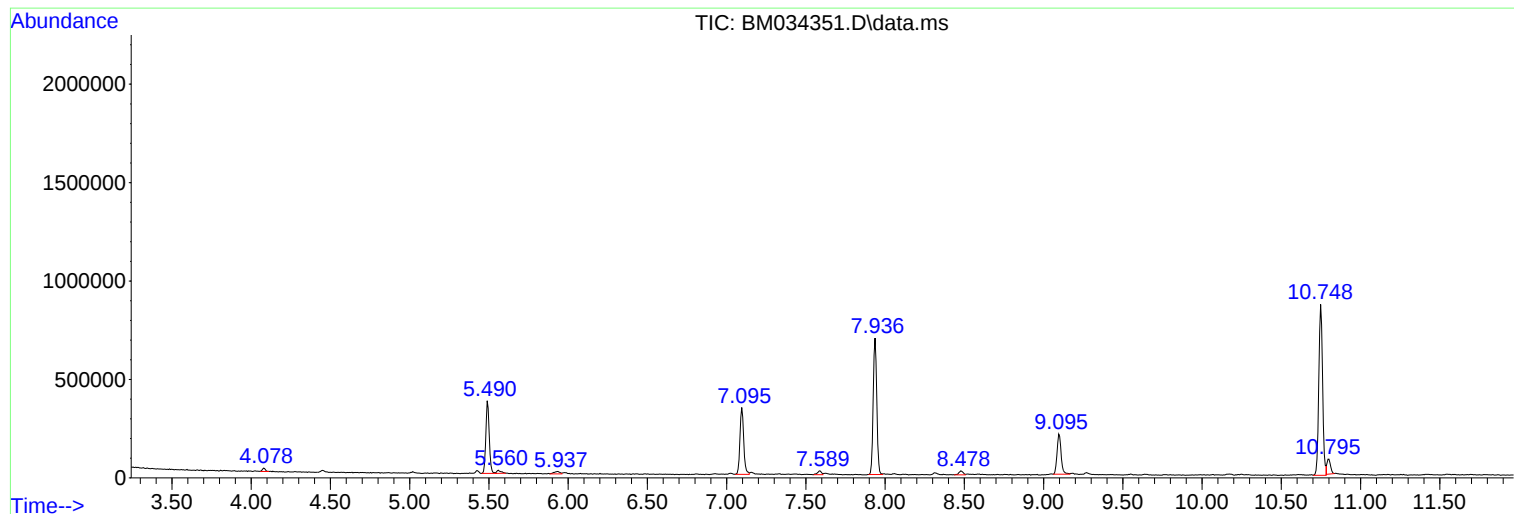

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034351.D
Acq On : 23 Mar 2022 22:33
Operator : CG/JU
Sample : N1958-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-5-4-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034351.D
Acq On : 23 Mar 2022 22:33
Operator : CG/JU
Sample : N1958-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-5-4-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------