


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034339.D
 Acq On : 23 Mar 2022 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 02:40:59 2022

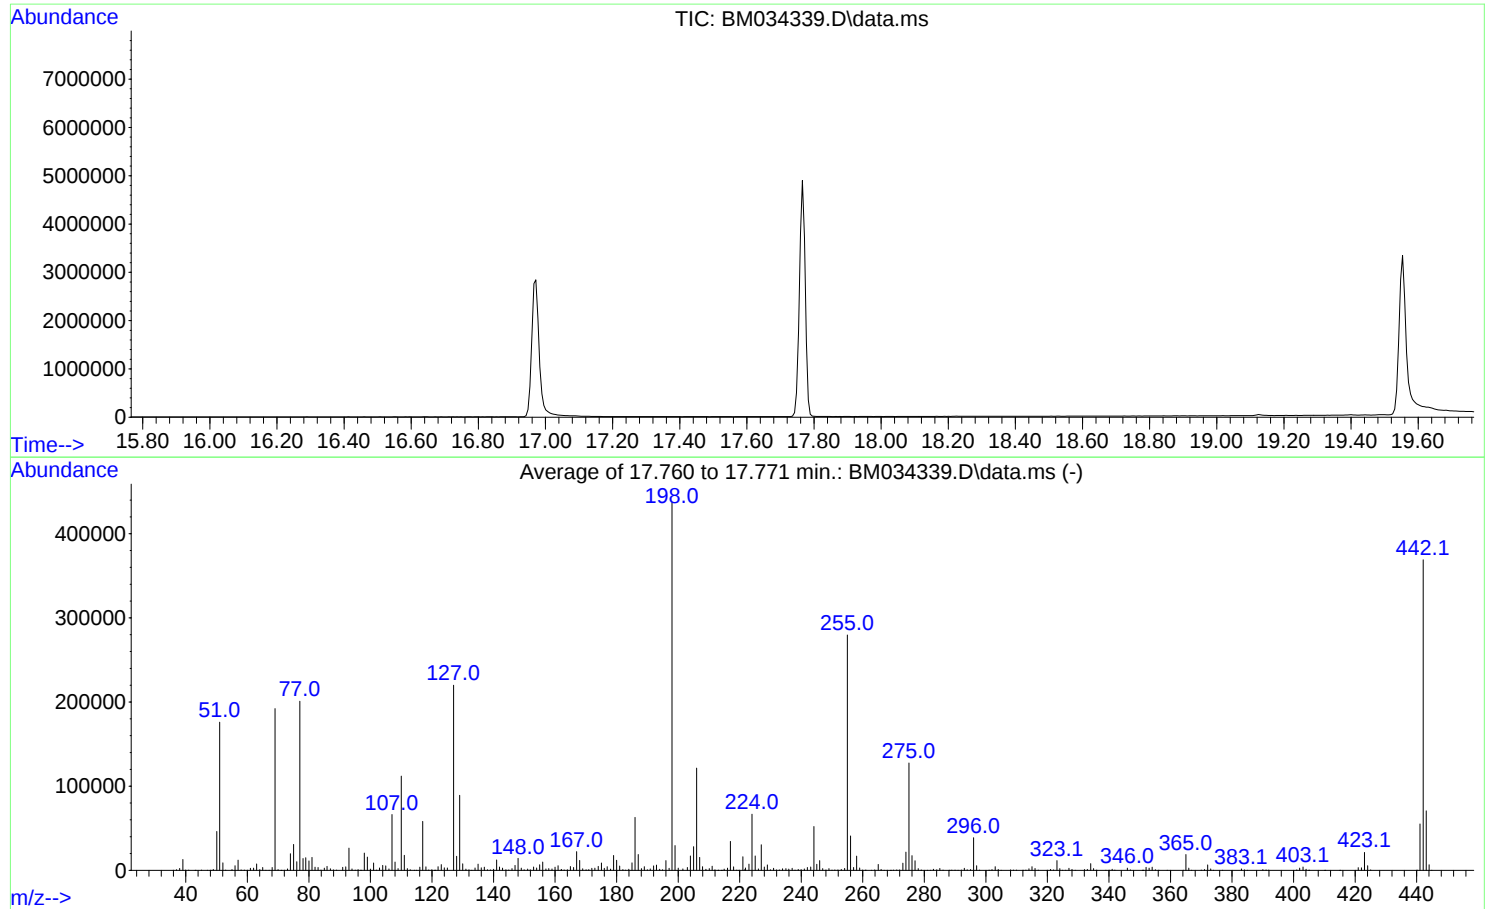




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	176064	PASS
68	69	0.00	2	1.8	3528	PASS
69	198	0.00	100	44.0	192171	PASS
70	69	0.00	2	0.5	948	PASS
127	198	10	80	50.3	219968	PASS
197	198	0.00	2	0.6	2492	PASS
198	198	100	100	100.0	437077	PASS
199	198	5	9	6.8	29560	PASS
275	198	10	60	29.2	127651	PASS
365	198	1	100	4.3	18805	PASS
441	198	0.01	100	12.6	55147	PASS
442	442	50	100	100.0	369045	PASS
443	442	15	24	19.2	70696	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
Data File : BM034339.D
Acq On : 23 Mar 2022 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 24 06:46:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 02:40:59 2022
Response via : Initial Calibration

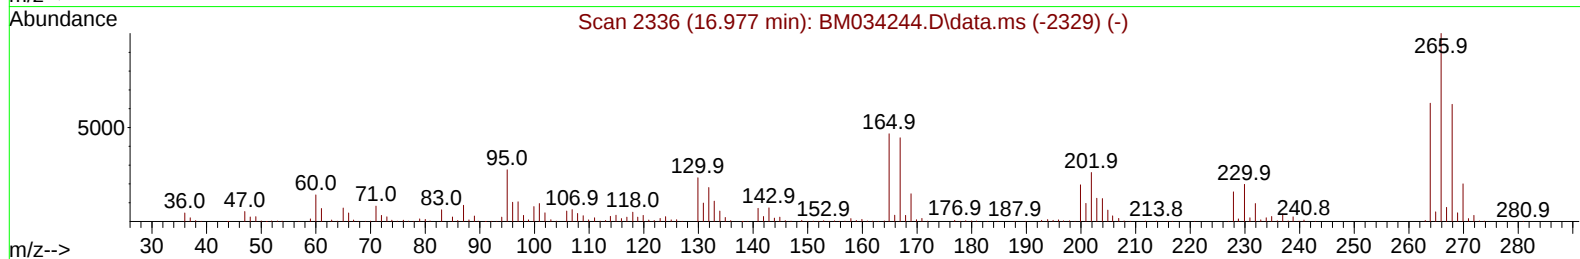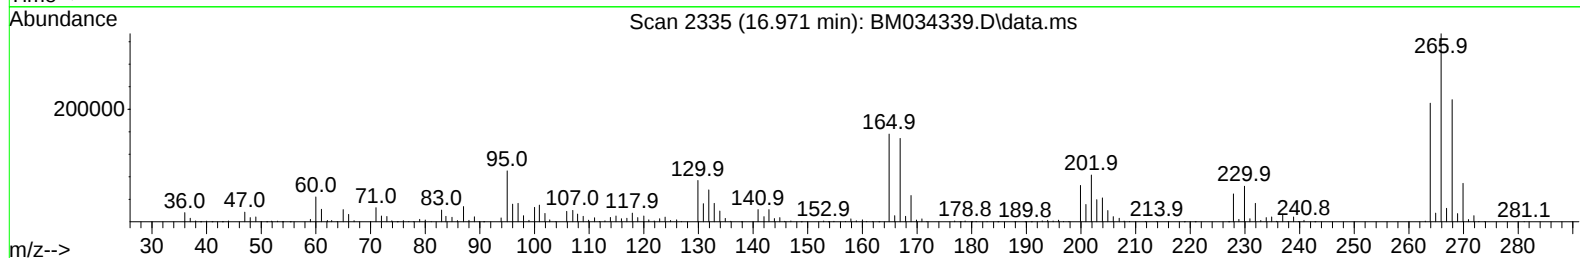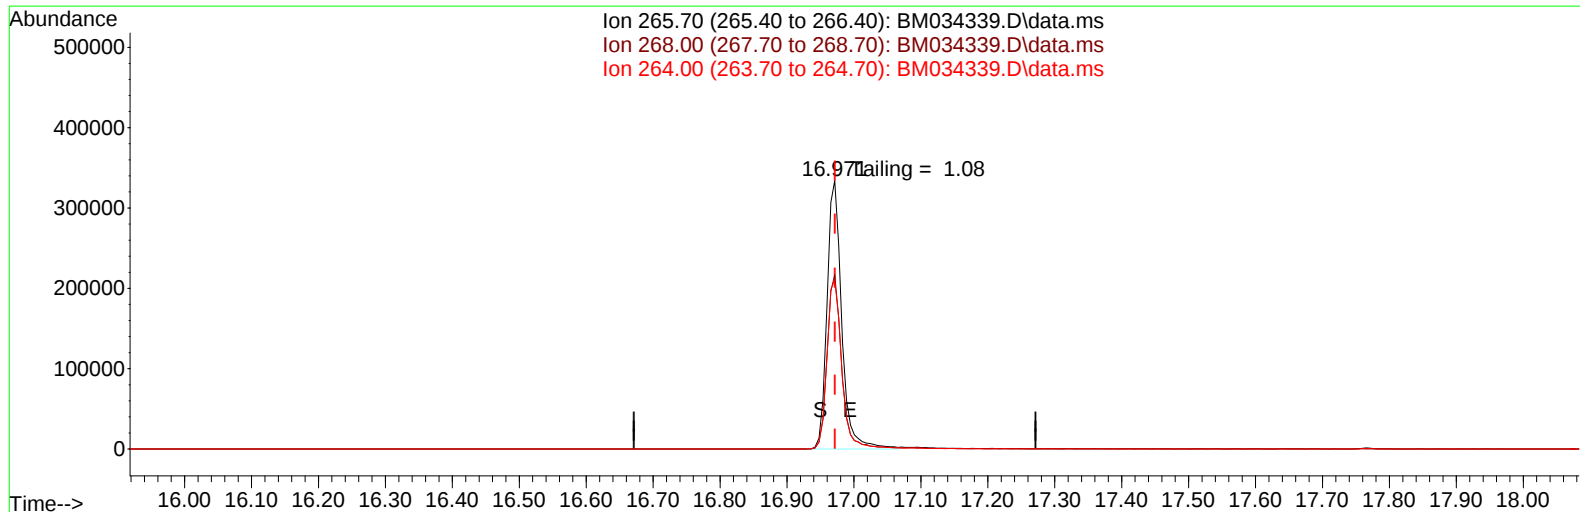

TIC: BM034339.D\data.ms

(70) Pentachlorophenol (C)

16.971min (0.000) 0.00 ng




response 513887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.94
264.00	62.90	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032322\
 Data File : BM034339.D
 Acq On : 23 Mar 2022 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 24 06:46:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 02:40:59 2022
 Response via : Initial Calibration

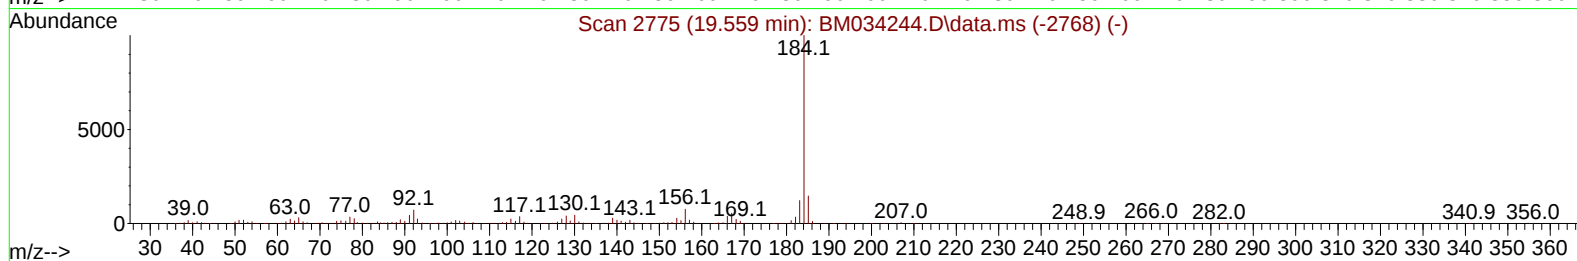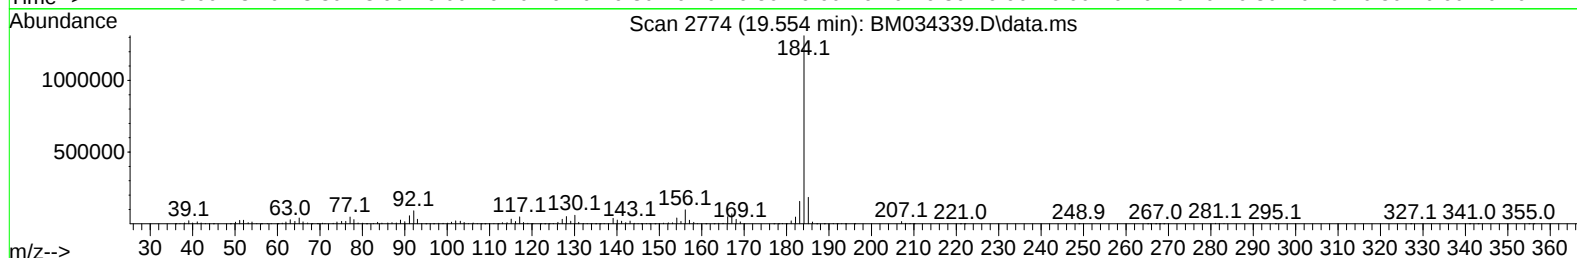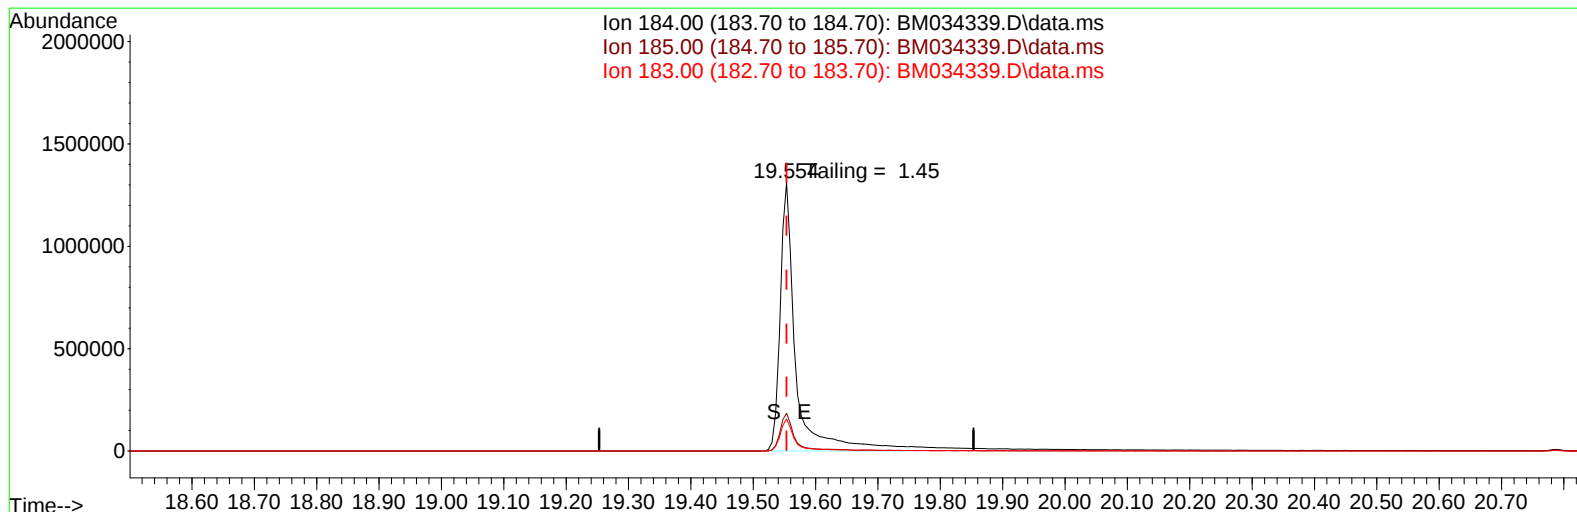

TIC: BM034339.D\data.ms

(77) Benzidine

19.554min (0.000) 1104186.34 ng

response 2378628

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.07
183.00	12.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2022	BNA_M	<u>BM034339.D</u>
Compound Name	Response	Retention Time
DDT	1639730	20.789
DDD	21167	20.348
DDE	2930	19.842
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24097	1663827	1.45

Instrument :
BNA_M
ClientSampleId :
DFTPP