

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032419\  
 Data File : BM019400.D  
 Acq On : 24 Mar 2019 20:01  
 Operator : JU/SJ  
 Sample : K2044-09  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :

Quant Time: Mar 25 03:04:16 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM032219MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Mar 25 02:03:45 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.60  | 152  | 120644   | 20.00 | ng/ul | -0.01    |
| 18) Naphthalene-d8        | 10.39 | 136  | 511632   | 20.00 | ng/ul | -0.01    |
| 36) Acenaphthene-d10      | 14.26 | 164  | 299883   | 20.00 | ng/ul | -0.01    |
| 62) Phenanthrene-d10      | 17.02 | 188  | 685741   | 20.00 | ng/ul | -0.01    |
| 78) Chrysene-d12          | 21.23 | 240  | 761232   | 20.00 | ng/ul | -0.01    |
| 86) Perylene-d12          | 23.44 | 264  | 846115   | 20.00 | ng/ul | -0.02    |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.15  | 96   | 20551    | 6.67  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.79  | 99   | 190219   | 17.71 | ng/ul | -0.01    |
| 7) Bis-(2-Chloroethyl)ether-d  | 6.96  | 67   | 127168   | 17.68 | ng/ul | -0.01    |
| 9) 2-Chlorophenol-d4           | 7.14  | 132  | 156812   | 19.26 | ng/ul | -0.01    |
| 13) 4-Methylphenol-d8          | 8.32  | 113  | 152287   | 18.88 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.78  | 128  | 68388    | 18.74 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.49  | 143  | 78532    | 19.33 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 10.02 | 165  | 132679   | 17.31 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 10.56 | 131  | 192753   | 20.94 | ng/ul | 0.00     |
| 44) Dimethylphthalate-d6       | 13.69 | 166  | 509177   | 21.04 | ng/ul | 0.00     |
| 47) Acenaphthylene-d8          | 13.96 | 160  | 569574   | 18.82 | ng/ul | -0.01    |
| 52) 4-Nitrophenol-d4           | 14.52 | 143  | 46992    | 12.39 | ng/ul | 0.00     |
| 58) Fluorene-d10               | 15.26 | 176  | 432087   | 20.73 | ng/ul | -0.01    |
| 63) 4,6-Dinitro-2-methylphenol | 15.41 | 200  | 59543    | 13.13 | ng/ul | 0.00     |
| 71) Anthracene-d10             | 17.12 | 188  | 683450   | 20.77 | ng/ul | -0.01    |
| 79) Pyrene-d10                 | 19.43 | 212  | 767041   | 21.81 | ng/ul | -0.01    |
| 90) Benzo(a)pyrene-d12         | 23.30 | 264  | 865701   | 19.30 | ng/ul | -0.02    |


| Target Compounds      | R.T.  | QIon | Response | Conc  | Units  | Ovalue |
|-----------------------|-------|------|----------|-------|--------|--------|
| 6) Phenol             | 6.82  | 94   | 14583    | 1.301 | ng/ul# | 83     |
| 45) Dimethylphthalate | 13.73 | 163  | 71656    | 2.952 | ng/ul  | 97     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032419\  
Data File : BM019400.D  
Acq On : 24 Mar 2019 20:01  
Operator : JU/SJ  
Sample : K2044-09  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Quant Time: Mar 25 03:04:16 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM032219MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Mar 25 02:03:45 2019  
Response via : Initial Calibration

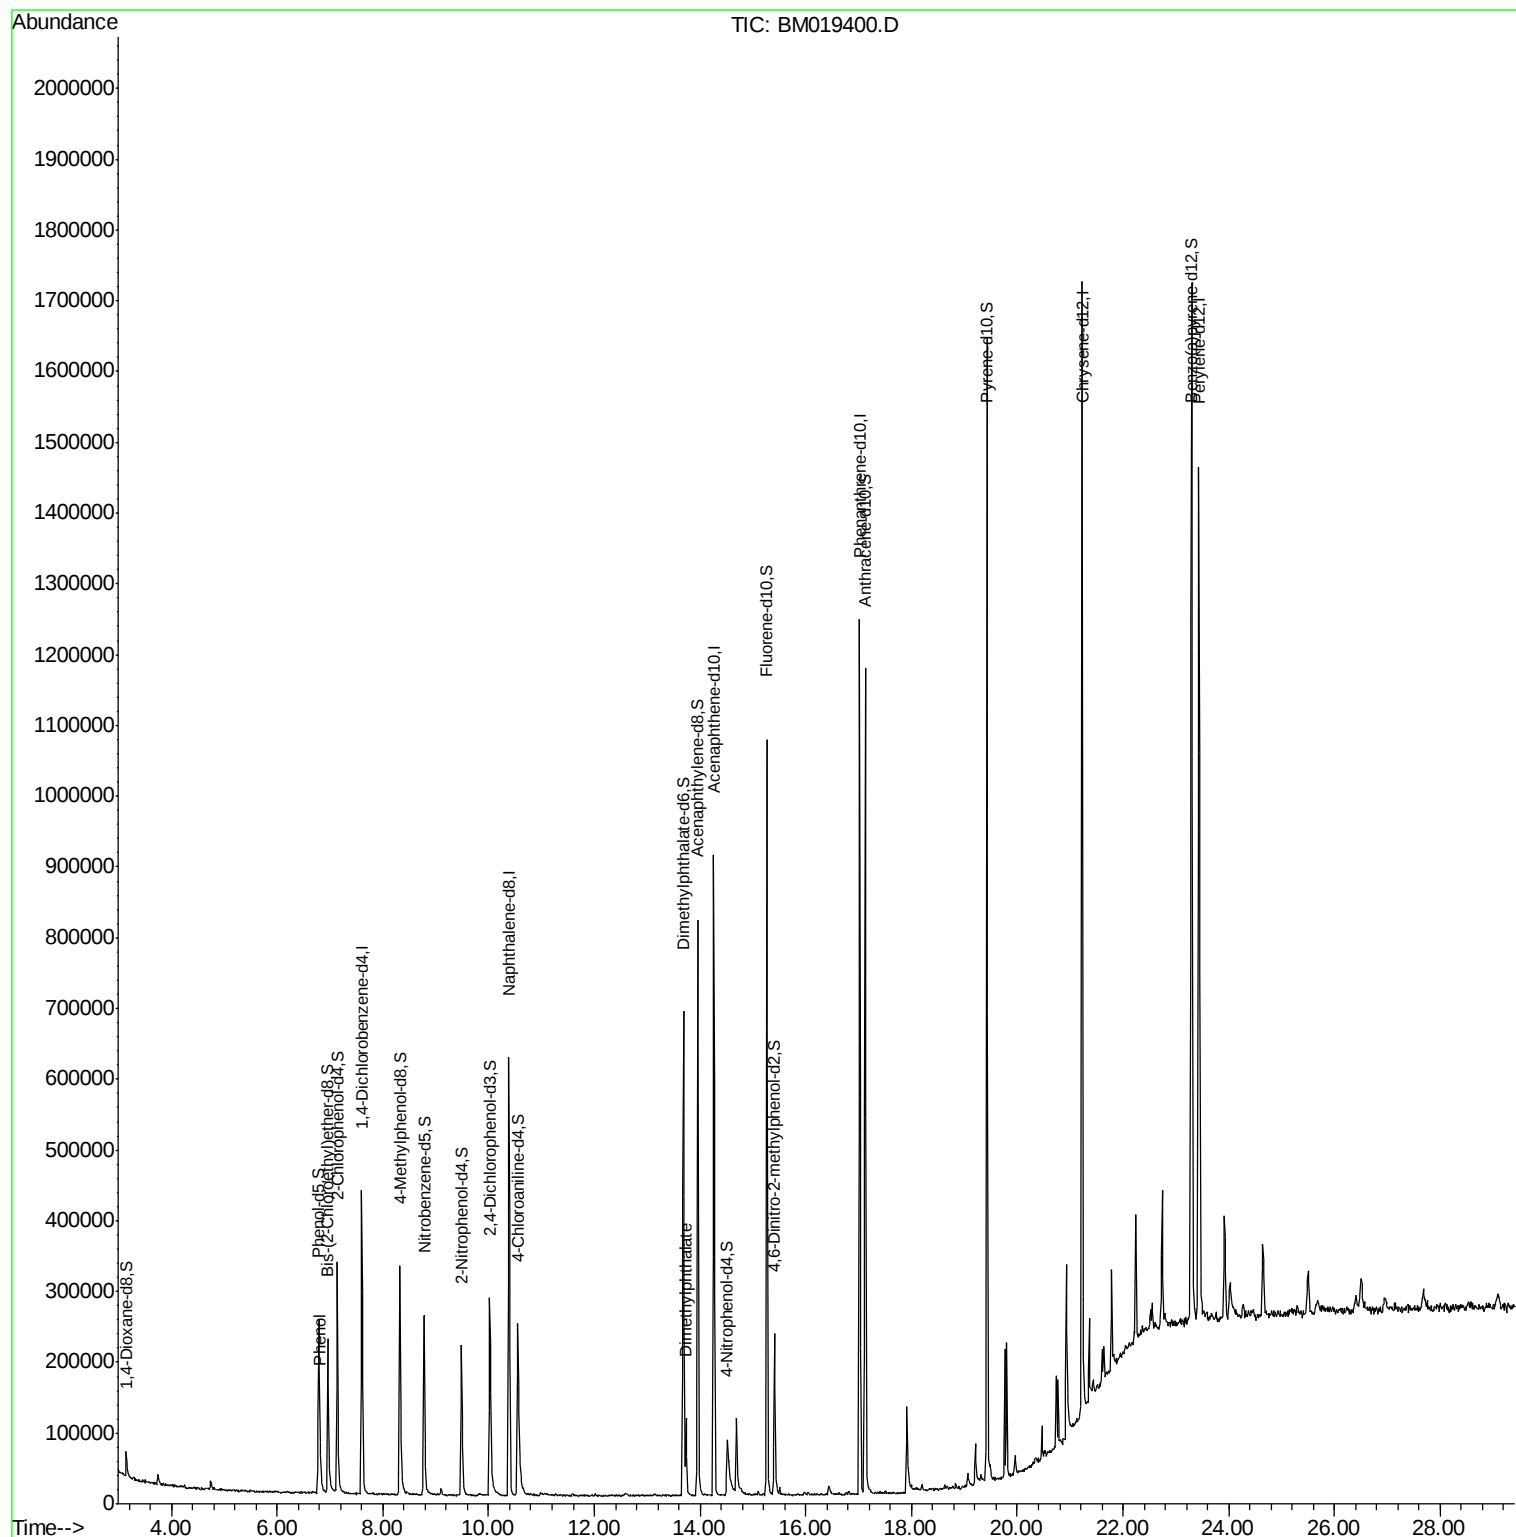

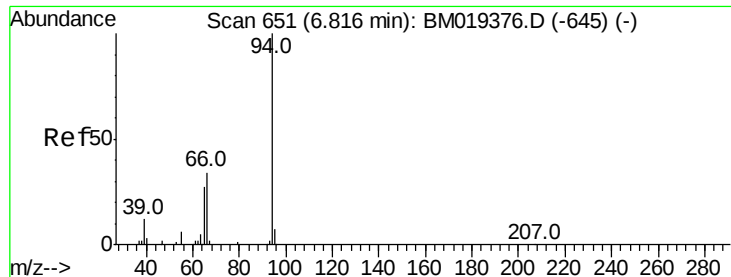





#6

Phenol

Concen: 1.301 ng/ul  
 RT: 6.82 min Scan# 651  
 Delta R.T. -0.01 min  
 Lab File: BM019400.D  
 Acq: 24 Mar 2019 20:01

Instrument :  
 BNA\_M  
 ClientSampleId :

Tot Ion: 94 Resp: 14583  
 Ion Ratio Lower Upper  
 94 100  
 65 28.7 23.0 34.6  
 66 56.2 30.4 45.6#

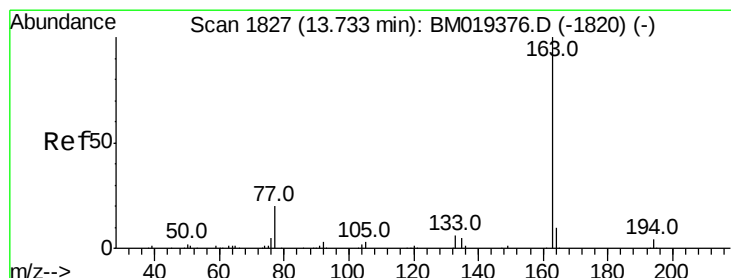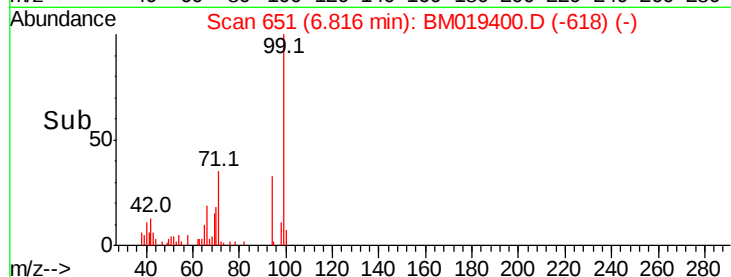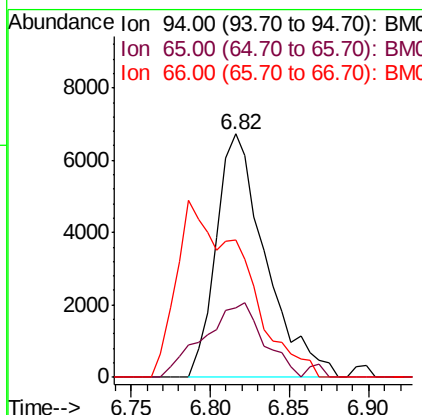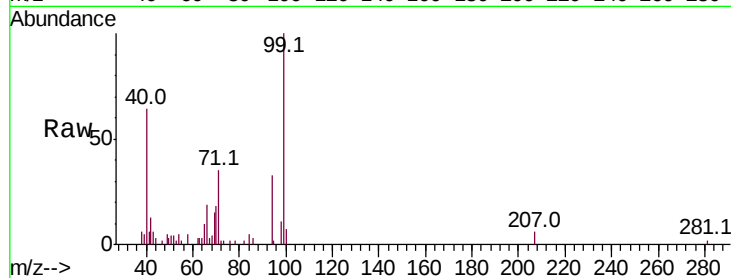

#45

Dimethylphthalate

Concen: 2.952 ng/ul  
 RT: 13.73 min Scan# 1827  
 Delta R.T. -0.01 min  
 Lab File: BM019400.D  
 Acq: 24 Mar 2019 20:01

Tgt Ion: 163 Resp: 71656  
 Ion Ratio Lower Upper  
 163 100  
 194 4.0 4.0 6.0  
 164 9.5 8.4 12.6

