


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032419\
Data File : BM019412.D
Acq On : 25 Mar 2019 03:13
Operator : JU/SJ
Sample : K2044-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5W4

Manual Integrations
APPROVED

Sohil
3/26/2019 6:29:31 PM

Quant Time: Mar 25 05:19:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

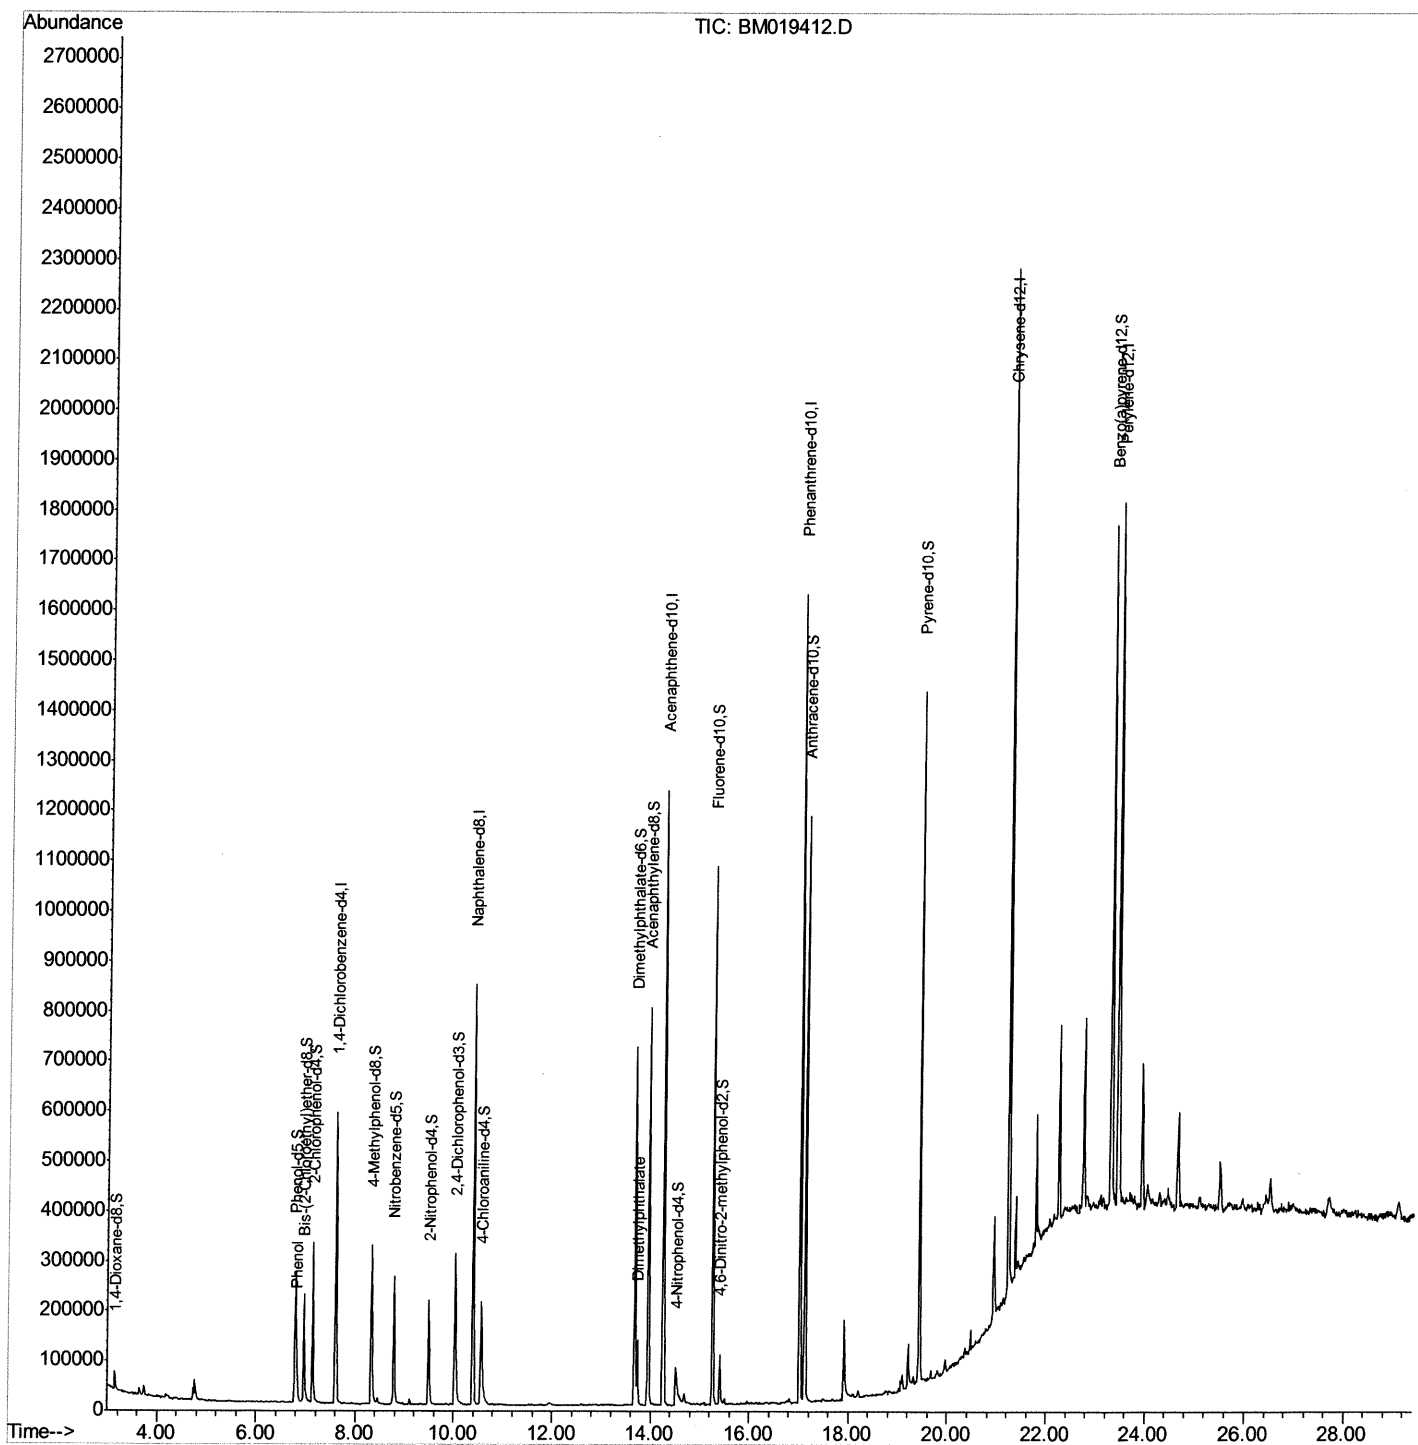

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032419\
 Data File : BM019412.D
 Acq On : 25 Mar 2019 03:13
 Operator : JU/SJ
 Sample : K2044-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5W4

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:29:31 PM

Quant Time: Mar 25 05:17:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

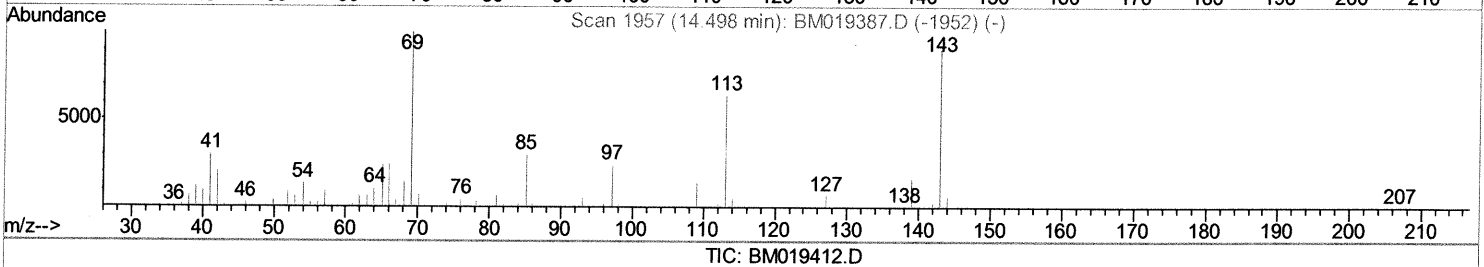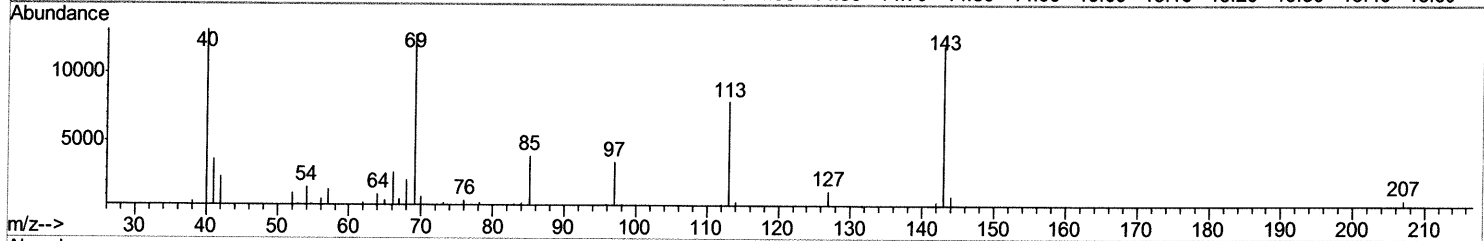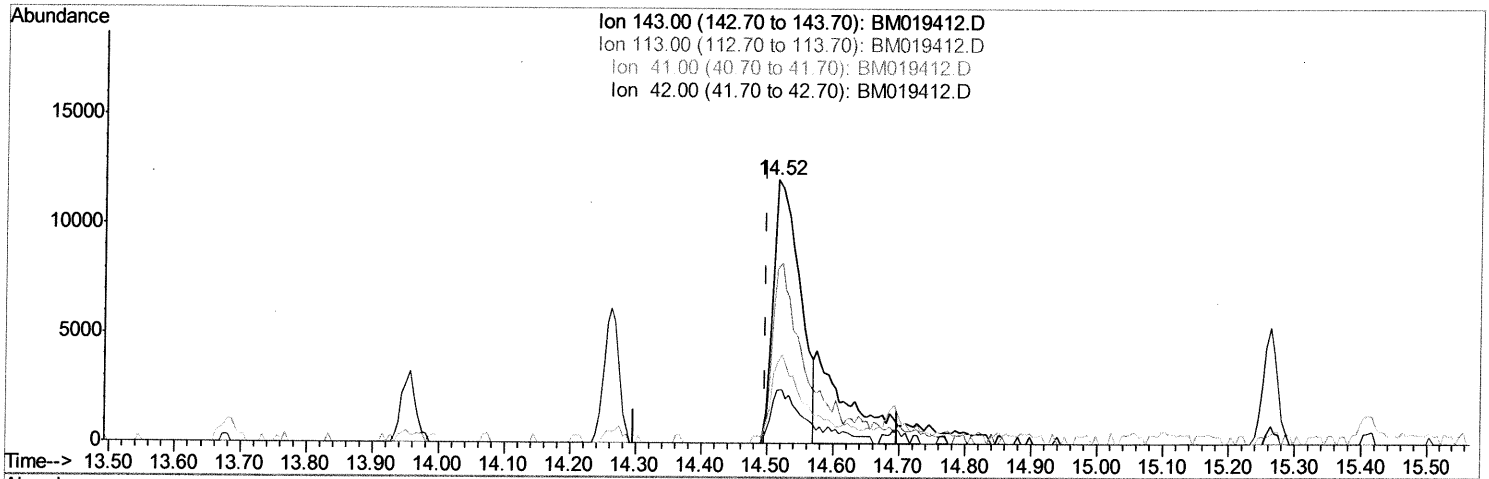

TIC: BM019412.D

(52) 4-Nitrophenol-d4 (S)

14.515min (+0.018) 6.83ng/ul

response 33866

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	66.02
41.00	32.60	30.06
42.00	22.30	20.18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032419\
Data File : BM019412.D
Acq On : 25 Mar 2019 03:13
Operator : JU/SJ
Sample : K2044-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5W4

Manual Integrations
APPROVED

Sohil
3/26/2019 6:29:31 PM

Quant Time: Mar 25 05:17:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

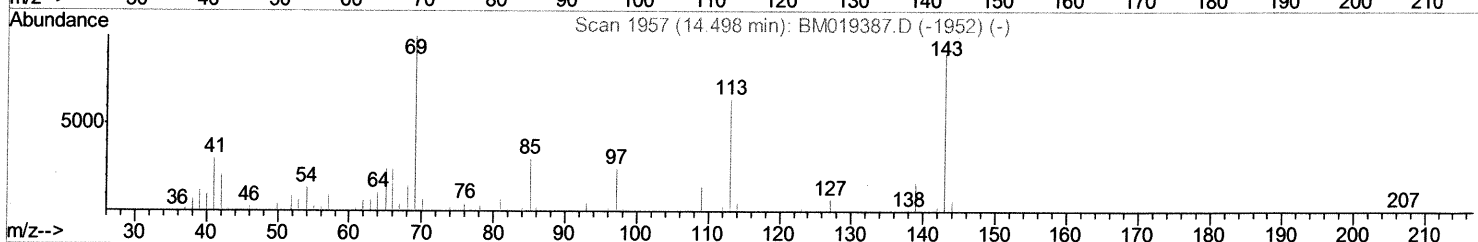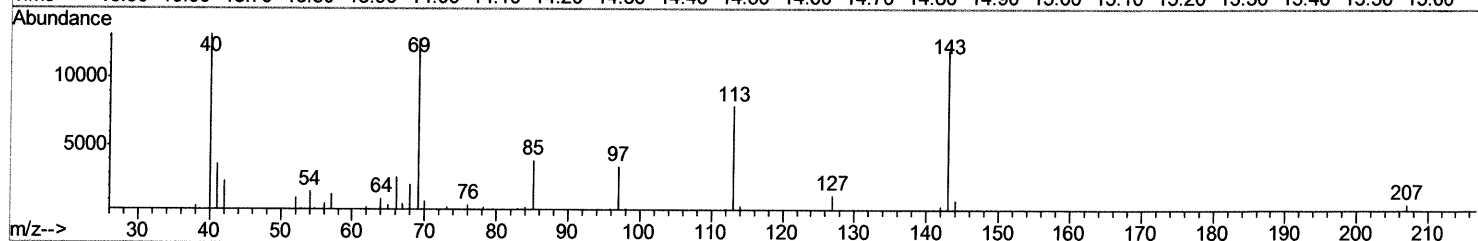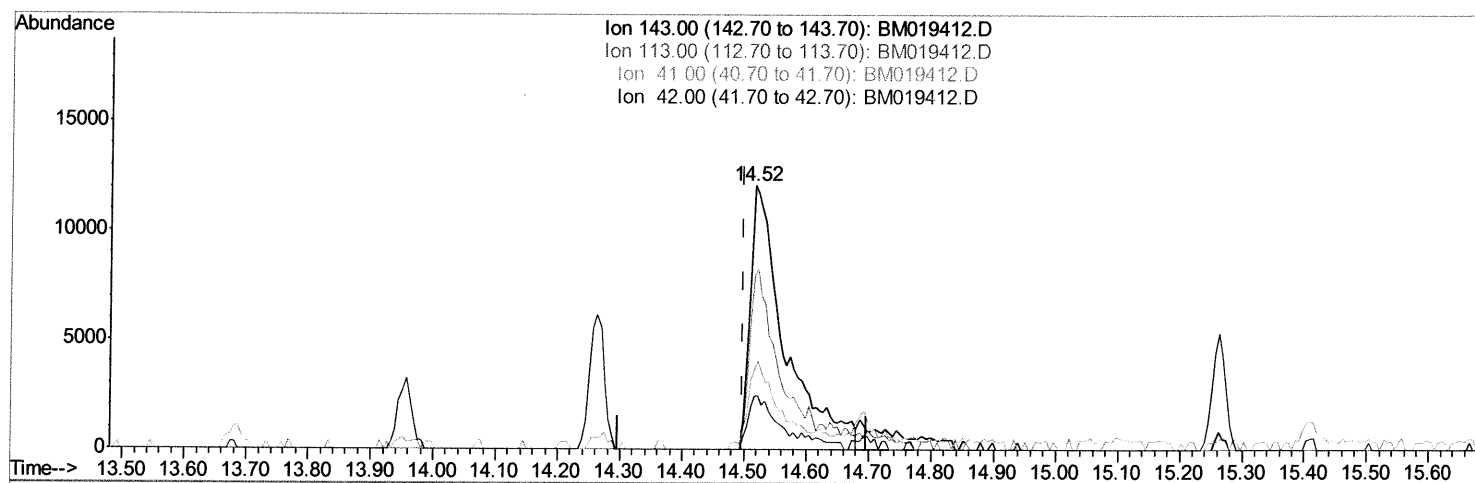

TIC: BM019412.D

(52) 4-Nitrophenol-d4 (S)

14.515min (+0.018) 9.61ng/ul m> SJ 4/1/19

response 47594

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	66.02
41.00	32.60	30.06
42.00	22.30	20.18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032419\
 Data File : BM019412.D
 Acq On : 25 Mar 2019 03:13
 Operator : JU/SJ
 Sample : K2044-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5W4

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:29:31 PM

Quant Time: Mar 25 05:19:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	165079	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	693764	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	391760	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	867062	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	892612	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	969228	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	19185	4.55	ng/uL	0.00
5) Phenol-d5	6.79	99	188607	12.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	120892	12.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	154934	13.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	146233	13.25	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	70005	14.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	77732	14.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	137054	13.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	161085	12.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	488738	15.46	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	577967	14.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	47594m	9.61	ng/ul	0.02
58) Fluorene-d10	15.26	176	424062	15.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	25410	4.43	ng/ul	0.00
71) Anthracene-d10	17.12	188	647176	15.55	ng/ul	0.00
79) Pyrene-d10	19.43	212	676777	16.41	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	714868	13.91	ng/ul	0.00

SD 4/1/19

Target Compounds

					Qvalue
6) Phenol	6.82	94	40698	2.653 ng/ul	99
45) Dimethylphthalate	13.73	163	88940	2.804 ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed