

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032419\
 Data File : BM019417.D
 Acq On : 25 Mar 2019 06:12
 Operator : JU/SJ
 Sample : K2025-13DL 20X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0966DL

Quant Time: Mar 25 07:43:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	145565	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	626319	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	356892	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	769908	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	786442	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	863070	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	366	0.10	ng/uL	0.02
5) Phenol-d5	6.80	99	1340	0.10	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.97	67	7535	0.87	ng/ul	0.02
9) 2-Chlorophenol-d4	7.15	132	9489	0.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	3533	0.36	ng/ul	0.04
19) Nitrobenzene-d5	8.77	128	5592	1.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	4742	0.95	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.03	165	8515	0.91	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.70	166	38701	1.34	ng/ul	0.01
47) Acenaphthylene-d8	13.96	160	46275	1.29	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.27	176	37245	1.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.13	188	59843	1.62	ng/ul	0.00
79) Pyrene-d10	19.43	212	62994	1.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	66467	1.45	ng/ul	0.00


Target Compounds				Ovalue	
20) Nitrobenzene	8.82	77	462669	34.788	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032419\
Data File : BM019417.D
Acq On : 25 Mar 2019 06:12
Operator : JU/SJ
Sample : K2025-13DL 20X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0966DL

Quant Time: Mar 25 07:43:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

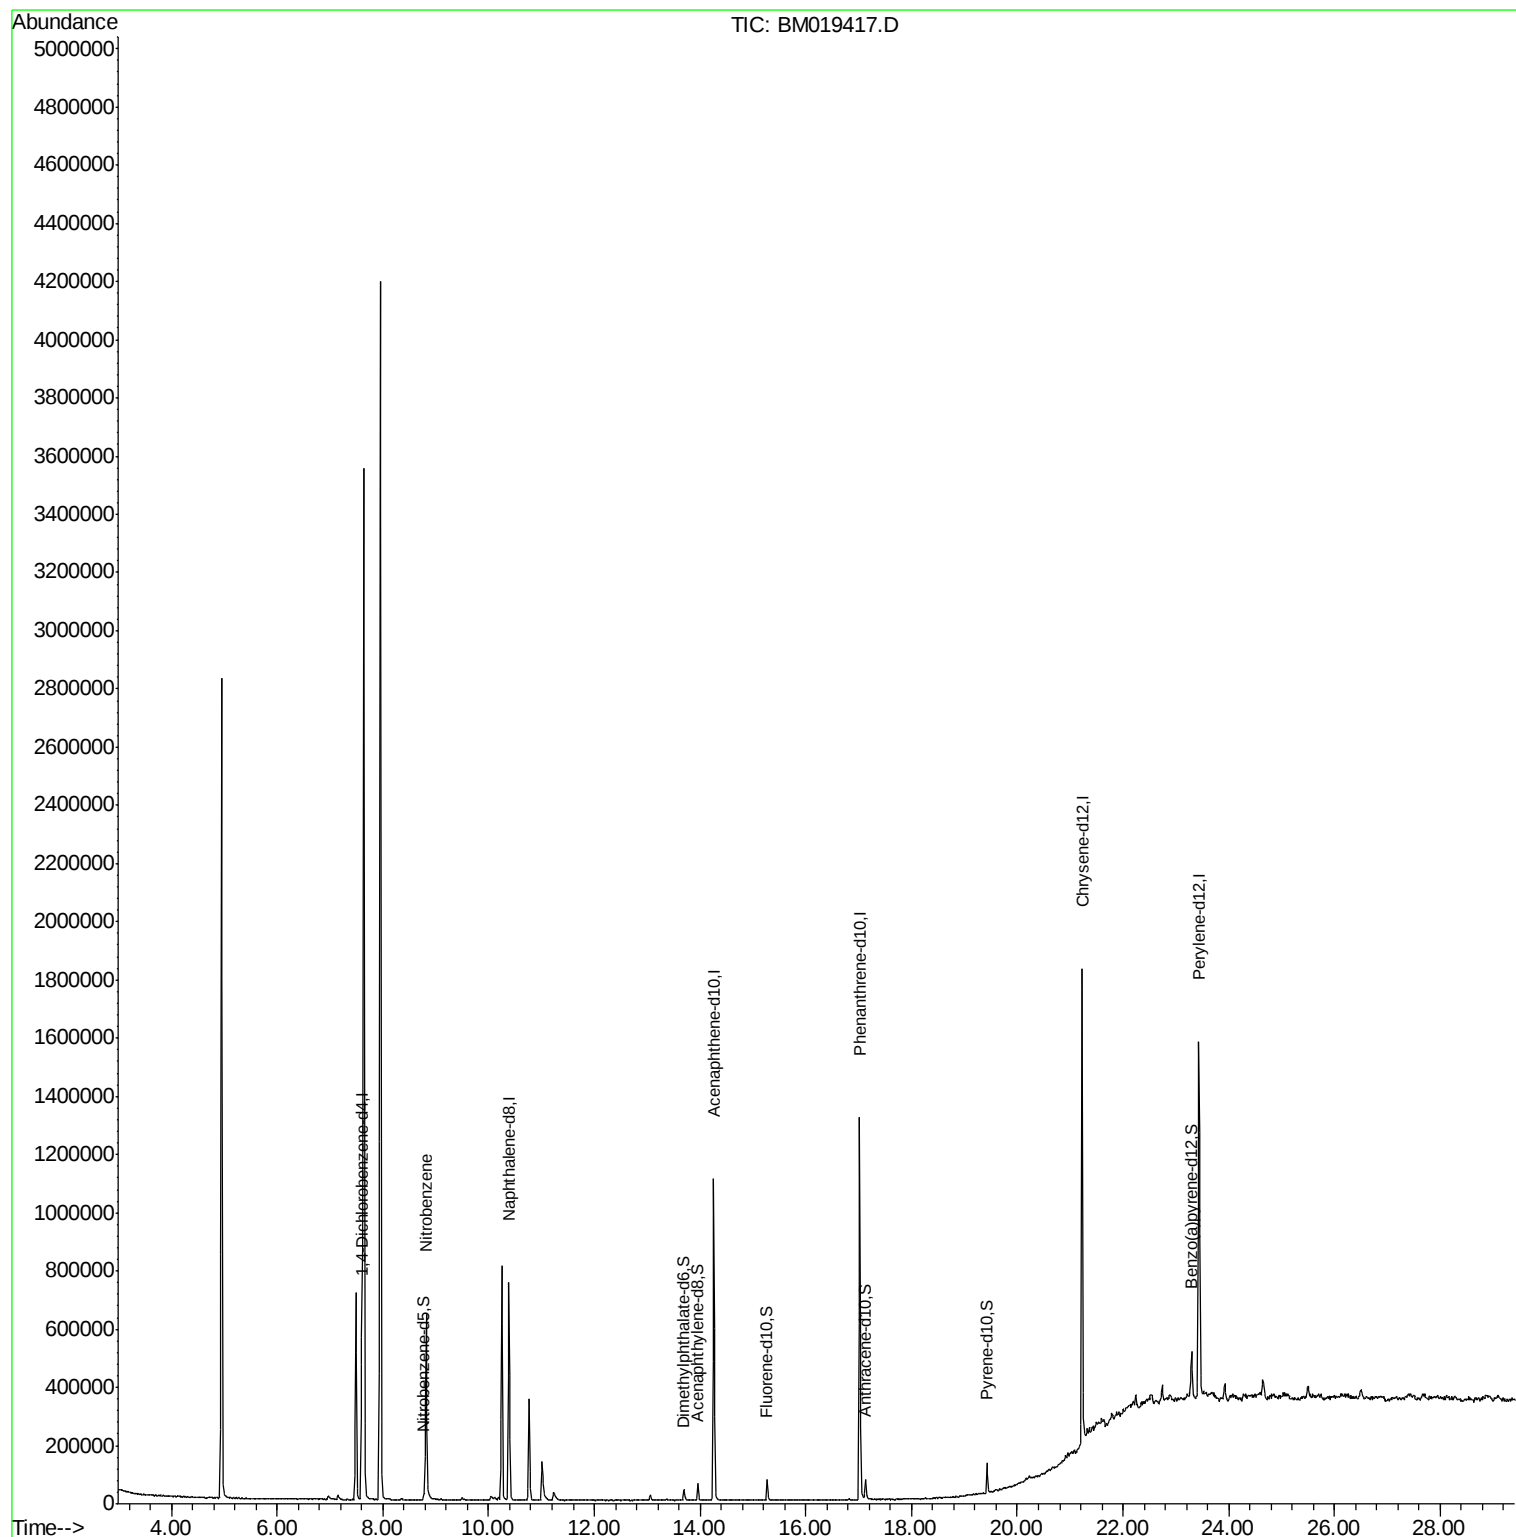

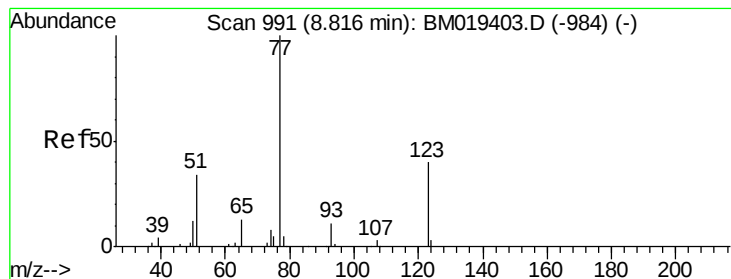

#20
 Nitrobenzene
 Concen: 34.788 ng/ul
 RT: 8.82 min Scan# 991
 Delta R.T. 0.00 min
 Lab File: BM019417.D
 Acq: 25 Mar 2019 06:12

Instrument :
 BNA_M
 ClientSampleId :
 C0966DL

Tot Ion	Ion	Ratio	Lower	Upper
77	100			
123	41.2	31.8	47.8	
65	12.1	10.6	16.0	

