
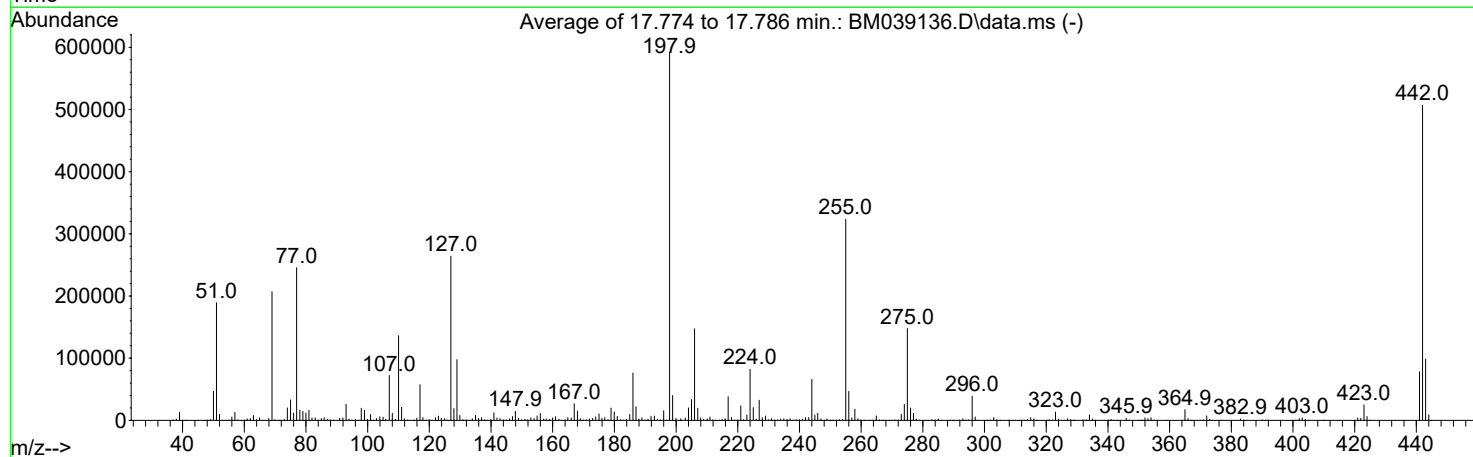


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032423\
 Data File : BM039136.D
 Acq On : 24 Mar 2023 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 24 15:04:20 2023

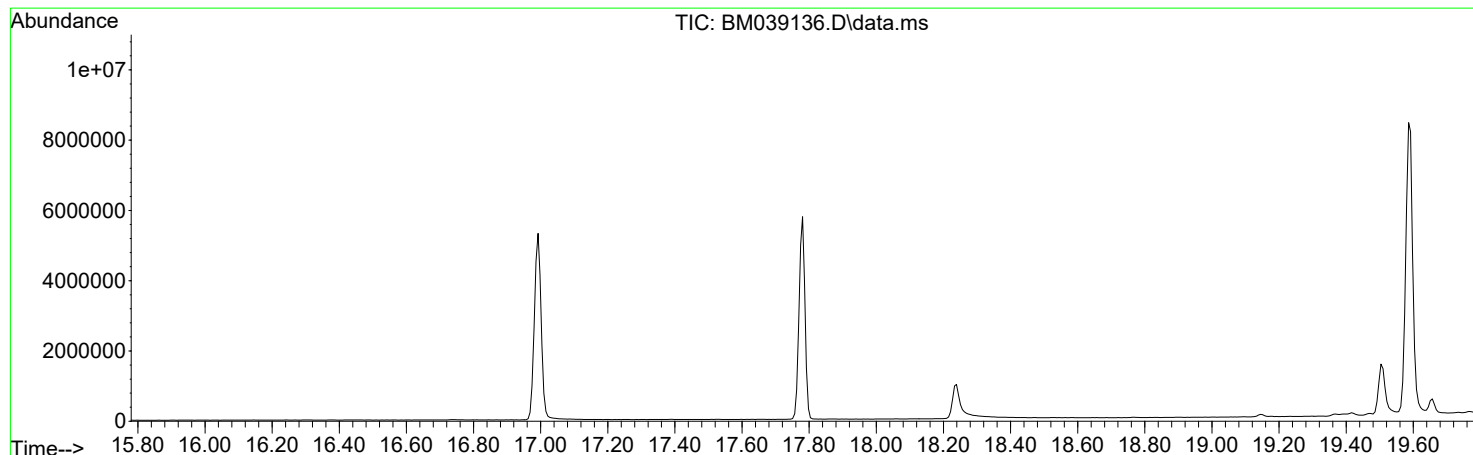

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	189152	PASS
68	69	0.00	2	1.4	2837	PASS
69	198	0.00	100	35.0	207188	PASS
70	69	0.00	2	0.5	1137	PASS
127	198	10	80	44.6	264171	PASS
197	198	0.00	2	0.1	590	PASS
198	198	100	100	100.0	591701	PASS
199	198	5	9	6.7	39875	PASS
275	198	10	60	25.0	147861	PASS
365	198	1	100	2.9	17231	PASS
441	198	0.01	100	13.2	77947	PASS
442	442	50	100	100.0	507051	PASS
443	442	15	24	19.5	98683	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/24/2023	BNA_M	<u>BM039136.D</u>
Compound Name	Response	Retention Time
DDT	2477846	20.815
DDD	55756	20.374
DDE	1556	19.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57312	2535158	2.26

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032423\
Data File : BM039136.D
Acq On : 24 Mar 2023 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 03:59:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 15:04:20 2023
Response via : Initial Calibration

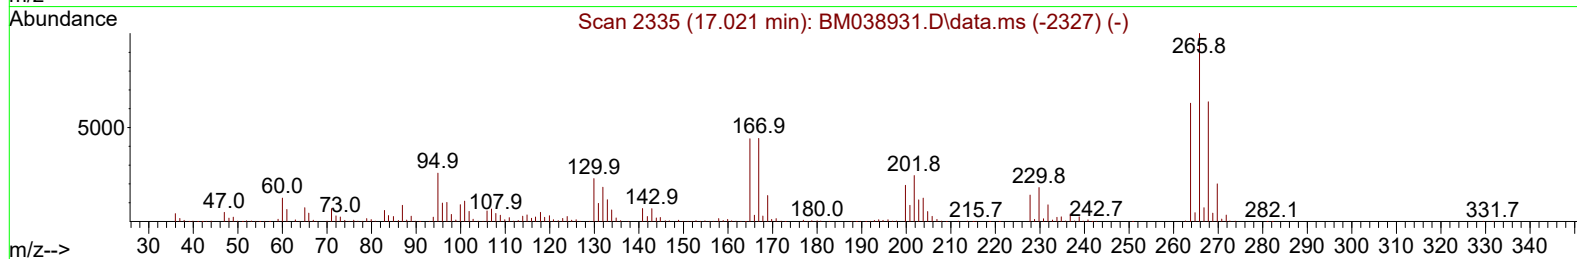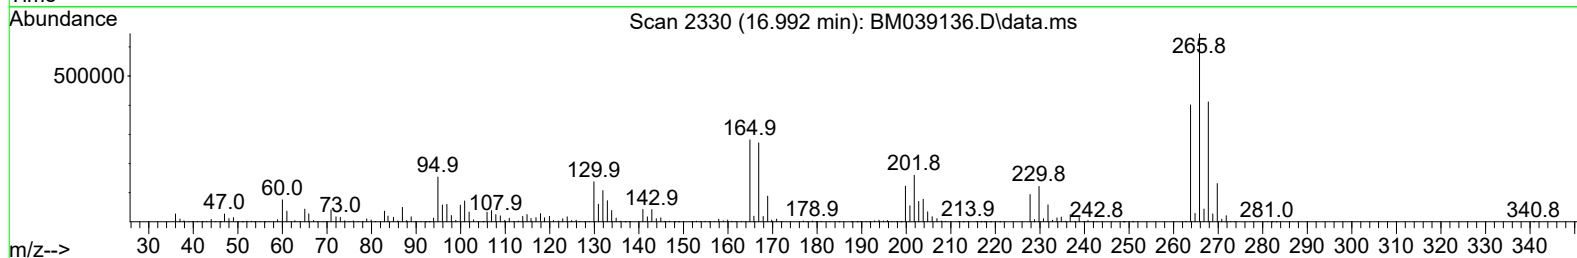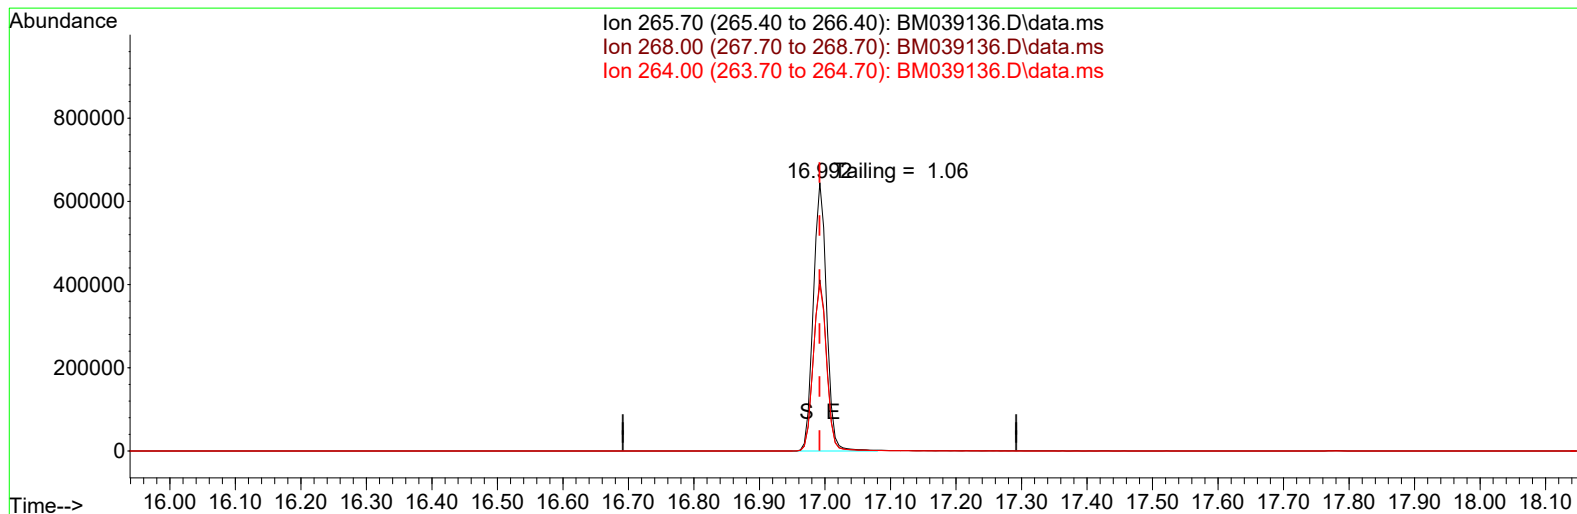

TIC: BM039136.D\data.ms

(70) Pentachlorophenol (C)

16.992min (+ 0.000) 66287.86 ng




response 913649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.75
264.00	62.90	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032423\
Data File : BM039136.D
Acq On : 24 Mar 2023 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 03:59:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 15:04:20 2023
Response via : Initial Calibration

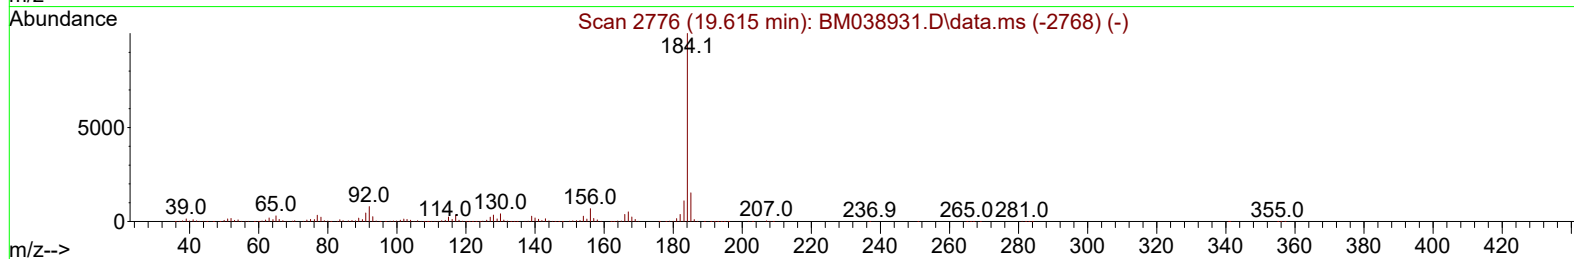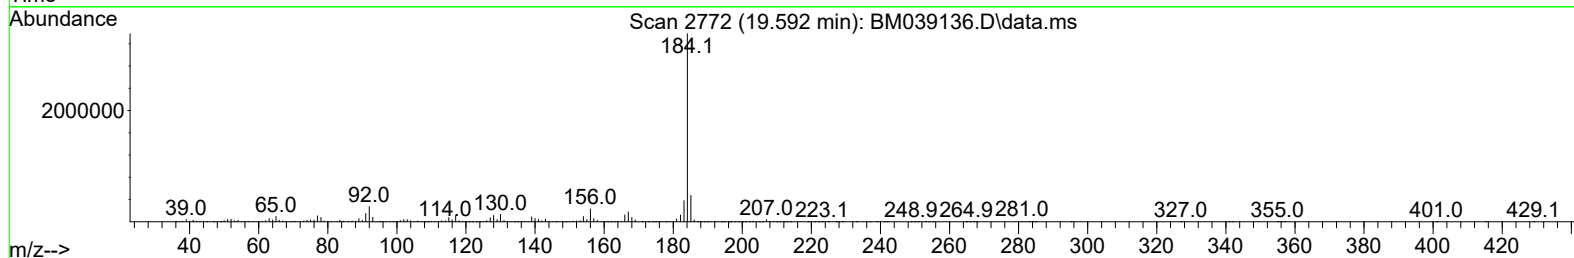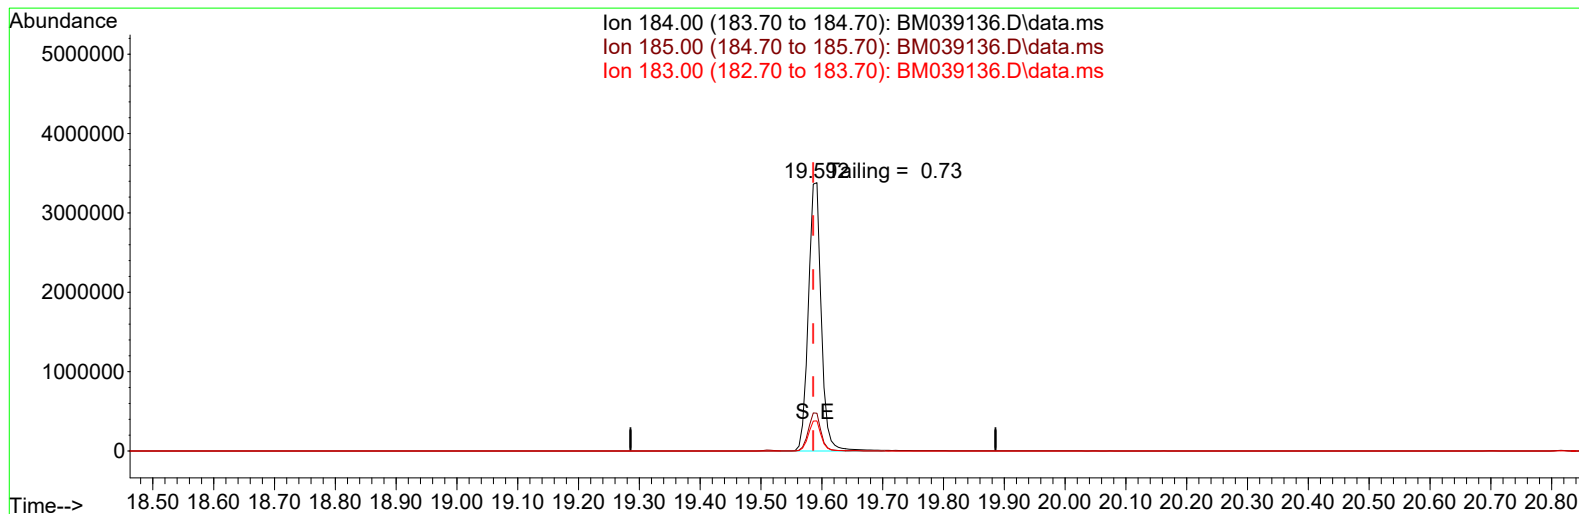

TIC: BM039136.D\data.ms

(77) Benzidine

19.592min (+ 0.006) 35955.21 ng

response 5032193

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.09
183.00	11.00	11.22
0.00	0.00	0.00