

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
 Data File : BM019423.D
 Acq On : 25 Mar 2019 10:09
 Operator : JU/SJ
 Sample : K2027-09DL 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0988DL

Quant Time: Mar 26 05:39:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	138382	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	564862	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	313748	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	700146	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	707221	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	786424	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	263	0.07	ng/uL	-0.05
5) Phenol-d5	6.80	99	6341	0.51	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.96	67	21046	2.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	22570	2.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	11470	1.24	ng/ul	0.02
19) Nitrobenzene-d5	8.77	128	12584	3.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	12410	2.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	20064	2.37	ng/ul	0.02
29) 4-Chloroaniline-d4	10.39	131	601	0.06	ng/ul	-0.16
44) Dimethylphthalate-d6	13.69	166	80689	3.19	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	97476	3.08	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.26	176	75835	3.48	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	4102	0.89	ng/ul	0.02
71) Anthracene-d10	17.12	188	110164	3.28	ng/ul	0.00
79) Pyrene-d10	19.43	212	123796	3.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	140443	3.37	ng/ul	0.00

Target Compounds


					Qvalue	
11) 2-Methylphenol	7.97	108	137383	15.319	ng/ul	92
20) Nitrobenzene	8.82	77	381046	31.768	ng/ul	100
32) Caprolactam	11.23	113	5436	2.190	ng/ul#	1
37) 1,2,4,5-Tetrachlorobenzene	12.43	216	45443	4.552	ng/ul#	95
73) 1,2,3,4-Tetrachlorobenzene	13.05	216	151038	14.879	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
Data File : BM019423.D
Acq On : 25 Mar 2019 10:09
Operator : JU/SJ
Sample : K2027-09DL 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0988DL

Quant Time: Mar 26 05:39:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

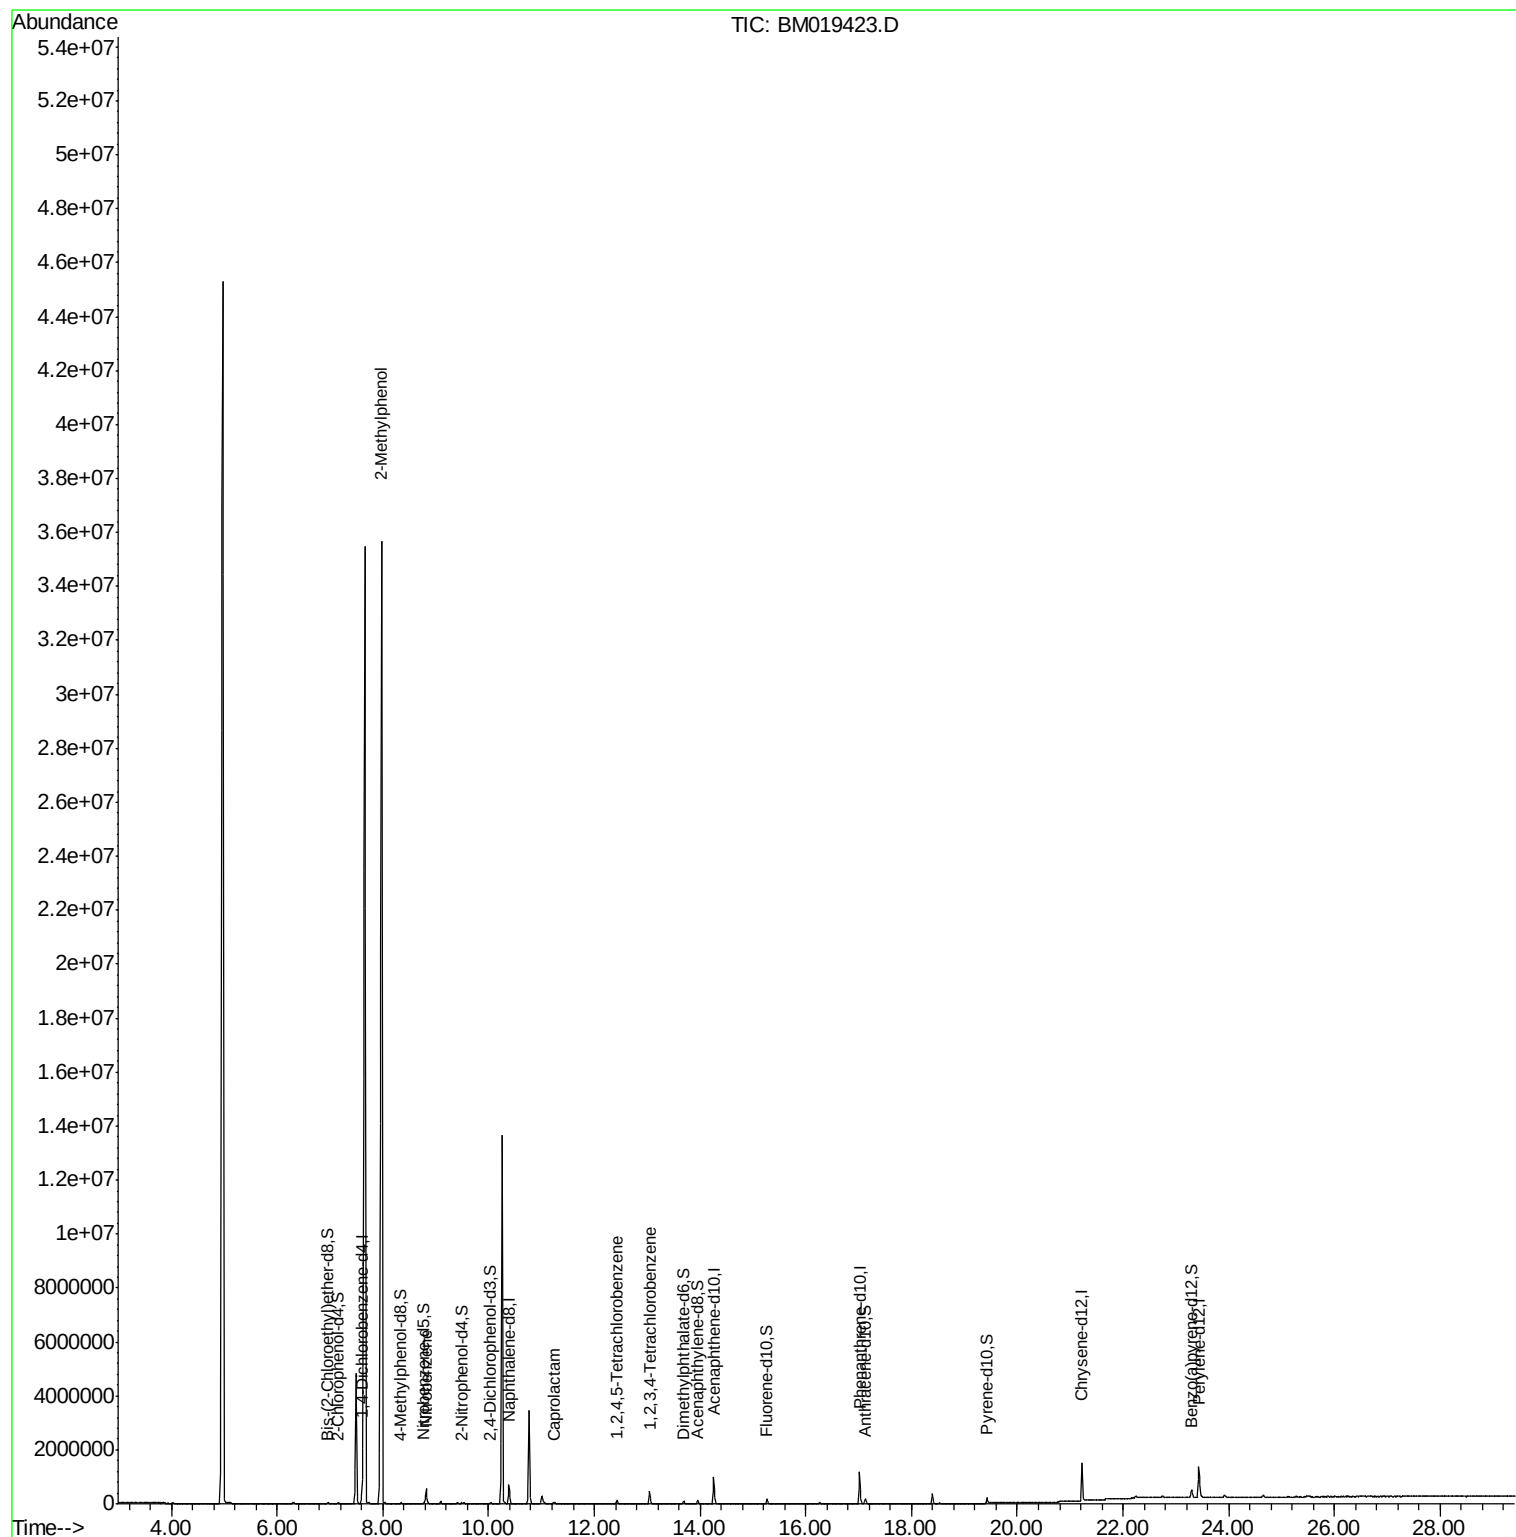


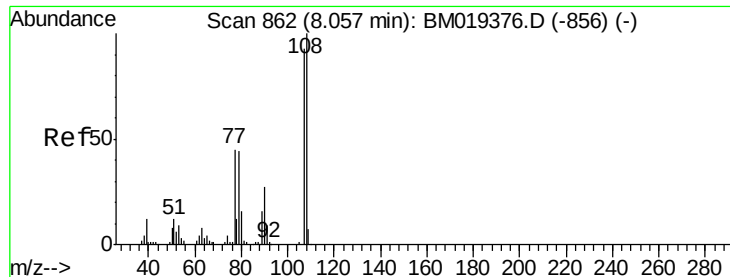




#11
2-Methylphenol
Concen: 15.319 ng/ul
RT: 7.97 min Scan# 848
Delta R.T. -0.08 min
Lab File: BM019423.D
Acq: 25 Mar 2019 10:09

Instrument :
BNA_M
ClientSampleID :
C0988DL

Tgt Ion: 108 Resp: 137383
Ion Ratio Lower Upper
108 100
107 85.1 74.1 111.1

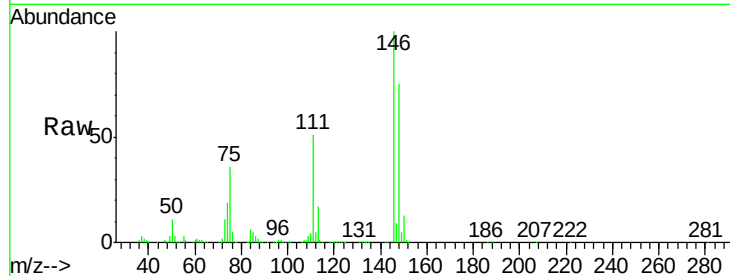


Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E

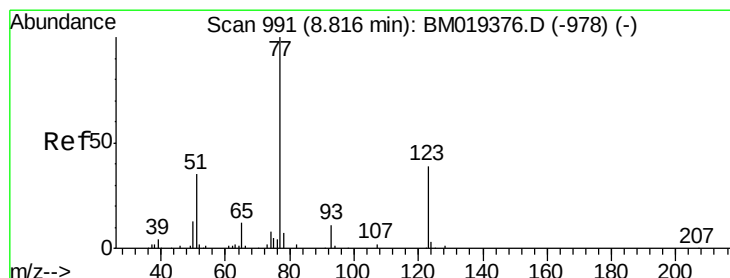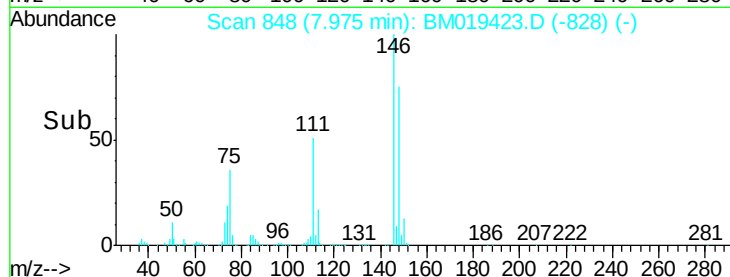
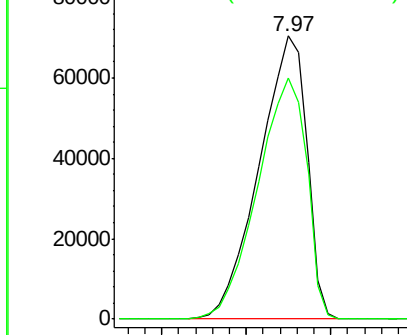



#20
Nitrobenzene
Concen: 31.768 ng/ul
RT: 8.82 min Scan# 991
Delta R.T. -0.00 min
Lab File: BM019423.D
Acq: 25 Mar 2019 10:09

Tgt Ion: 77 Resp: 381046
Ion Ratio Lower Upper
77 100
123 39.6 31.8 47.8
65 13.0 10.6 16.0

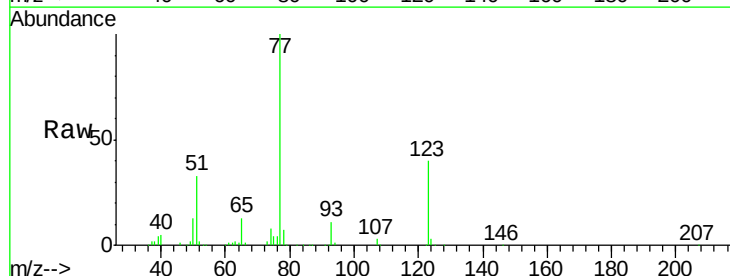

Abundance Ion 77.00 (76.70 to 77.70): BM0
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BM0



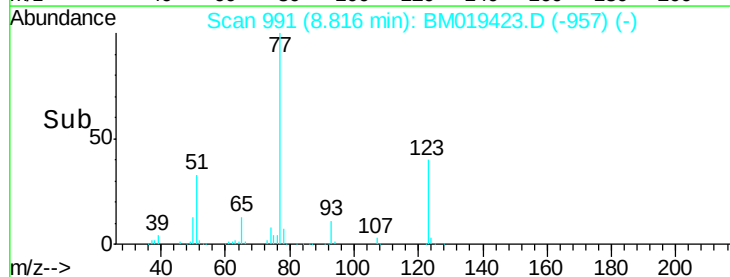
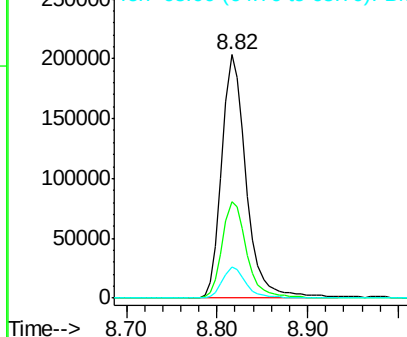


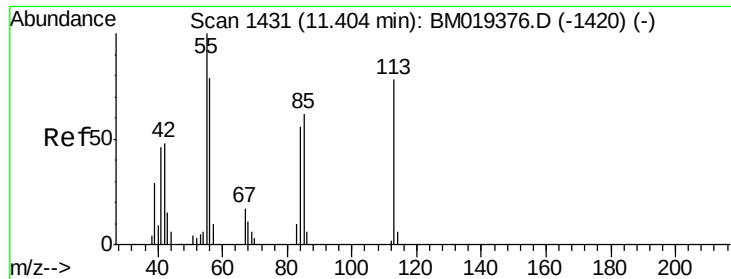

#32
 Caprolactam
 Concen: 2.190 ng/ul
 RT: 11.23 min Scan# 1401
 Delta R.T. -0.16 min
 Lab File: BM019423.D
 Acq: 25 Mar 2019 10:09




Instrument :
 BNA_M
 ClientSampleId :
 C0988DL


Tgt Ion:113 Resp: 5436
 Ion Ratio Lower Upper
 113 100
 55 0.0 131.7 197.5#
 56 0.0 92.7 139.1#

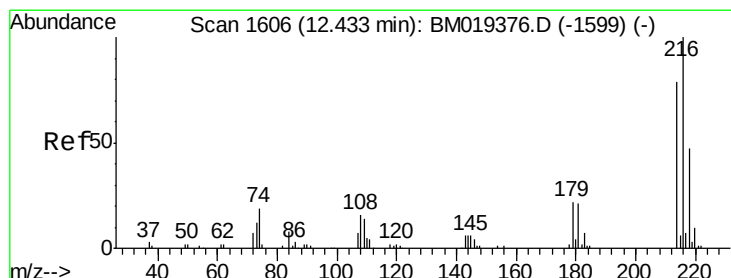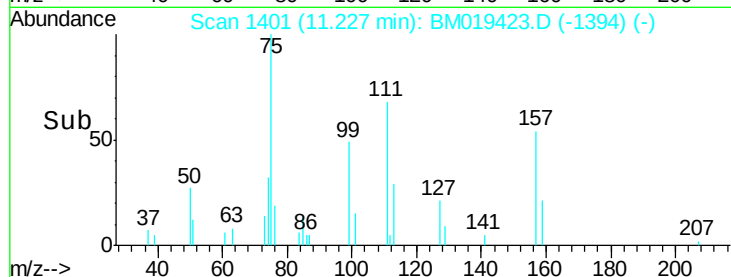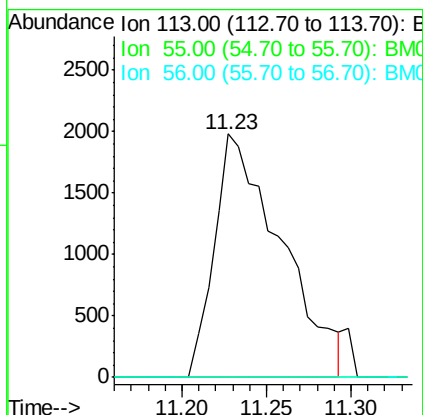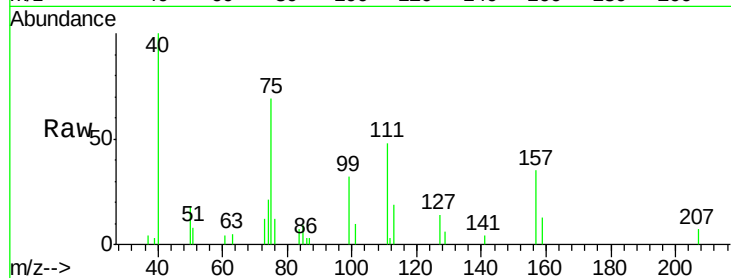

#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 4.552 ng/ul
 RT: 12.43 min Scan# 1606
 Delta R.T. -0.00 min
 Lab File: BM019423.D
 Acq: 25 Mar 2019 10:09

Tgt Ion:216 Resp: 45443
 Ion Ratio Lower Upper
 216 100
 214 82.8 64.1 96.1
 179 22.6 14.5 21.7#
 108 18.2 10.4 15.6#

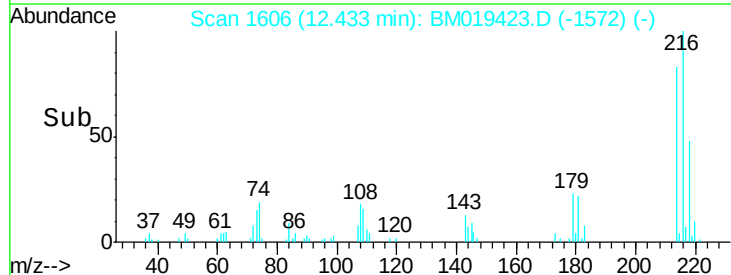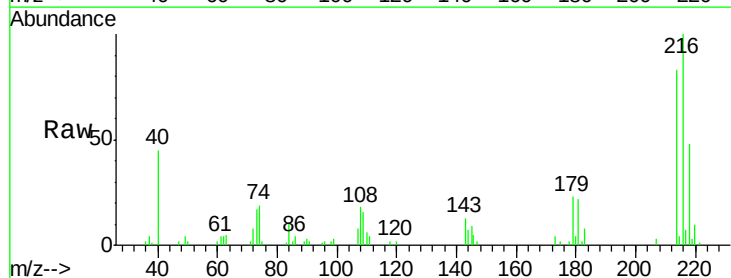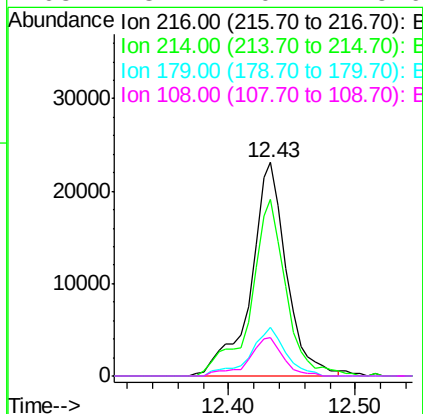

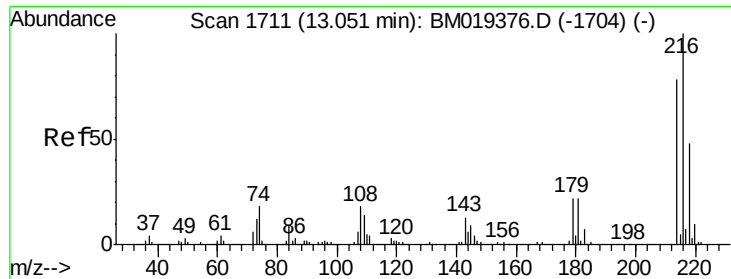

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 14.879 ng/uL
 RT: 13.05 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BM019423.D
 Acq: 25 Mar 2019 10:09

Instrument :
 BNA_M
 ClientSampleId :
 C0988DL

Tgt Ion	Ratio	Lower	Upper
216	100		
214	79.7	64.1	96.1
218	46.6	39.4	59.0

