

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
 Data File : BM019426.D
 Acq On : 25 Mar 2019 11:57
 Operator : JU/SJ
 Sample : PB118219BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK19

Quant Time: Mar 26 05:39:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	125252	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	546837	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	316316	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	700902	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	696954	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	775212	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	20641	6.45	ng/uL	0.00
5) Phenol-d5	6.79	99	378600	33.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	238274	31.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	300585	35.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	311425	37.20	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	142416	36.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	163985	37.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	293856	35.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	418199	42.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	1021979	40.04	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1264208	39.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	128970	32.24	ng/ul	0.00
58) Fluorene-d10	15.26	176	880660	40.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	123882	26.73	ng/ul	0.00
71) Anthracene-d10	17.12	188	1405999	41.80	ng/ul	0.00
79) Pyrene-d10	19.43	212	1497979	46.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1628326	39.62	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.32	70	7693	1.007	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
Data File : BM019426.D
Acq On : 25 Mar 2019 11:57
Operator : JU/SJ
Sample : PB118219BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK19

Quant Time: Mar 26 05:39:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

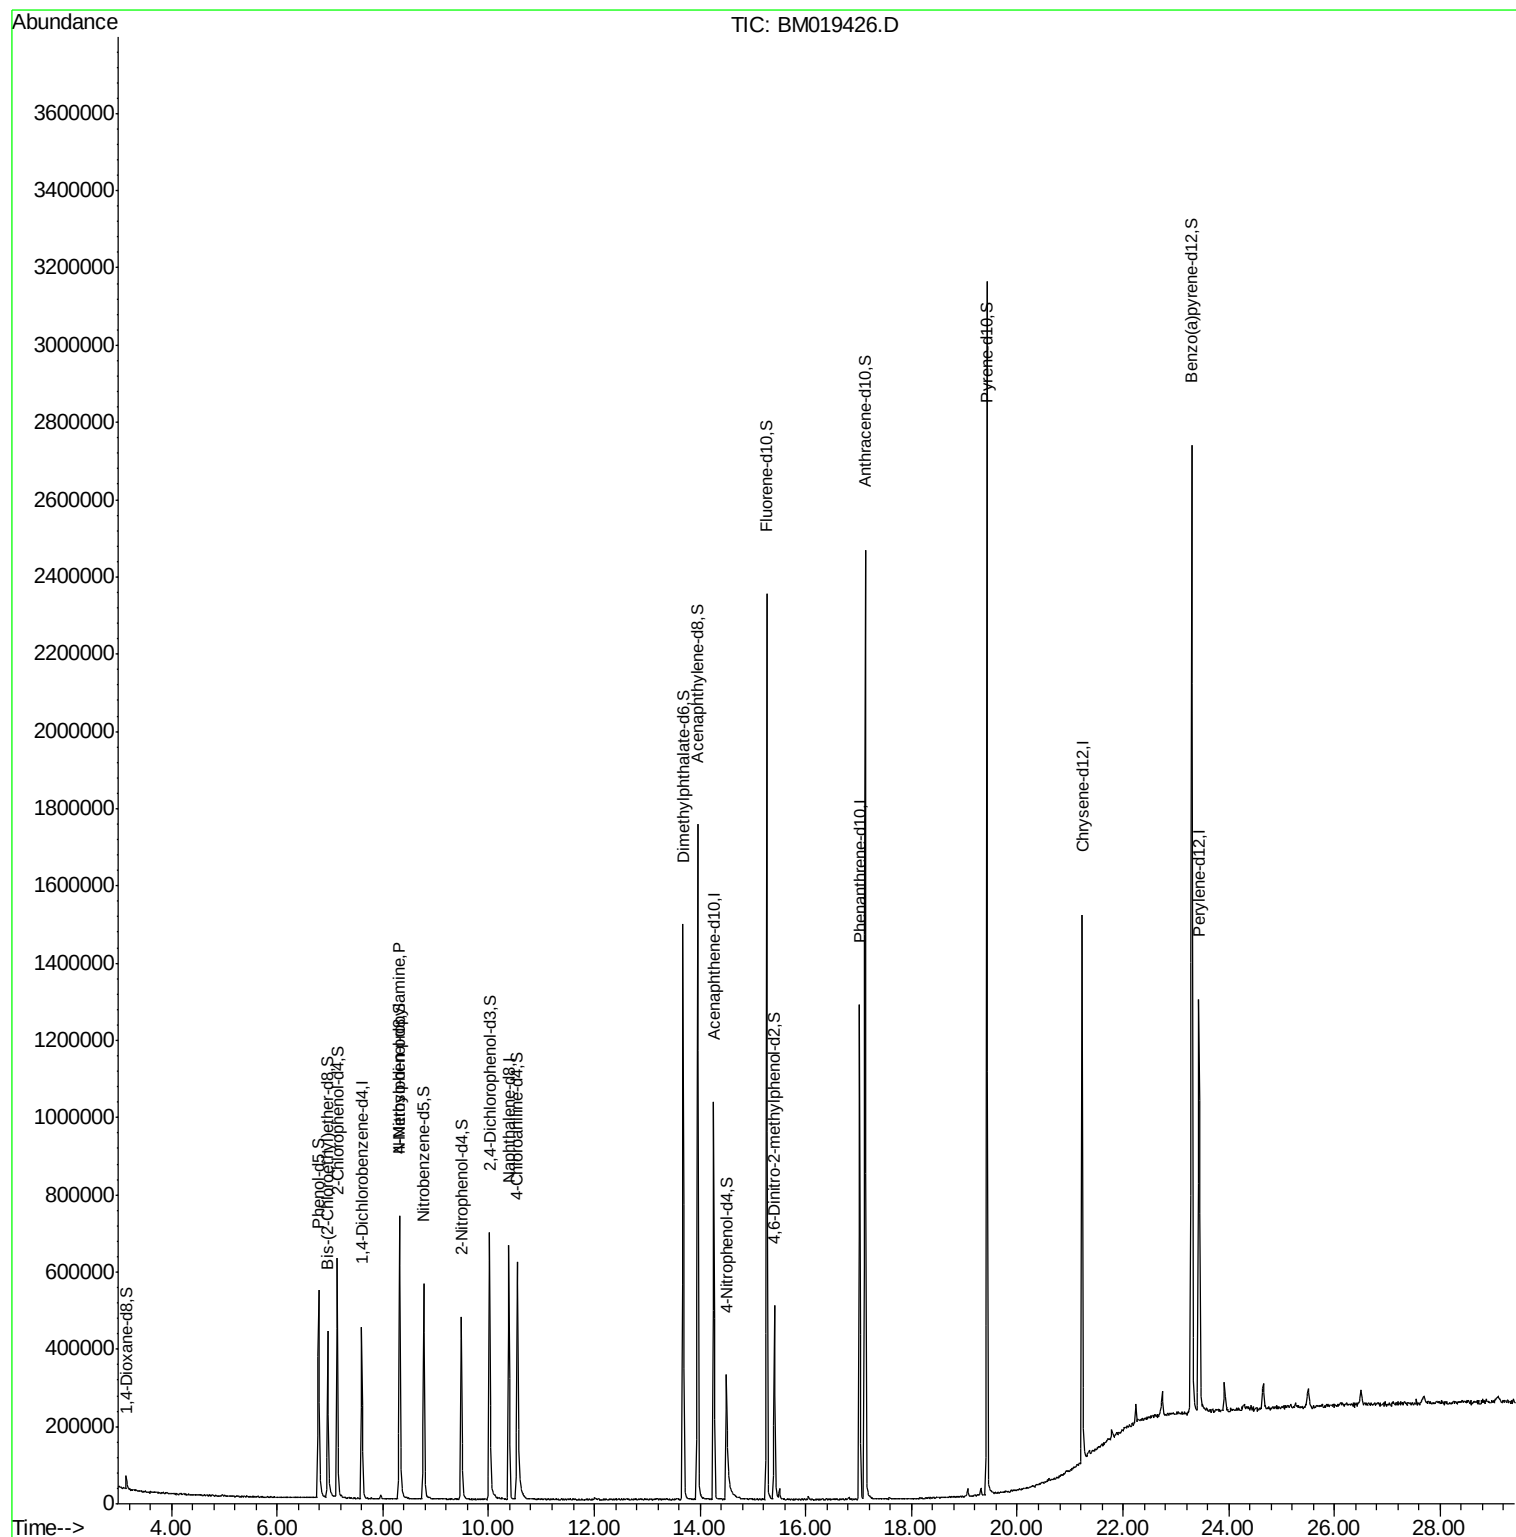

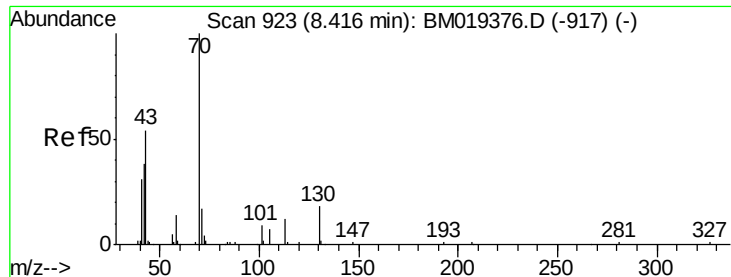

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.007 ng/ul
 RT: 8.32 min Scan# 906
 Delta R.T. -0.10 min
 Lab File: BM019426.D
 Acq: 25 Mar 2019 11:57

Instrument :
 BNA_M
 ClientSampleId :
 SBLK19

Tgt Ion:	70	Resp:	7693
Ion	Ratio	Lower	Upper
70	100		
42	245.3	40.2	60.4#
101	0.0	7.7	11.5#
130	0.0	17.8	26.6#

