

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
 Data File : BM019438.D
 Acq On : 25 Mar 2019 19:14
 Operator : JU/SJ
 Sample : K2027-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C09D1

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:32:20 PM

Quant Time: Apr 05 07:30:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 03:11:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	139109	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	589194	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	341263	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	753846	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	789450	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	862473	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	11435	3.22	ng/uL	0.00
5) Phenol-d5	6.79	99	62320	5.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	157520	18.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	174653	18.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	112031	12.05	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	95146	22.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	109005	23.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	189232	21.44	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.68	166	667253	24.23	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	841874	24.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	15259m	3.54	ng/ul	0.05
58) Fluorene-d10	15.26	176	597605	25.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	89776	18.01	ng/ul	0.00
71) Anthracene-d10	17.12	188	937159	25.91	ng/ul	0.00
79) Pyrene-d10	19.43	212	1022558	28.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1113069	24.34	ng/ul	0.00

Target Compounds

				Ovalue	
73) 1,2,3,4-Tetrachlorobenzene	13.05	216	66141	6.052	ng/uL 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
Data File : BM019438.D
Acq On : 25 Mar 2019 19:14
Operator : JU/SJ
Sample : K2027-15
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C09D1

Quant Time: Apr 05 07:30:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 03:11:42 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/26/2019 6:32:20 PM

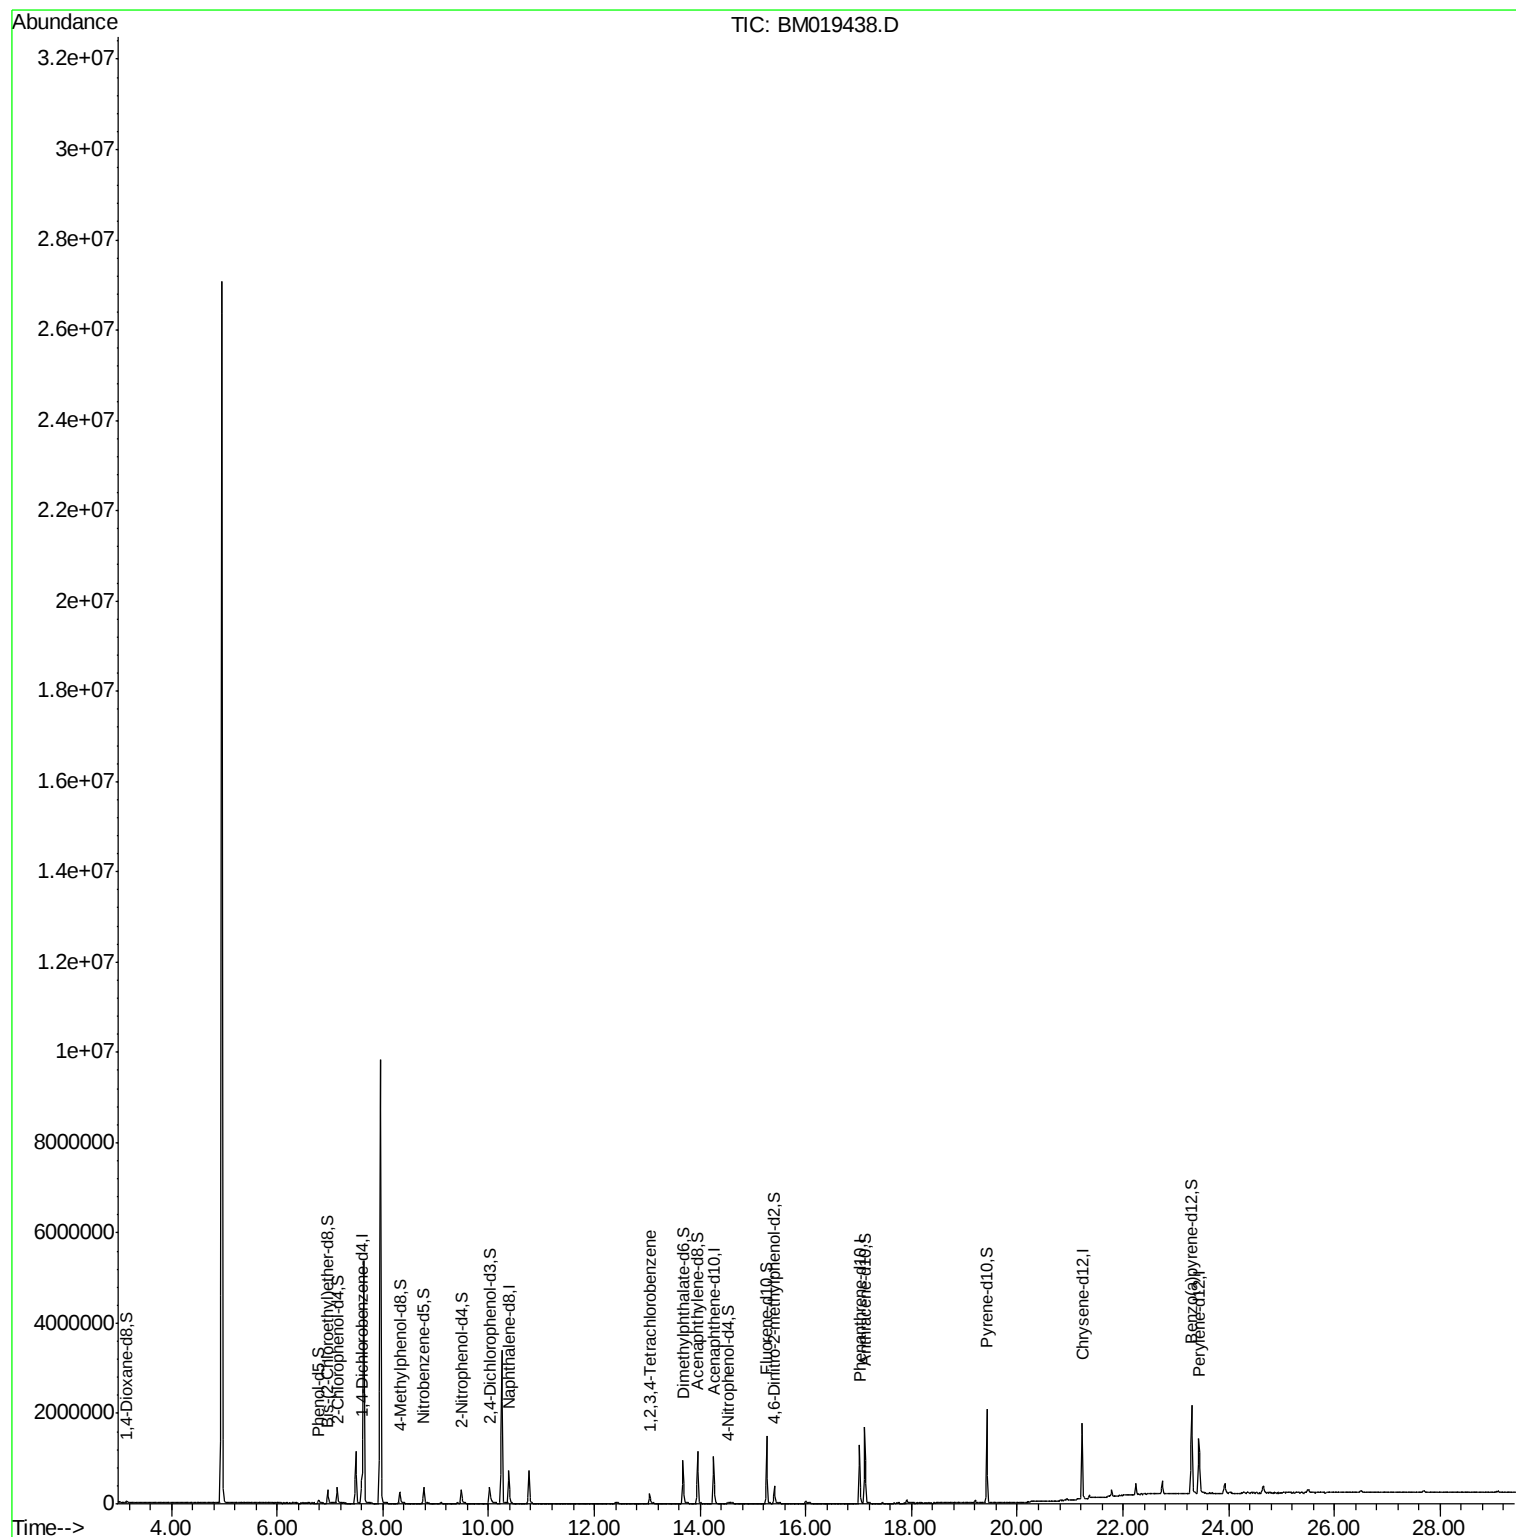

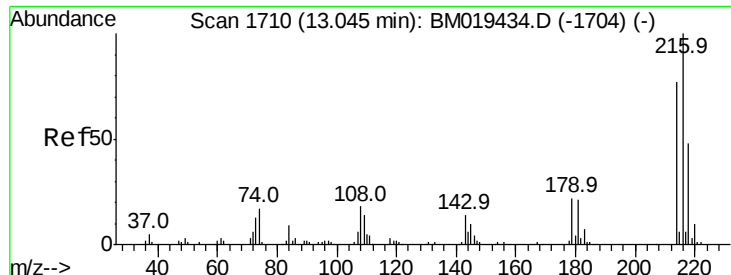

#73

1,2,3,4-Tetrachlorobenzene

Concen: 6.052 ng/uL

RT: 13.05 min Scan# 1711

Delta R.T. -0.00 min

Lab File: BM019438.D

Acq: 25 Mar 2019 19:14

Instrument :

BNA_M


ClientSampleId :

C09D1

Tot Ion:	216	Resp:	66141
Ion Ratio	Lower	Upper	
216	100		
214	79.5	64.1	96.1
218	47.2	39.4	59.0

Manual Integrations
APPROVED

Sohil
3/26/2019 6:32:20 PM

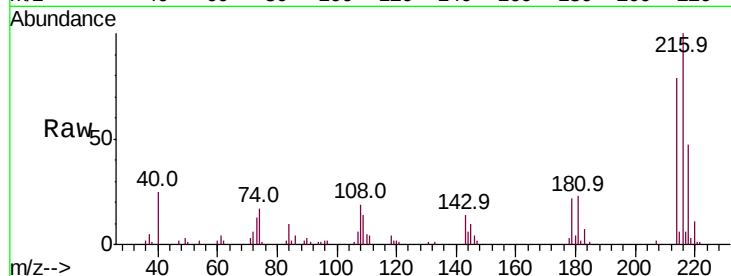

Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 218.00 (217.70 to 218.70): E

