

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
 Data File : BM019435.D
 Acq On : 25 Mar 2019 17:25
 Operator : JU/SJ
 Sample : PB118220BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	37	rVB	38689	58057	1.30%	0.144%
2	6.781	639	645	661	rBV	542241	980440	21.91%	2.438%
3	6.957	669	675	688	rBV	445634	785182	17.54%	1.953%
4	7.134	699	705	721	rVB	642613	1064350	23.78%	2.647%
5	7.604	779	785	796	rBV	500175	811966	18.14%	2.019%
6	8.316	900	906	924	rBV	711824	1278682	28.57%	3.180%
7	8.775	977	984	1000	rBV	539614	972807	21.74%	2.419%
8	9.486	1098	1105	1123	rBV	465264	818209	18.28%	2.035%
9	10.016	1189	1195	1224	rBV	673215	1289962	28.82%	3.208%
10	10.386	1250	1258	1267	rBV	715003	1209570	27.03%	3.008%
11	10.545	1278	1285	1314	rBV	595194	1325404	29.62%	3.296%
12	12.028	1530	1537	1541	rBV4	5764	12824	0.29%	0.032%
13	13.680	1812	1818	1831	rBV	1379236	2054298	45.90%	5.108%
14	13.951	1858	1864	1882	rBV	1706475	2552697	57.04%	6.348%
15	14.263	1908	1917	1926	rBV2	1014835	1594128	35.62%	3.964%
16	14.498	1951	1957	1978	rBV	291539	740542	16.55%	1.842%
17	15.263	2080	2087	2101	rBV	2201004	3188649	71.25%	7.929%
18	15.404	2106	2111	2123	rVV	529059	799113	17.86%	1.987%
19	15.504	2124	2128	2135	rVB	26678	38298	0.86%	0.095%
20	16.051	2217	2221	2224	rVB4	6603	9069	0.20%	0.023%
21	16.810	2348	2350	2356	rVB2	4719	6748	0.15%	0.017%
22	17.015	2379	2385	2396	rBV2	1273932	1825541	40.79%	4.540%
23	17.115	2396	2402	2423	rVV	2295087	3448099	77.05%	8.574%
24	19.062	2729	2733	2739	rVV3	17660	26793	0.60%	0.067%
25	19.315	2771	2776	2781	rBV	18820	25273	0.56%	0.063%
26	19.427	2789	2795	2808	rBV	2944393	3930536	87.83%	9.774%
27	19.798	2856	2858	2861	rBV3	4490	5985	0.13%	0.015%
28	21.227	3096	3101	3111	rBV	1600943	2080864	46.50%	5.174%
29	21.792	3194	3197	3205	rBV2	60510	77535	1.73%	0.193%
30	22.244	3270	3274	3278	rBV2	120057	153795	3.44%	0.382%
31	22.739	3355	3358	3364	rVB2	141829	184155	4.11%	0.458%
32	23.303	3446	3454	3466	rBV2	2430638	4475333	100.00%	11.129%
33	23.439	3471	3477	3490	rVV2	1154077	2190886	48.95%	5.448%
34	23.927	3556	3560	3567	rVB2	114009	198220	4.43%	0.493%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
Data File : BM019435.D
Acq On : 25 Mar 2019 17:25
Operator : JU/SJ
Sample : PB118220BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 40214010

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
Data File : BM019435.D
Acq On : 25 Mar 2019 17:25
Operator : JU/SJ
Sample : PB118220BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

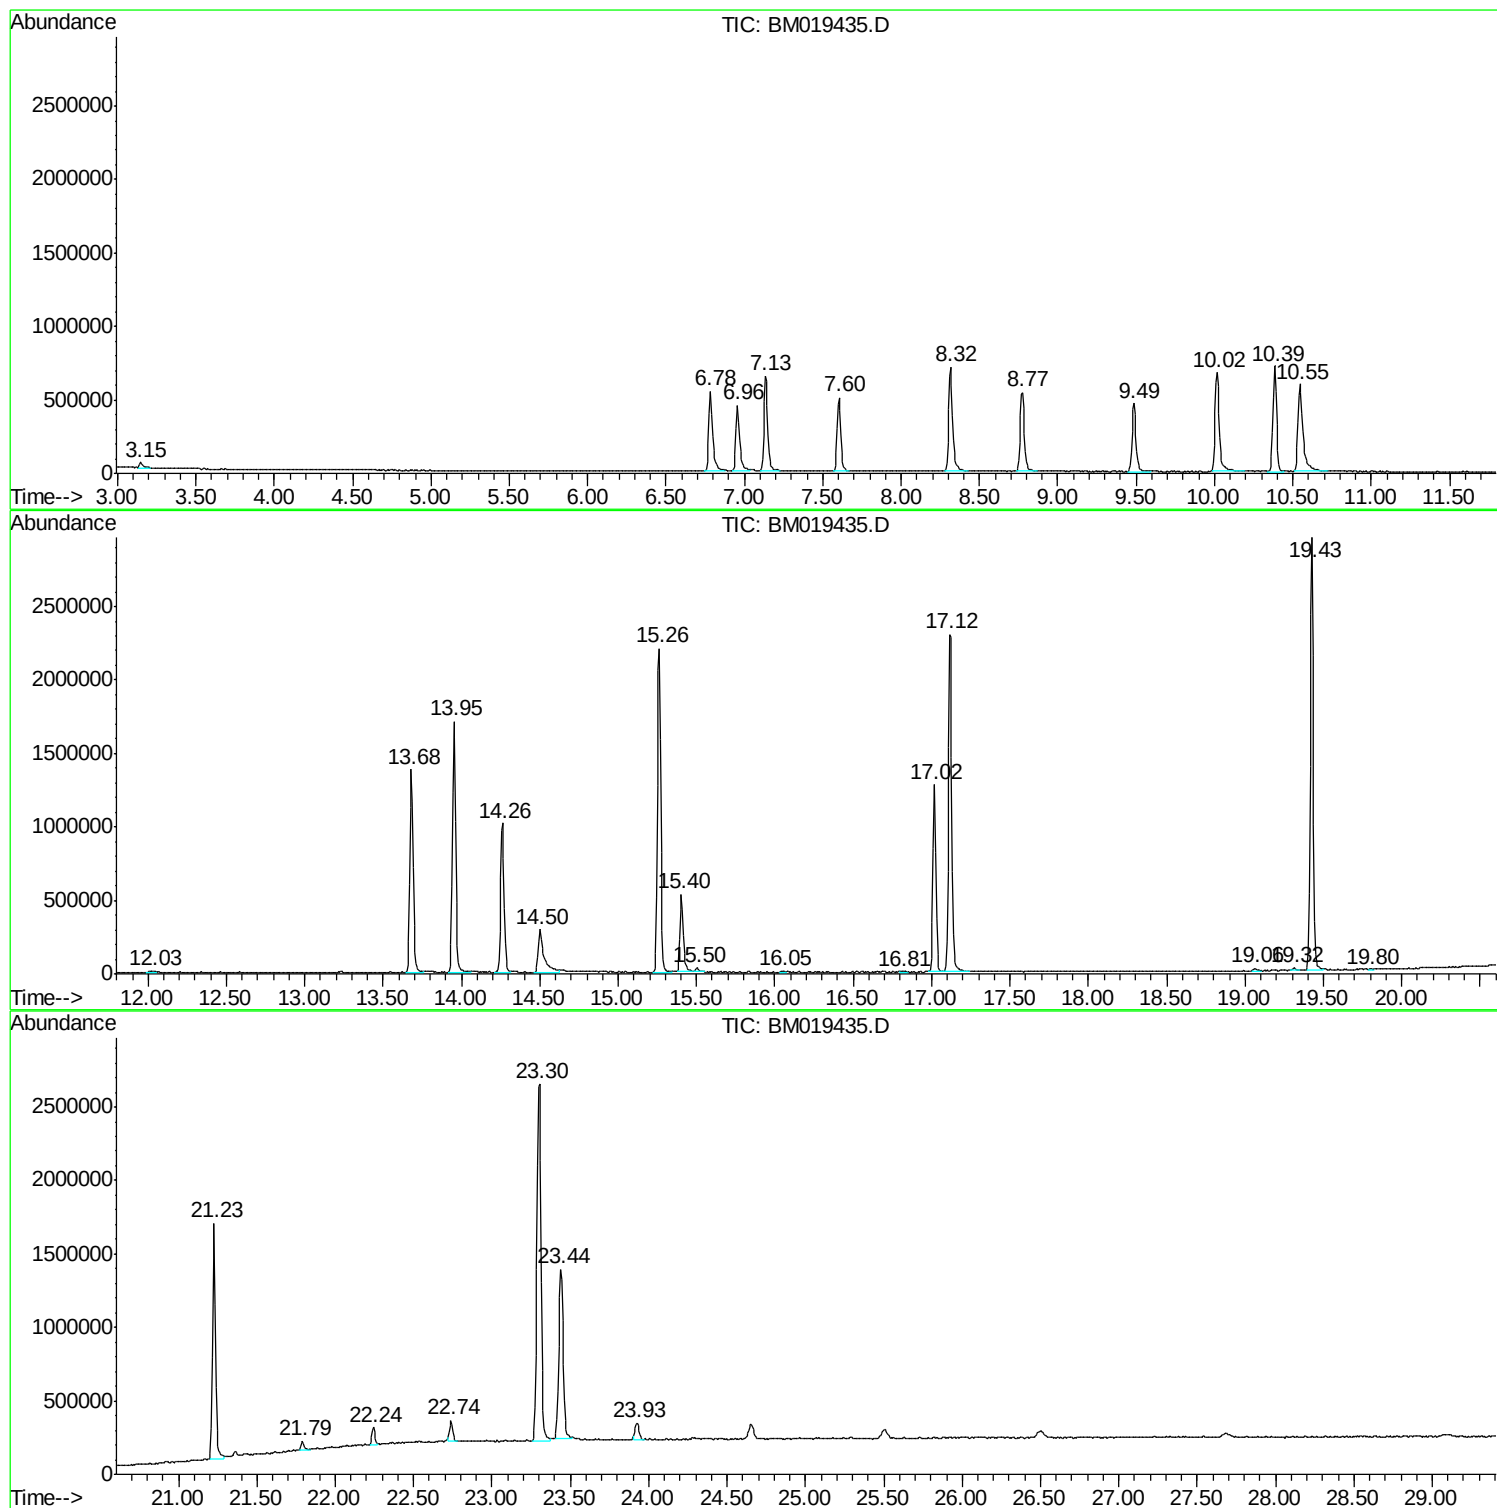

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
Data File : BM019435.D
Acq On : 25 Mar 2019 17:25
Operator : JU/SJ
Sample : PB118220BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
Data File : BM019435.D
Acq On : 25 Mar 2019 17:25
Operator : JU/SJ
Sample : PB118220BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc