

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
 Data File : BM019459.D
 Acq On : 26 Mar 2019 07:51
 Operator : JU/SJ
 Sample : K2049-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P003-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	32	rBV	15430	20966	0.77%	0.101%
2	4.946	327	333	348	rVB	599275	886201	32.75%	4.263%
3	6.804	644	649	652	rBV5	10333	17872	0.66%	0.086%
4	6.963	670	676	688	rBV	56457	123697	4.57%	0.595%
5	7.140	700	706	718	rBV	79304	142282	5.26%	0.684%
6	7.487	756	765	775	rVB	51519	84751	3.13%	0.408%
7	7.598	777	784	788	rBV	616261	1033461	38.20%	4.972%
8	7.634	788	790	802	rVB	258007	383540	14.18%	1.845%
9	7.945	837	843	857	rVB	264227	461614	17.06%	2.221%
10	8.334	902	909	921	rBV2	40438	92331	3.41%	0.444%
11	8.781	979	985	994	rBV	68356	142408	5.26%	0.685%
12	9.104	1036	1040	1043	rVB2	3056	3404	0.13%	0.016%
13	9.492	1100	1106	1118	rBV	54850	110221	4.07%	0.530%
14	10.045	1193	1200	1202	rBV2	36345	64476	2.38%	0.310%
15	10.245	1228	1234	1246	rBV	257068	432617	15.99%	2.081%
16	10.380	1251	1257	1272	rVV	897761	1556033	57.51%	7.486%
17	10.475	1272	1273	1279	rVV3	2370	3460	0.13%	0.017%
18	10.769	1316	1323	1334	rBV2	53093	97935	3.62%	0.471%
19	13.063	1709	1713	1721	rBV3	9059	15658	0.58%	0.075%
20	13.686	1813	1819	1832	rBV	216259	376887	13.93%	1.813%
21	13.951	1858	1864	1873	rBV	272930	430637	15.92%	2.072%
22	14.257	1910	1916	1931	rBV2	1398161	2202457	81.40%	10.595%
23	15.262	2081	2087	2107	rBV	354189	607344	22.45%	2.922%
24	15.415	2109	2113	2124	rVV3	33553	66941	2.47%	0.322%
25	15.510	2127	2129	2135	rVB4	3819	5109	0.19%	0.025%
26	16.809	2347	2350	2354	rVB3	4509	5552	0.21%	0.027%
27	17.015	2379	2385	2397	rBV2	1770685	2542262	93.96%	12.230%
28	17.121	2397	2403	2425	rVB2	379624	662264	24.48%	3.186%
29	17.621	2487	2488	2493	rVB2	2396	3236	0.12%	0.016%
30	17.827	2520	2523	2526	rBV3	2274	3364	0.12%	0.016%
31	17.909	2533	2537	2541	rBV5	8926	15240	0.56%	0.073%
32	19.068	2731	2734	2738	rVB4	3661	5241	0.19%	0.025%
33	19.156	2745	2749	2751	rBV3	2884	4191	0.15%	0.020%
34	19.209	2754	2758	2760	rVV3	4813	6364	0.24%	0.031%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
Data File : BM019459.D
Acq On : 26 Mar 2019 07:51
Operator : JU/SJ
Sample : K2049-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P003-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Title : SVOA CALIBRATION

35	19.315	2772	2776	2779	rBV3	4905	5700	0.21%	0.027%
36	19.421	2789	2794	2803	rBV2	532096	802347	29.66%	3.860%
37	19.492	2804	2806	2814	rVB2	10697	16143	0.60%	0.078%
38	19.956	2882	2885	2889	rBV6	11594	12856	0.48%	0.062%
39	20.456	2967	2970	2972	rBV3	16599	17796	0.66%	0.086%
40	20.921	3046	3049	3056	rBV5	39861	64328	2.38%	0.309%
41	21.221	3095	3100	3112	rBV	2037611	2705565	100.00%	13.016%
42	21.362	3121	3124	3129	rVB2	56145	60153	2.22%	0.289%
43	21.786	3193	3196	3200	rBV	79624	84778	3.13%	0.408%
44	22.239	3270	3273	3278	rVB	127746	146421	5.41%	0.704%
45	22.733	3354	3357	3364	rVB	133165	186396	6.89%	0.897%
46	23.291	3446	3452	3463	rBV2	540819	998138	36.89%	4.802%
47	23.433	3470	3476	3493	rVB	1336503	2597294	96.00%	12.495%
48	23.921	3555	3559	3564	rVB	129647	226106	8.36%	1.088%
49	24.644	3678	3682	3692	rVB3	118791	253154	9.36%	1.218%


Sum of corrected areas: 20787191

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032519\
Data File : BM019459.D
Acq On : 26 Mar 2019 07:51
Operator : JU/SJ
Sample : K2049-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P003-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

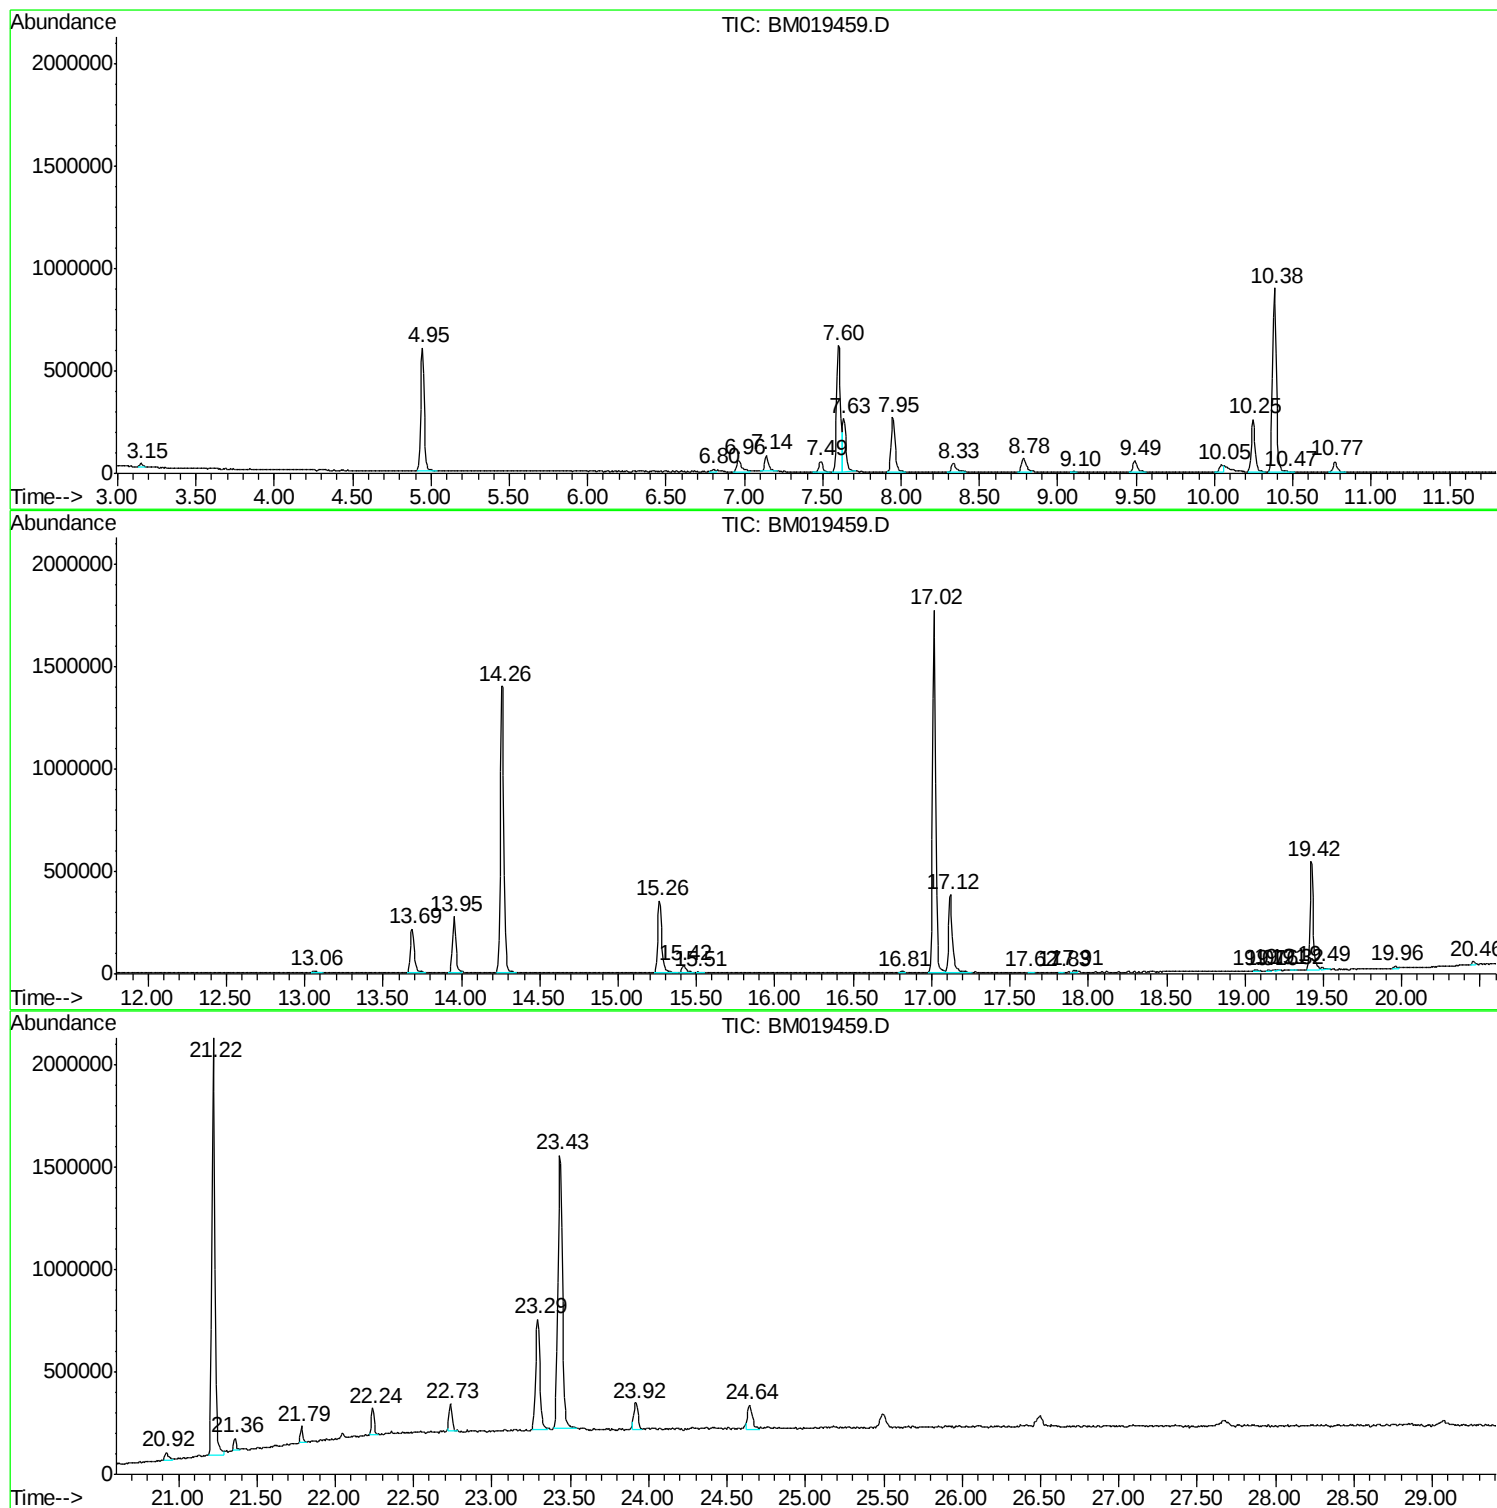

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032519\
Data_File : BM019459.D
Acq_On : 26-Mar-2019 07:511
Operator : JU/SJJ
Sample : K2049-055
Misc :
ALS_Vial : 38 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
P003-TW001-01

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
