
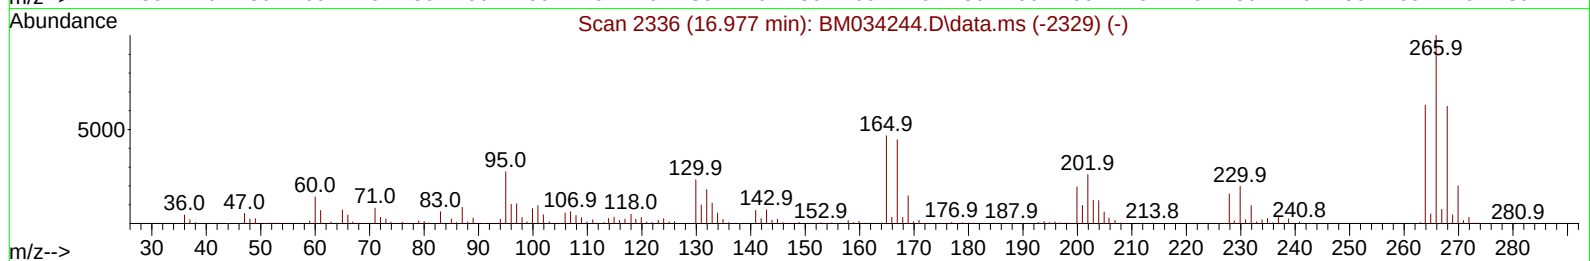
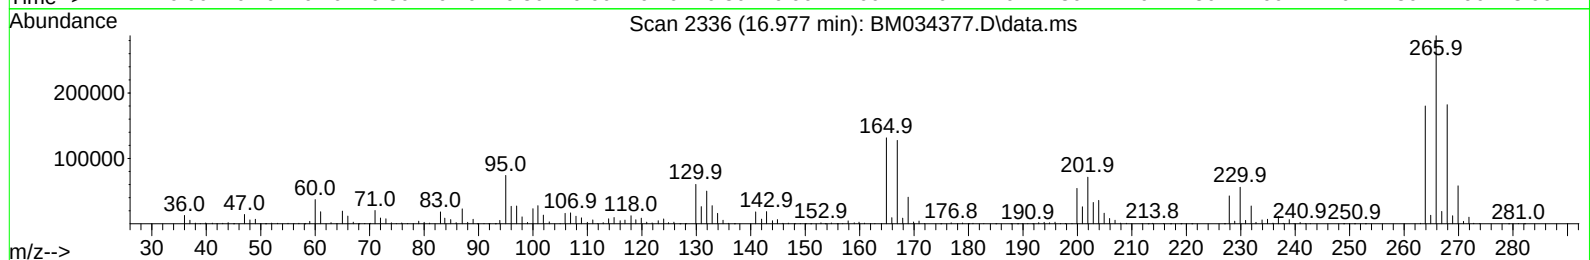


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034377.D
Acq On : 25 Mar 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:43:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 02:40:59 2022
Response via : Initial Calibration

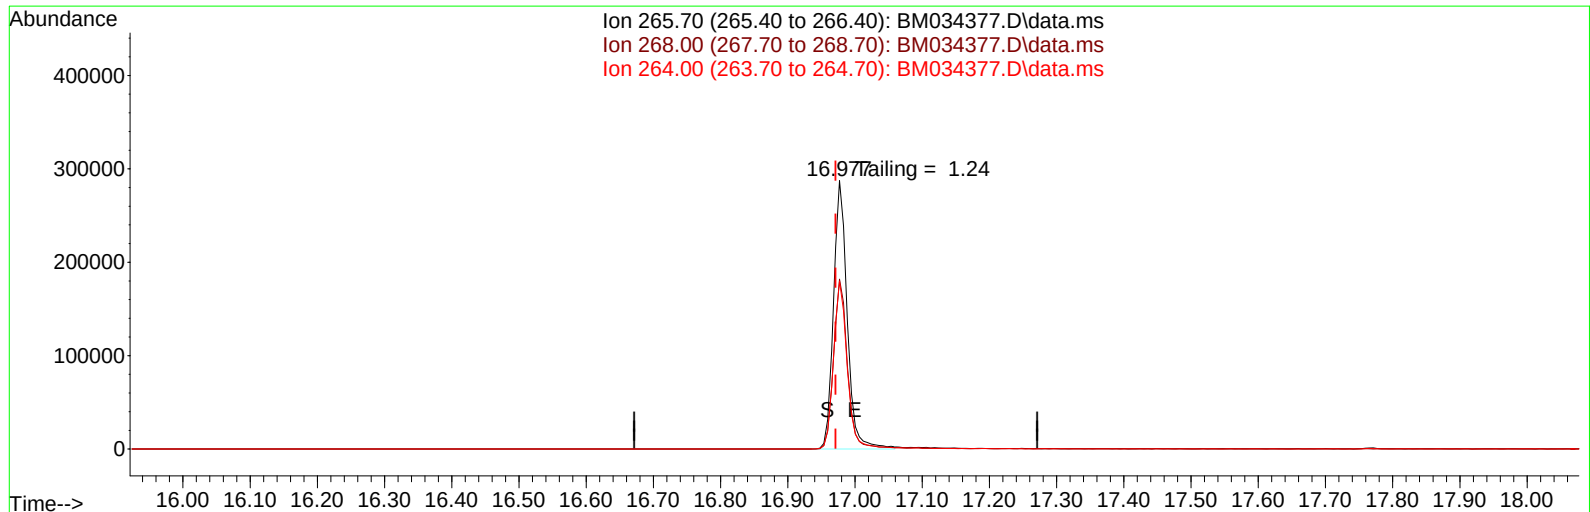

TIC: BM034377.D\data.ms

(70) Pentachlorophenol (C)




16.977min (+ 0.006) 329214.99 ng

response 410315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.35
264.00	62.90	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034377.D
Acq On : 25 Mar 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:43:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 02:40:59 2022
Response via : Initial Calibration

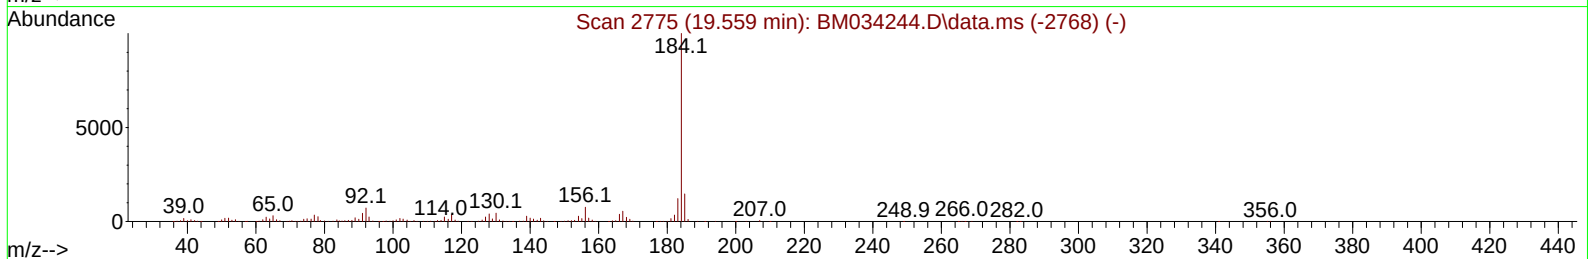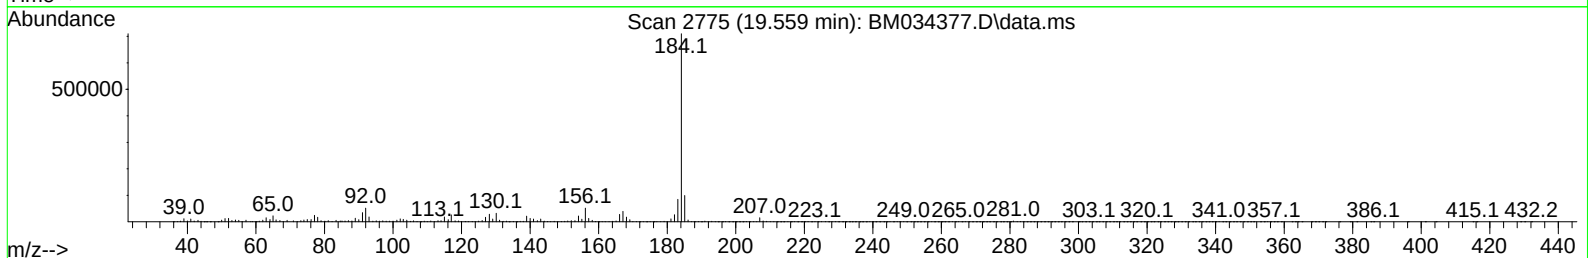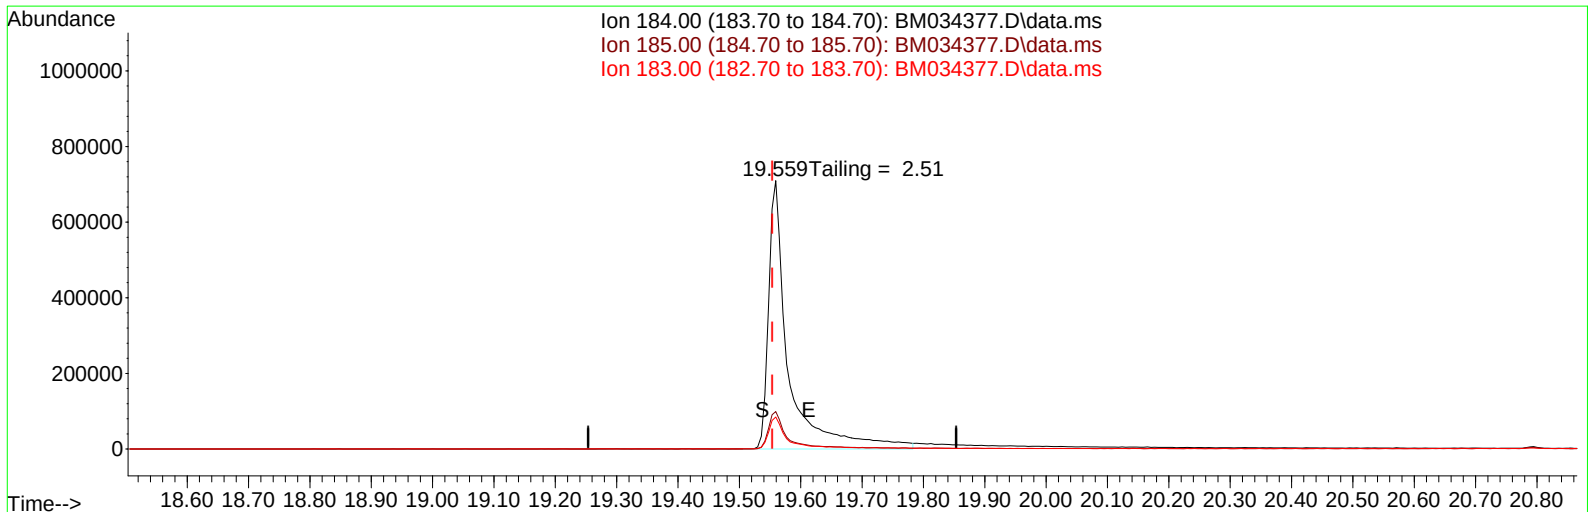

TIC: BM034377.D\data.ms

(77) Benzidine**19.559min (+ 0.006) 221201.80 ng****response 1675892**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.00
183.00	12.20	11.92
0.00	0.00	0.00