

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
 Data File : BM034379.D
 Acq On : 25 Mar 2022 10:40
 Operator : CG/JU
 Sample : PB143484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143484BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.495	377	384	397	rBV	4330869	6347679	46.32%	10.521%
2	7.107	650	658	676	rBV	4076850	6574924	47.98%	10.897%
3	7.936	793	799	809	rBV	716125	1164969	8.50%	1.931%
4	9.107	988	998	1014	rBV	2465646	4250170	31.02%	7.044%
5	10.754	1270	1278	1289	rBV	920932	1601665	11.69%	2.655%
6	13.213	1688	1696	1708	rBV	6671156	9759706	71.22%	16.176%
7	14.583	1922	1929	1949	rBV	1445985	2178945	15.90%	3.611%
8	16.071	2174	2182	2208	rBV	4888274	7718524	56.33%	12.793%
9	17.324	2388	2395	2409	rBV	1667607	2505907	18.29%	4.153%
10	19.942	2834	2840	2855	rBV	10939960	13702969	100.00%	22.711%
11	21.494	3099	3104	3117	rBV	1519443	2382559	17.39%	3.949%
12	23.912	3510	3515	3531	rVB2	938900	2147251	15.67%	3.559%




Sum of corrected areas: 60335268

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034379.D
Acq On : 25 Mar 2022 10:40
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

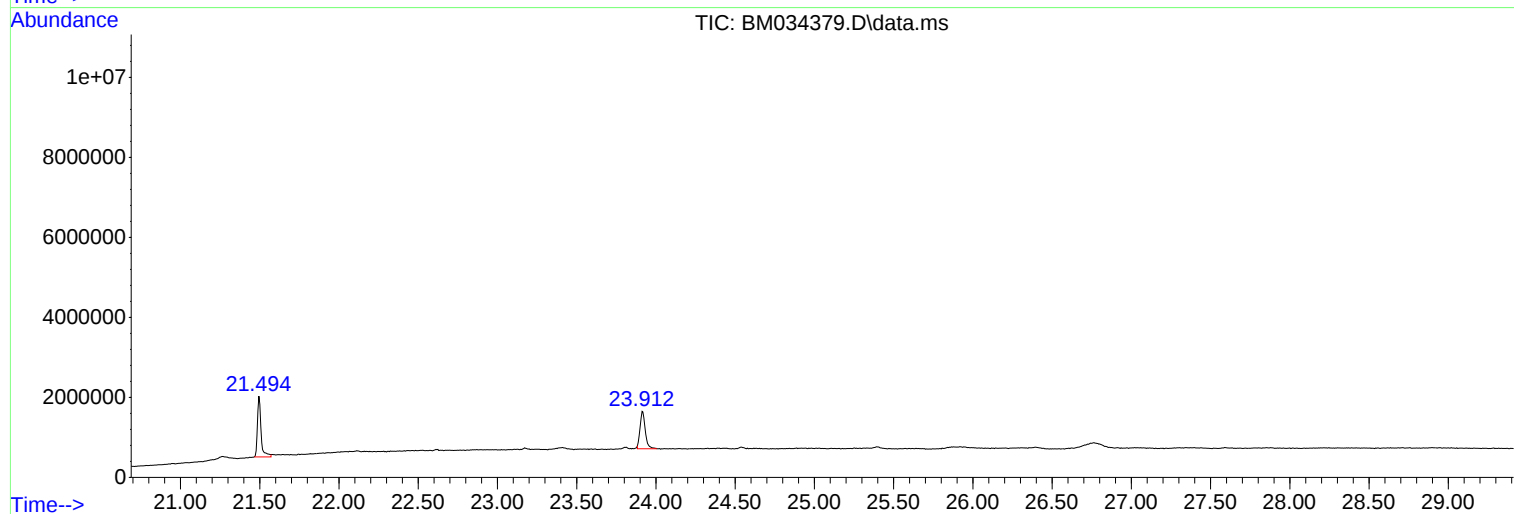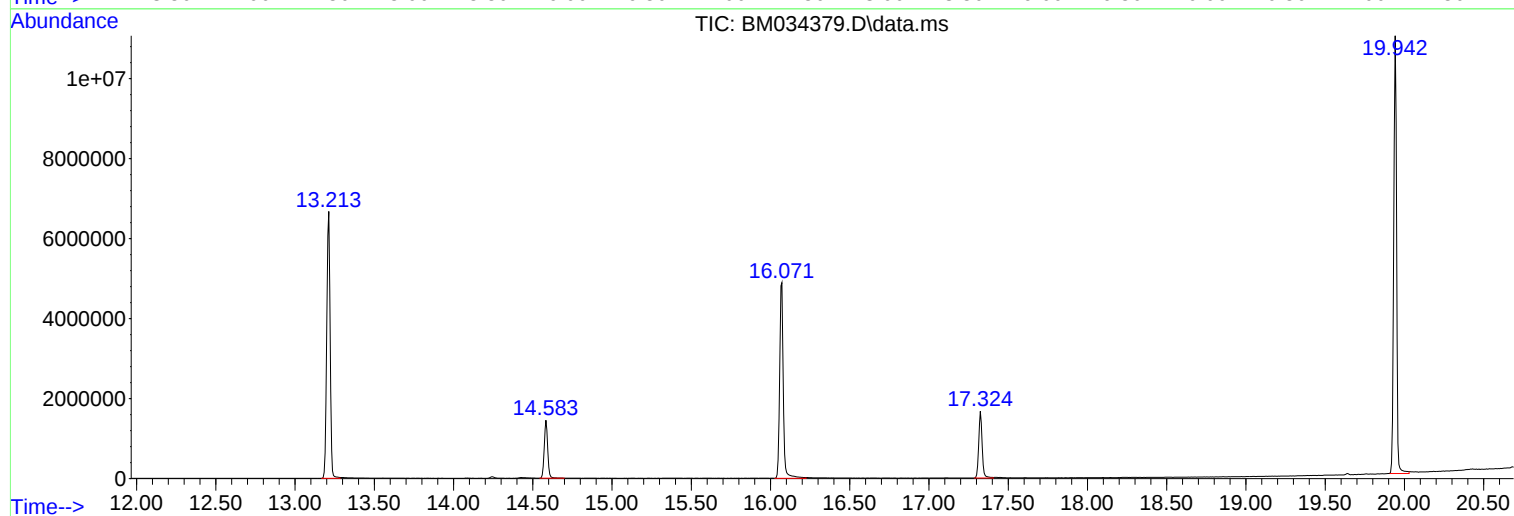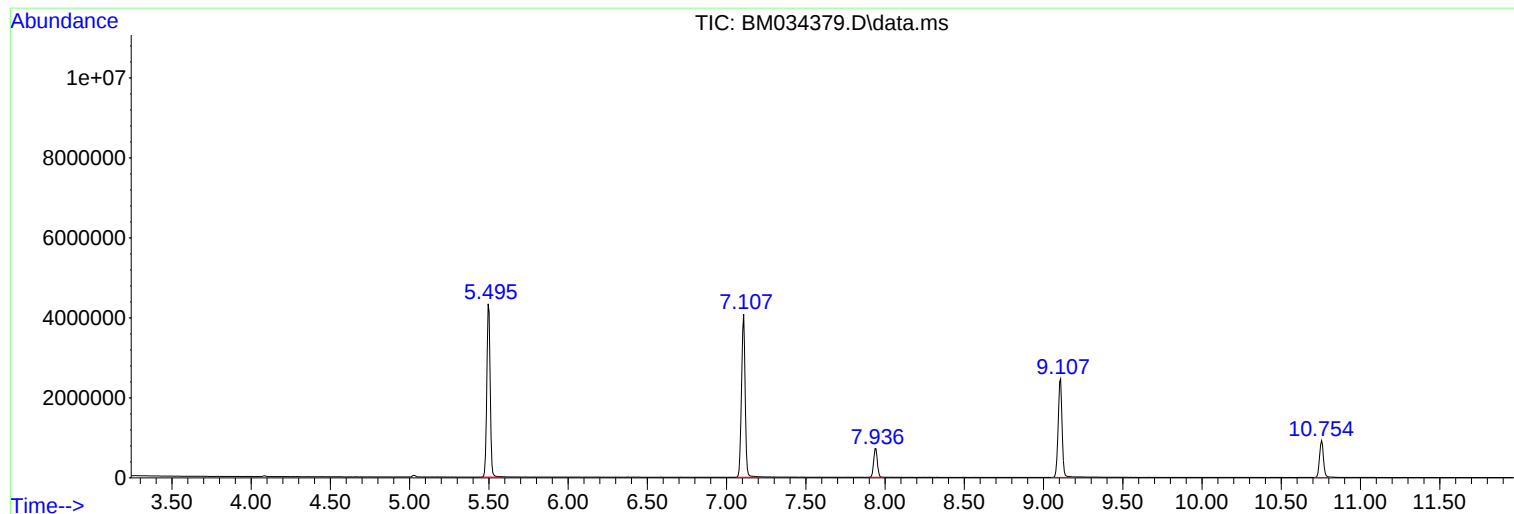

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034379.D
Acq On : 25 Mar 2022 10:40
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034379.D
Acq On : 25 Mar 2022 10:40
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------