

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
 Data File : BM034388.D
 Acq On : 25 Mar 2022 17:01
 Operator : CG/JU
 Sample : N2103-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CHRT-2001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	377	384	393	rBV	2341104	3369251	51.77%	6.630%
2	7.101	649	657	666	rBV	2115689	3401118	52.26%	6.693%
3	7.596	733	741	749	rBV3	30578	71997	1.11%	0.142%
4	7.937	792	799	810	rBV	528298	885778	13.61%	1.743%
5	9.101	991	997	1009	rVB	1324604	2181789	33.52%	4.294%
6	10.754	1270	1278	1283	rBV	639281	1114641	17.13%	2.194%
7	10.801	1283	1286	1295	rVB	56301	102414	1.57%	0.202%
8	12.413	1555	1560	1569	rVB2	42391	87958	1.35%	0.173%
9	13.207	1687	1695	1710	rBV	3351781	4974494	76.44%	9.789%
10	13.413	1727	1730	1738	rVB3	42117	65783	1.01%	0.129%
11	14.036	1828	1836	1839	rBV3	67547	143321	2.20%	0.282%
12	14.301	1876	1881	1892	rBV	216647	374689	5.76%	0.737%
13	14.419	1896	1901	1909	rVV5	42902	69181	1.06%	0.136%
14	14.583	1920	1929	1936	rBV	927935	1429577	21.97%	2.813%
15	14.642	1936	1939	1948	rVB	58951	103732	1.59%	0.204%
16	14.977	1992	1996	2003	rBV2	45056	75752	1.16%	0.149%
17	15.183	2016	2031	2046	rBV5	95781	513318	7.89%	1.010%
18	15.448	2071	2076	2084	rVB2	56401	97014	1.49%	0.191%
19	15.624	2102	2106	2109	rBV4	48801	79069	1.21%	0.156%
20	16.066	2174	2181	2188	rBV	2503276	3674157	56.46%	7.230%
21	16.313	2216	2223	2228	rBV3	74489	167566	2.57%	0.330%
22	17.142	2361	2364	2372	rVB2	49692	79224	1.22%	0.156%
23	17.324	2389	2395	2399	rBV	1071311	1527932	23.48%	3.007%
24	17.366	2399	2402	2412	rVV	338691	483298	7.43%	0.951%
25	17.454	2413	2417	2423	rVV	184208	276123	4.24%	0.543%
26	18.218	2541	2547	2550	rBV2	344417	504459	7.75%	0.993%
27	18.395	2573	2577	2581	rBV2	155930	259429	3.99%	0.511%
28	19.118	2696	2700	2704	rBV	136644	214929	3.30%	0.423%
29	19.318	2731	2734	2739	rVB	187734	208674	3.21%	0.411%
30	19.377	2740	2744	2750	rBV	885574	1162720	17.87%	2.288%
31	19.530	2767	2770	2774	rVB	118603	147417	2.27%	0.290%
32	19.736	2798	2805	2814	rVB	1059829	1734673	26.65%	3.414%
33	19.942	2835	2840	2845	rBV	5442433	6507953	100.00%	12.807%
34	20.059	2857	2860	2868	rVB4	127523	218504	3.36%	0.430%
35	20.336	2904	2907	2912	rVB2	110804	141375	2.17%	0.278%
36	20.530	2938	2940	2943	rBV2	119012	121170	1.86%	0.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034388.D
Acq On : 25 Mar 2022 17:01
Operator : CG/JU
Sample : N2103-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CHRT-2001

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.201	3050	3054	3063	rVB5	796873	1173782	18.04%	2.310%
38	21.406	3085	3089	3094	rVB	5372335	6044885	92.88%	11.896%
39	21.495	3098	3104	3108	rVV3	1490161	2639819	40.56%	5.195%
40	21.536	3108	3111	3121	rVB	525174	774300	11.90%	1.524%
41	23.177	3386	3390	3396	rBV2	531091	1135922	17.45%	2.235%
42	23.812	3493	3498	3506	rVB	532910	1031929	15.86%	2.031%
43	23.918	3511	3516	3523	rVB2	764864	1444334	22.19%	2.842%




Sum of corrected areas: 50815450

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034388.D
Acq On : 25 Mar 2022 17:01
Operator : CG/JU
Sample : N2103-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CHRT-2001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

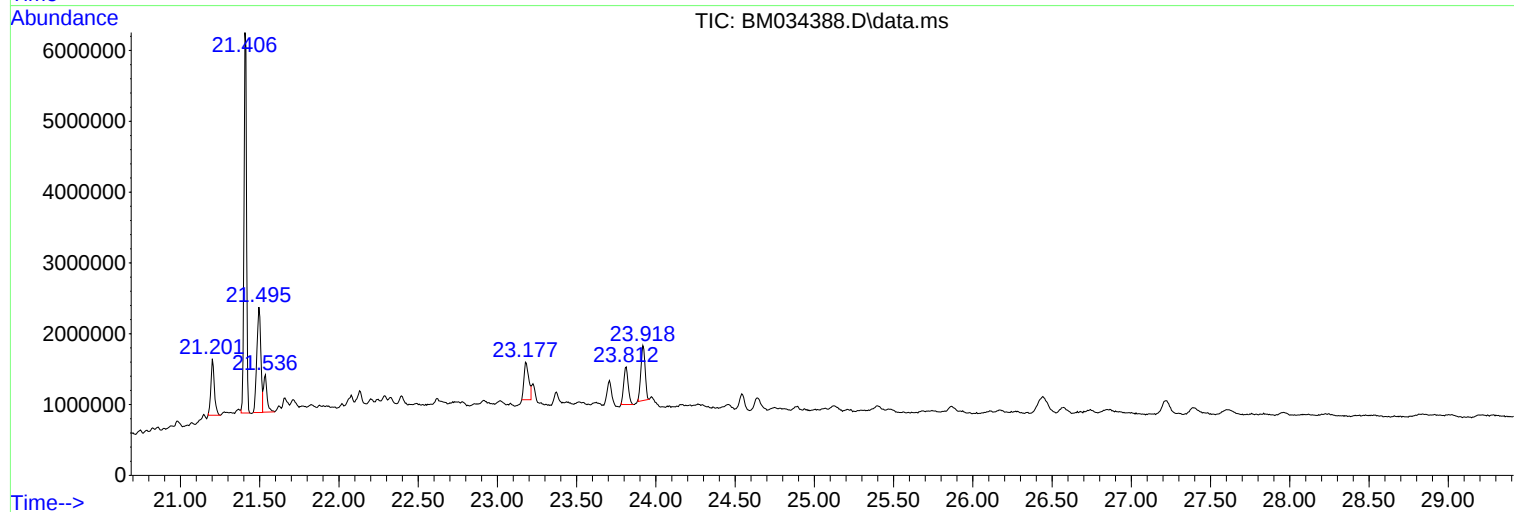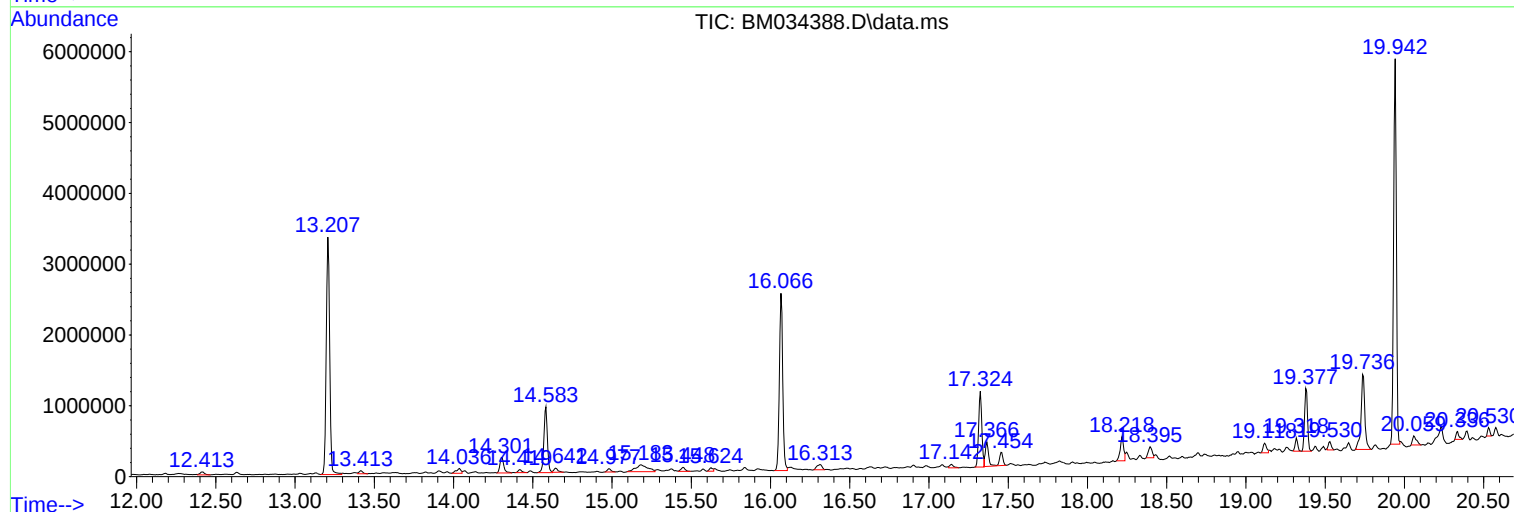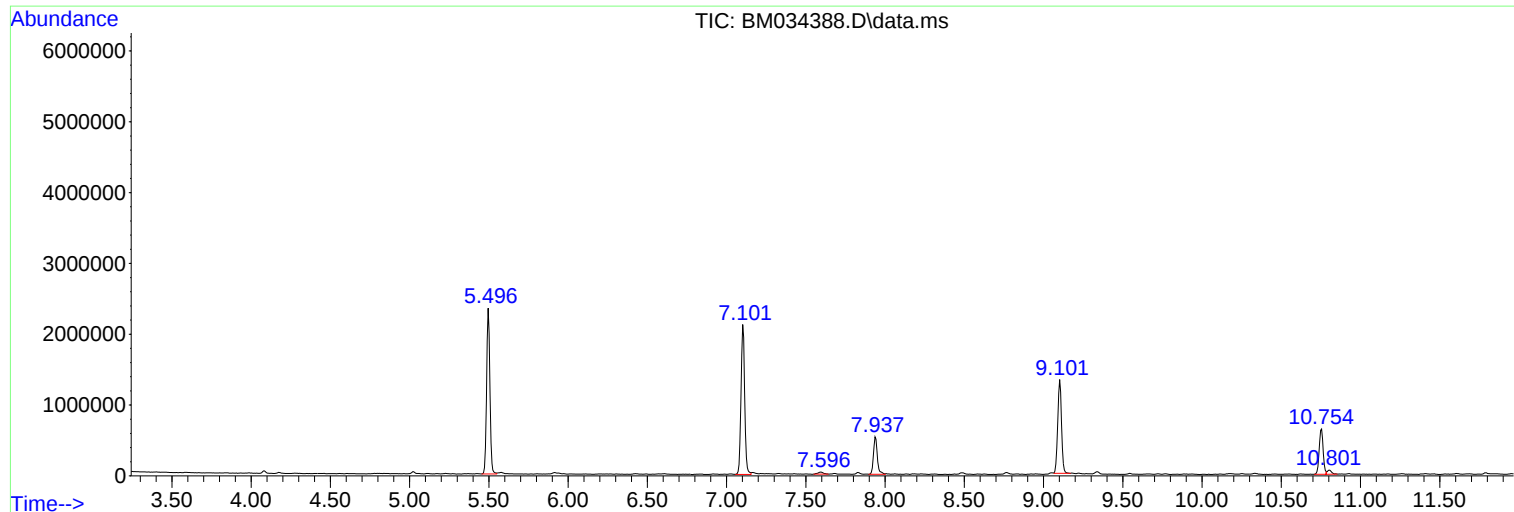

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034388.D
Acq On : 25 Mar 2022 17:01
Operator : CG/JU
Sample : N2103-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CHRT-2001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034388.D
Acq On : 25 Mar 2022 17:01
Operator : CG/JU
Sample : N2103-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CHRT-2001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------