


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
 Data File : BM034377.D
 Acq On : 25 Mar 2022 09:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 02:40:59 2022

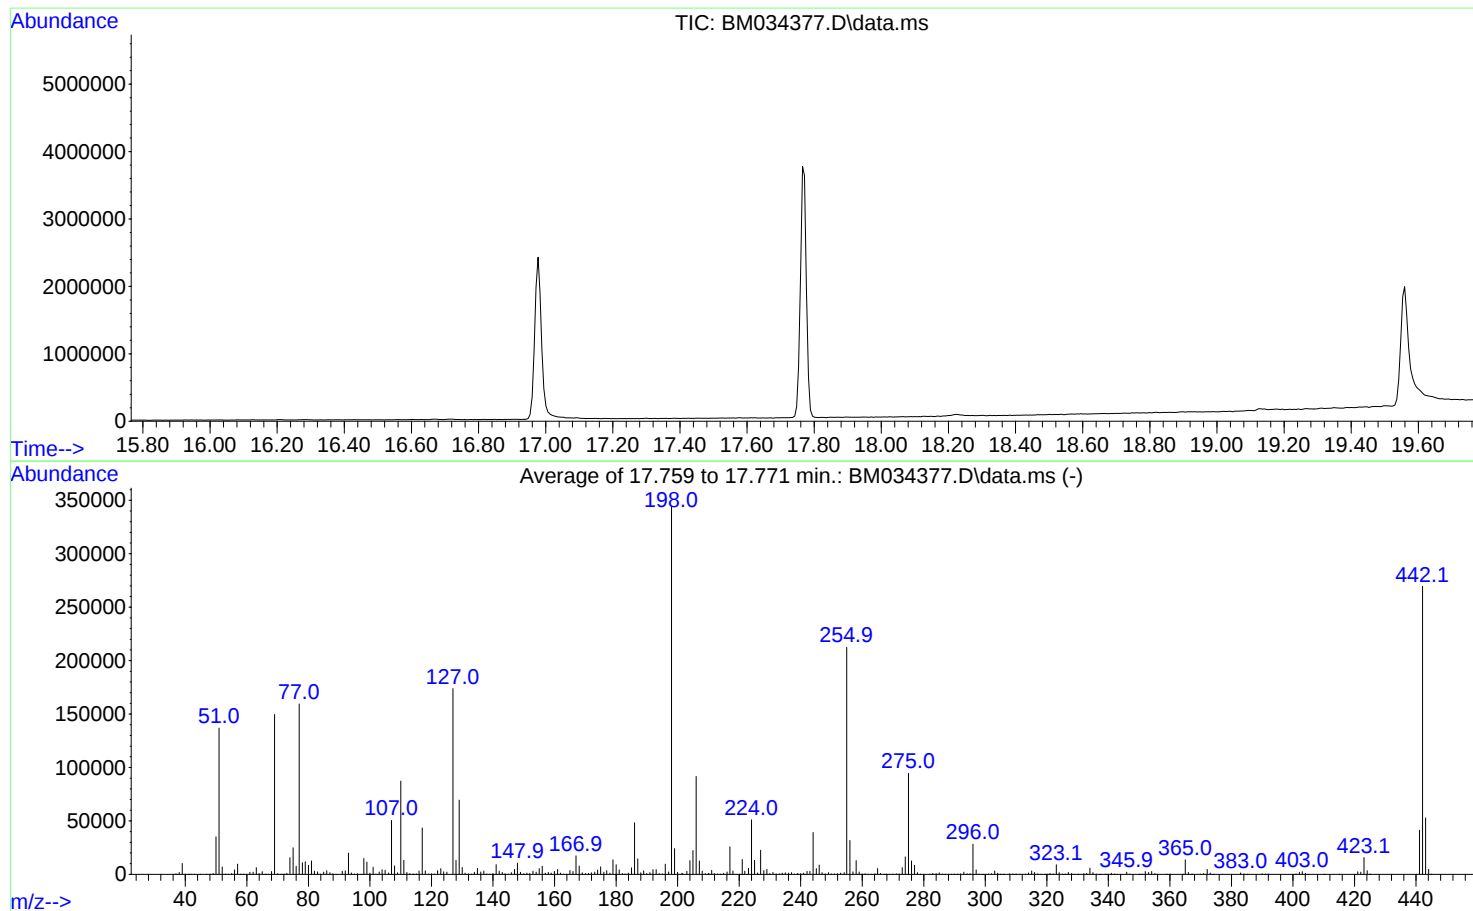




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	136927	PASS
68	69	0.00	2	1.8	2745	PASS
69	198	0.00	100	43.5	149617	PASS
70	69	0.00	2	0.5	754	PASS
127	198	10	80	50.5	173843	PASS
197	198	0.00	2	0.7	2273	PASS
198	198	100	100	100.0	344213	PASS
199	198	5	9	7.0	24091	PASS
275	198	10	60	27.5	94563	PASS
365	198	1	100	4.0	13602	PASS
441	198	0.01	100	12.0	41325	PASS
442	442	50	100	100.0	269461	PASS
443	442	15	24	19.6	52869	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
Data File : BM034377.D
Acq On : 25 Mar 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 26 07:43:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 02:40:59 2022
Response via : Initial Calibration

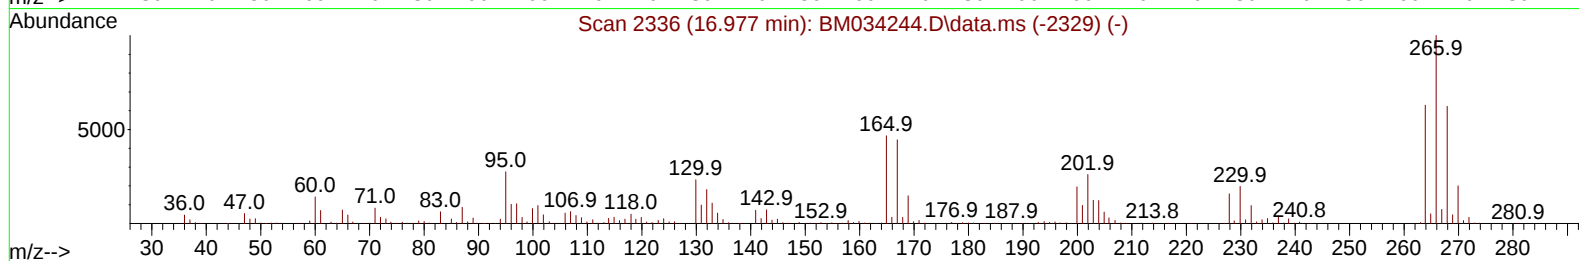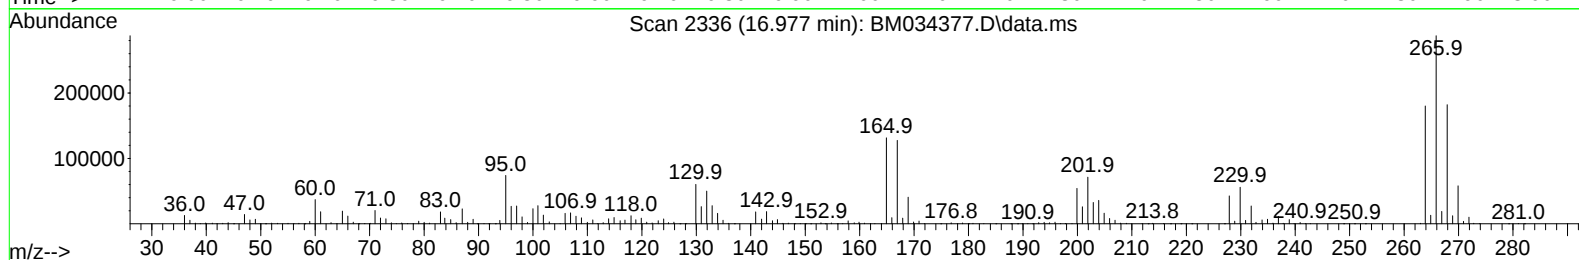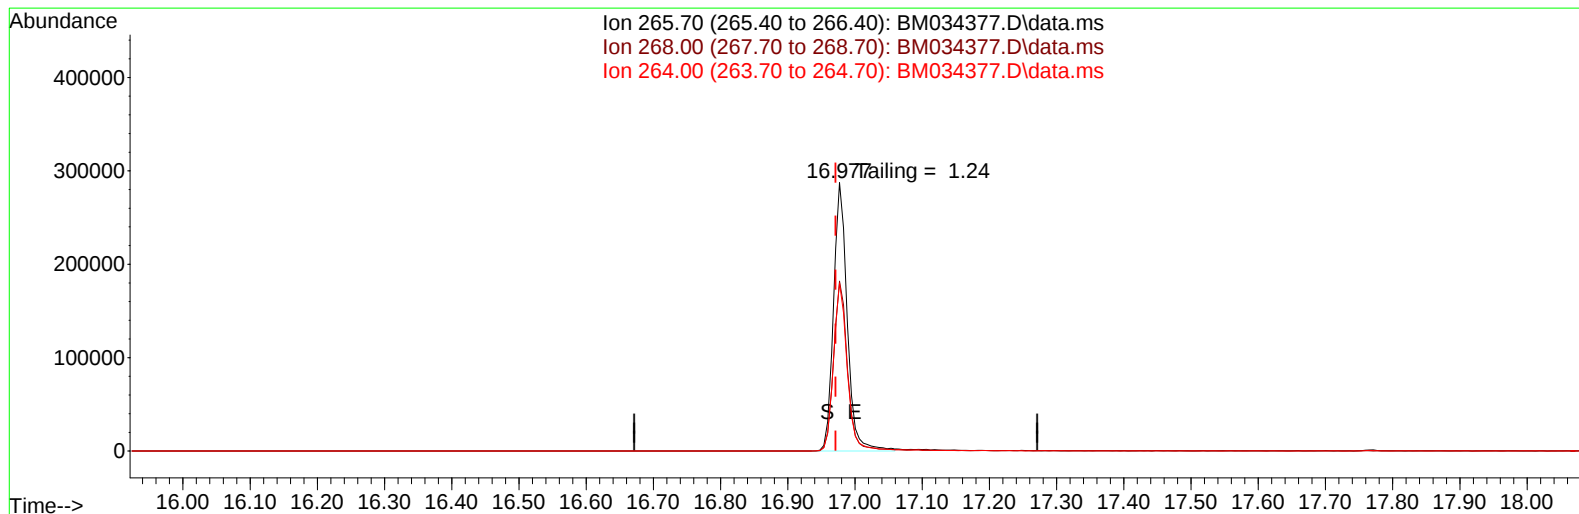

TIC: BM034377.D\data.ms

(70) Pentachlorophenol (C)

16.977min (+ 0.006) 329214.99 ng




response 410315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.35
264.00	62.90	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032522\
 Data File : BM034377.D
 Acq On : 25 Mar 2022 09:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 07:43:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 02:40:59 2022
 Response via : Initial Calibration

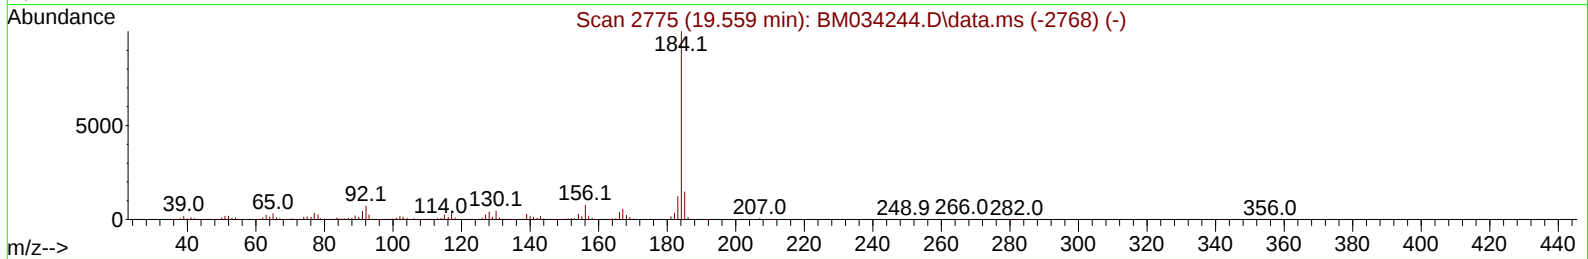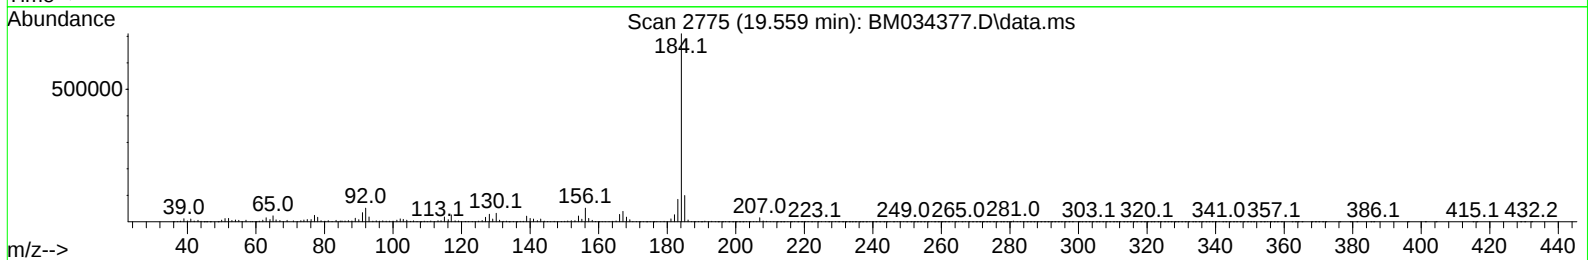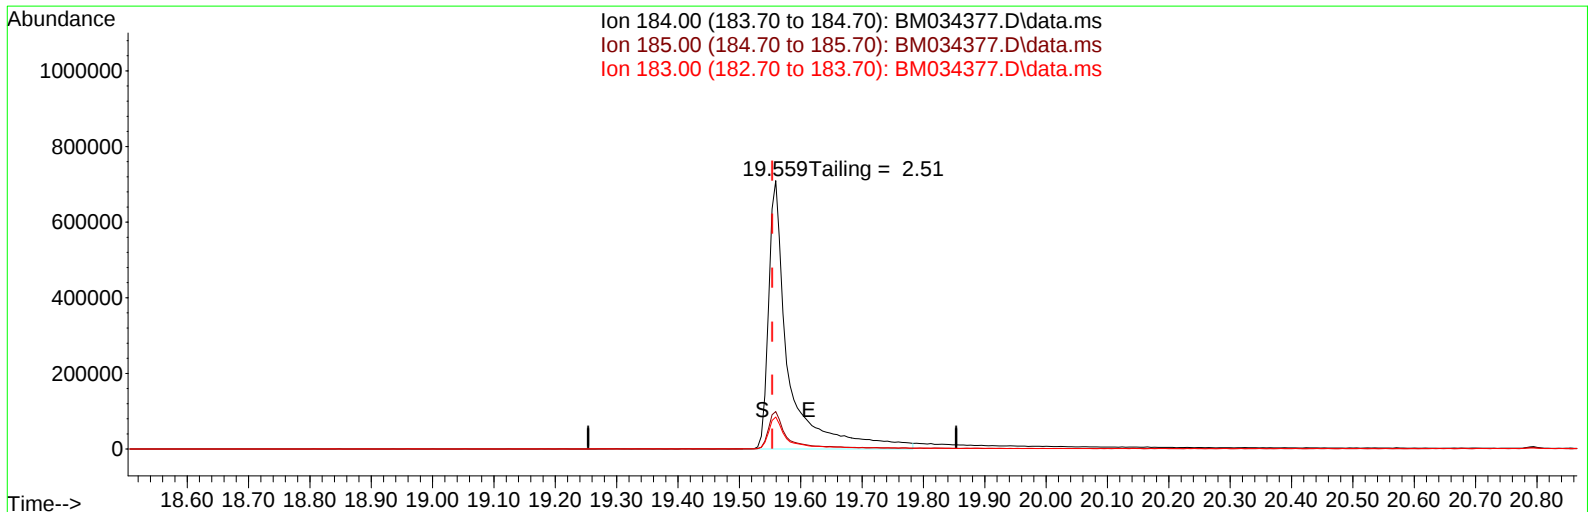

TIC: BM034377.D\data.ms

(77) Benzidine

19.559min (+ 0.006) 221201.80 ng

response 1675892

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.00
183.00	12.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2022	BNA_M	<u>BM034377.D</u>
Compound Name	Response	Retention Time
DDT	1121940	20.794
DDD	21798	20.353
DDE	2402	19.87
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24200	1146140	2.11