

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032619\
 Data File : BM019484.D
 Acq On : 26 Mar 2019 23:32
 Operator : JU/SJ
 Sample : K2063-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB6S2

Manual Integrations
 APPROVED

Sohil
 3/27/2019 5:46:35 PM

Quant Time: Mar 27 04:42:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 27 03:30:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	174456	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	761418	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	456513	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1019892	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	993382	20.00	ng/ul	0.00
86) Perylene-d12	23.43	264	959110	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	16107	3.61	ng/uL	0.00
5) Phenol-d5	6.79	99	106607	6.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	209115	20.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	243568	20.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	177898	15.26	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	130653	24.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	155799	25.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	266111	23.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	167	0.01	ng/ul	0.04
44) Dimethylphthalate-d6	13.67	166	958455	26.02	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1153870	25.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	50417m	8.73	ng/ul	0.01
58) Fluorene-d10	15.26	176	822095	25.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	171756	25.47	ng/ul	0.00
71) Anthracene-d10	17.12	188	1416603	28.94	ng/ul	0.00
79) Pyrene-d10	19.42	212	1555456	33.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.29	264	1427006	28.07	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.73	163	60375	1.634	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032619\
Data File : BM019484.D
Acq On : 26 Mar 2019 23:32
Operator : JU/SJ
Sample : K2063-15
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DB6S2

Quant Time: Mar 27 04:42:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 27 03:30:35 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/27/2019 5:46:35 PM

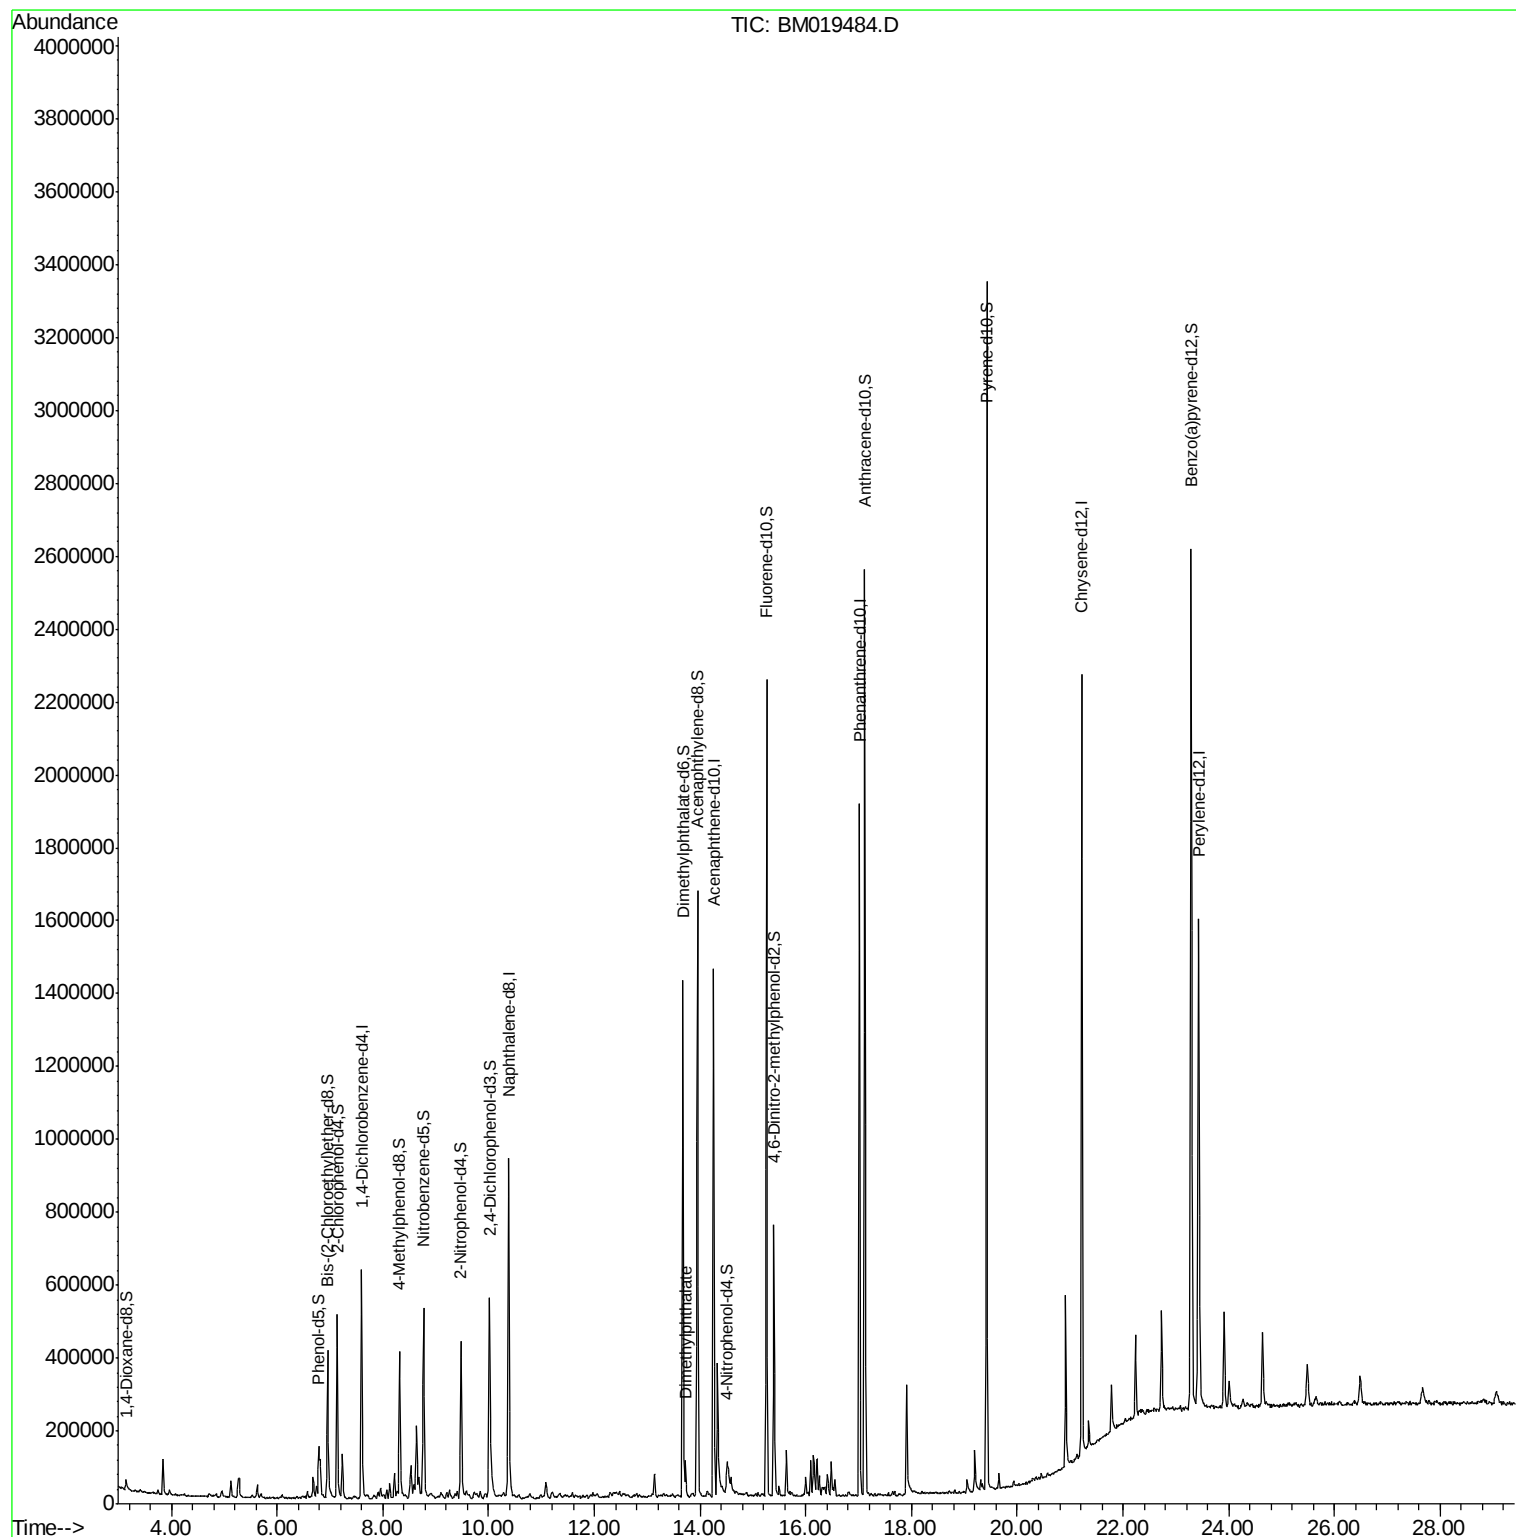

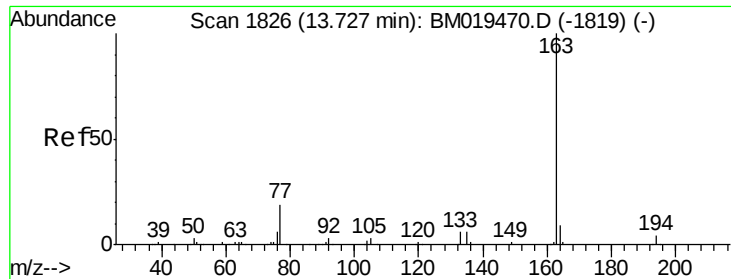

#45
 Dimethylphthalate
 Concen: 1.634 ng/ul
 RT: 13.73 min Scan# 1826
 Delta R.T. 0.00 min
 Lab File: BM019484.D
 Acq: 26 Mar 2019 23:32

Instrument :
 BNA_M
 ClientSampleId :
 DB6S2

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.2	4.0	6.0
164	11.1	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 3/27/2019 5:46:35 PM

