

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032619\
 Data File : BM019498.D
 Acq On : 27 Mar 2019 08:06
 Operator : JU/SJ
 Sample : K2031-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5S2

Quant Time: Mar 27 11:52:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 27 03:30:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	179202	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	701839	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	356216	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.03	188	701251	20.00	ng/ul	0.01
78) Chrysene-d12	21.23	240	761341	20.00	ng/ul	0.01
86) Perylene-d12	23.45	264	879970	20.00	ng/ul	0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	26916	5.88	ng/uL	0.00
5) Phenol-d5	6.79	99	265746	16.65	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.96	67	169715	15.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	220877	18.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	184127	15.37	ng/ul	0.01
19) Nitrobenzene-d5	8.77	128	101424	20.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	110019	19.74	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.02	165	184727	17.57	ng/ul	0.01
29) 4-Chloroaniline-d4	10.55	131	131457	10.41	ng/ul	0.01
44) Dimethylphthalate-d6	13.68	166	551710	19.20	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	674686	18.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	57073	12.67	ng/ul	0.02
58) Fluorene-d10	15.27	176	452232	18.26	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.42	200	15637	3.37	ng/ul	0.02
71) Anthracene-d10	17.12	188	633402	18.82	ng/ul	0.00
79) Pyrene-d10	19.43	212	629772	17.91	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.31	264	752341	16.13	ng/ul	0.02


Target Compounds				Qvalue		
6) Phenol	6.82	94	22843	1.372	ng/ul#	90
45) Dimethylphthalate	13.73	163	101786	3.530	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032619\
Data File : BM019498.D
Acq On : 27 Mar 2019 08:06
Operator : JU/SJ
Sample : K2031-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5S2

Quant Time: Mar 27 11:52:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 27 03:30:35 2019
Response via : Initial Calibration

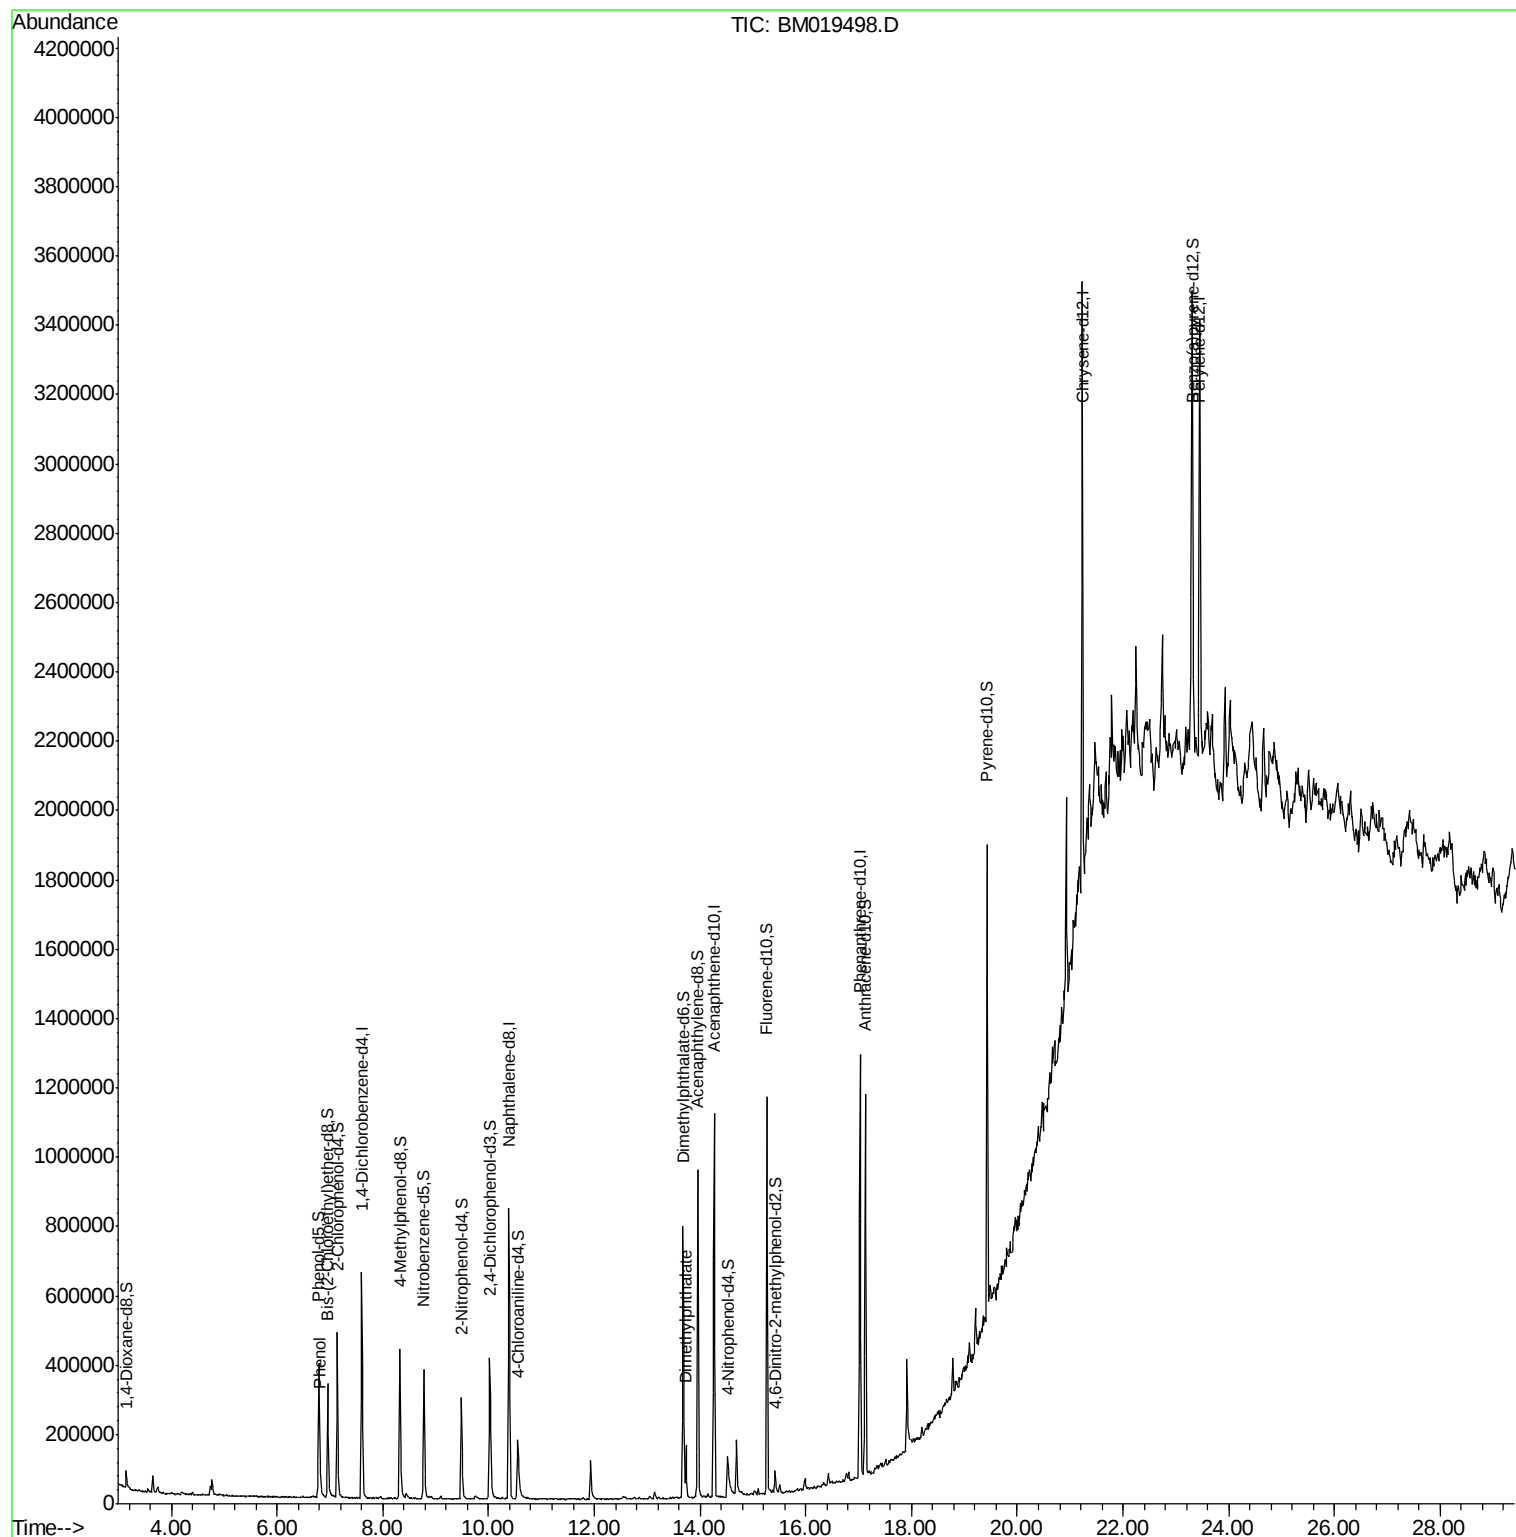

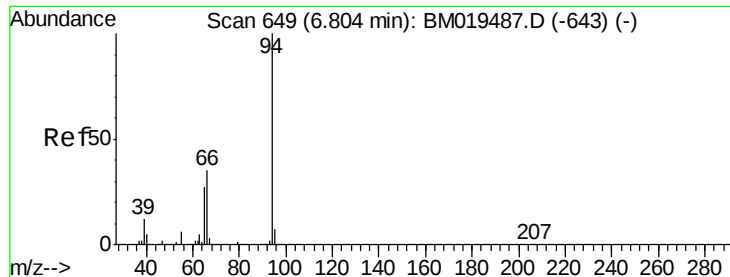





#6

Phenol

Concen: 1.372 ng/ul
 RT: 6.82 min Scan# 651
 Delta R.T. 0.01 min
 Lab File: BM019498.D
 Acq: 27 Mar 2019 08:06

Instrument :
 BNA_M
 ClientSampleId :
 BF5S2

Tgt Ion: 94 Resp: 22843
 Ion Ratio Lower Upper
 94 100
 65 31.8 23.0 34.6
 66 45.6 30.4 45.6#

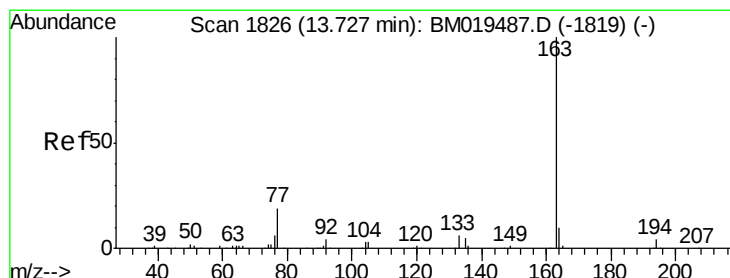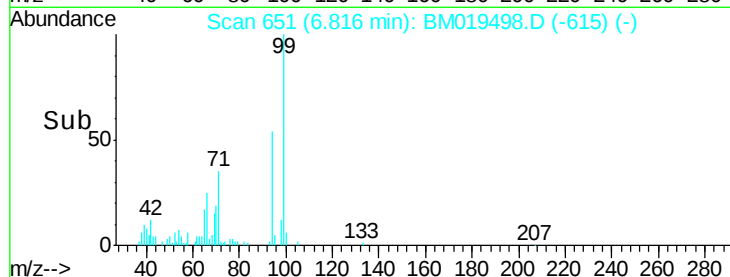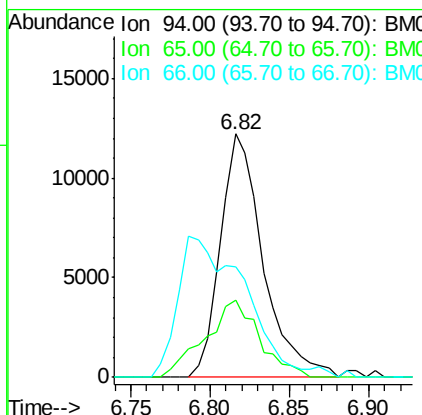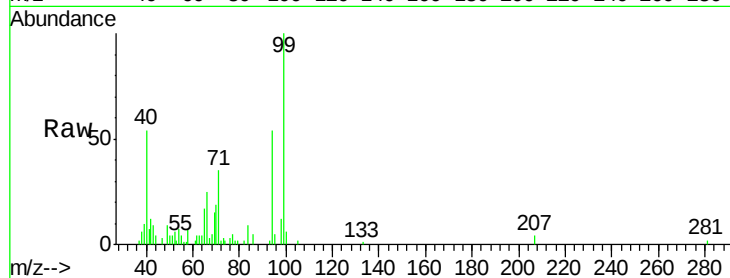

#45

Dimethylphthalate

Concen: 3.530 ng/ul
 RT: 13.73 min Scan# 1827
 Delta R.T. 0.01 min
 Lab File: BM019498.D
 Acq: 27 Mar 2019 08:06

Tgt Ion: 163 Resp: 101786
 Ion Ratio Lower Upper
 163 100
 194 4.4 4.0 6.0
 164 9.2 8.4 12.6

