

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025806.D
 Acq On : 26 Mar 2020 18:52
 Operator : CG/JU
 Sample : L1968-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DC8

Quant Time: Mar 27 00:56:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 26 18:34:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	188671	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	764950	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	474780	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1046479	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1162891	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	1315078	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	4796	1.07	ng/uL	0.00
5) Phenol-d5	6.75	99	83940	5.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	242322	28.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	282814	23.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	169197	13.83	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	180753	31.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	191750	31.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	336033	27.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	19985	1.39	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1214946	33.67	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1450227	33.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	31554	4.59	ng/ul	0.00
58) Fluorene-d10	15.20	176	1083194	34.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	166970	26.15	ng/ul	0.00
71) Anthracene-d10	17.05	188	1753573	35.88	ng/ul	0.00
79) Pyrene-d10	19.35	212	1944043	34.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2442117	36.27	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.67	163	131178	3.492	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025806.D
Acq On : 26 Mar 2020 18:52
Operator : CG/JU
Sample : L1968-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DC8

Quant Time: Mar 27 00:56:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 26 18:34:50 2020
Response via : Initial Calibration

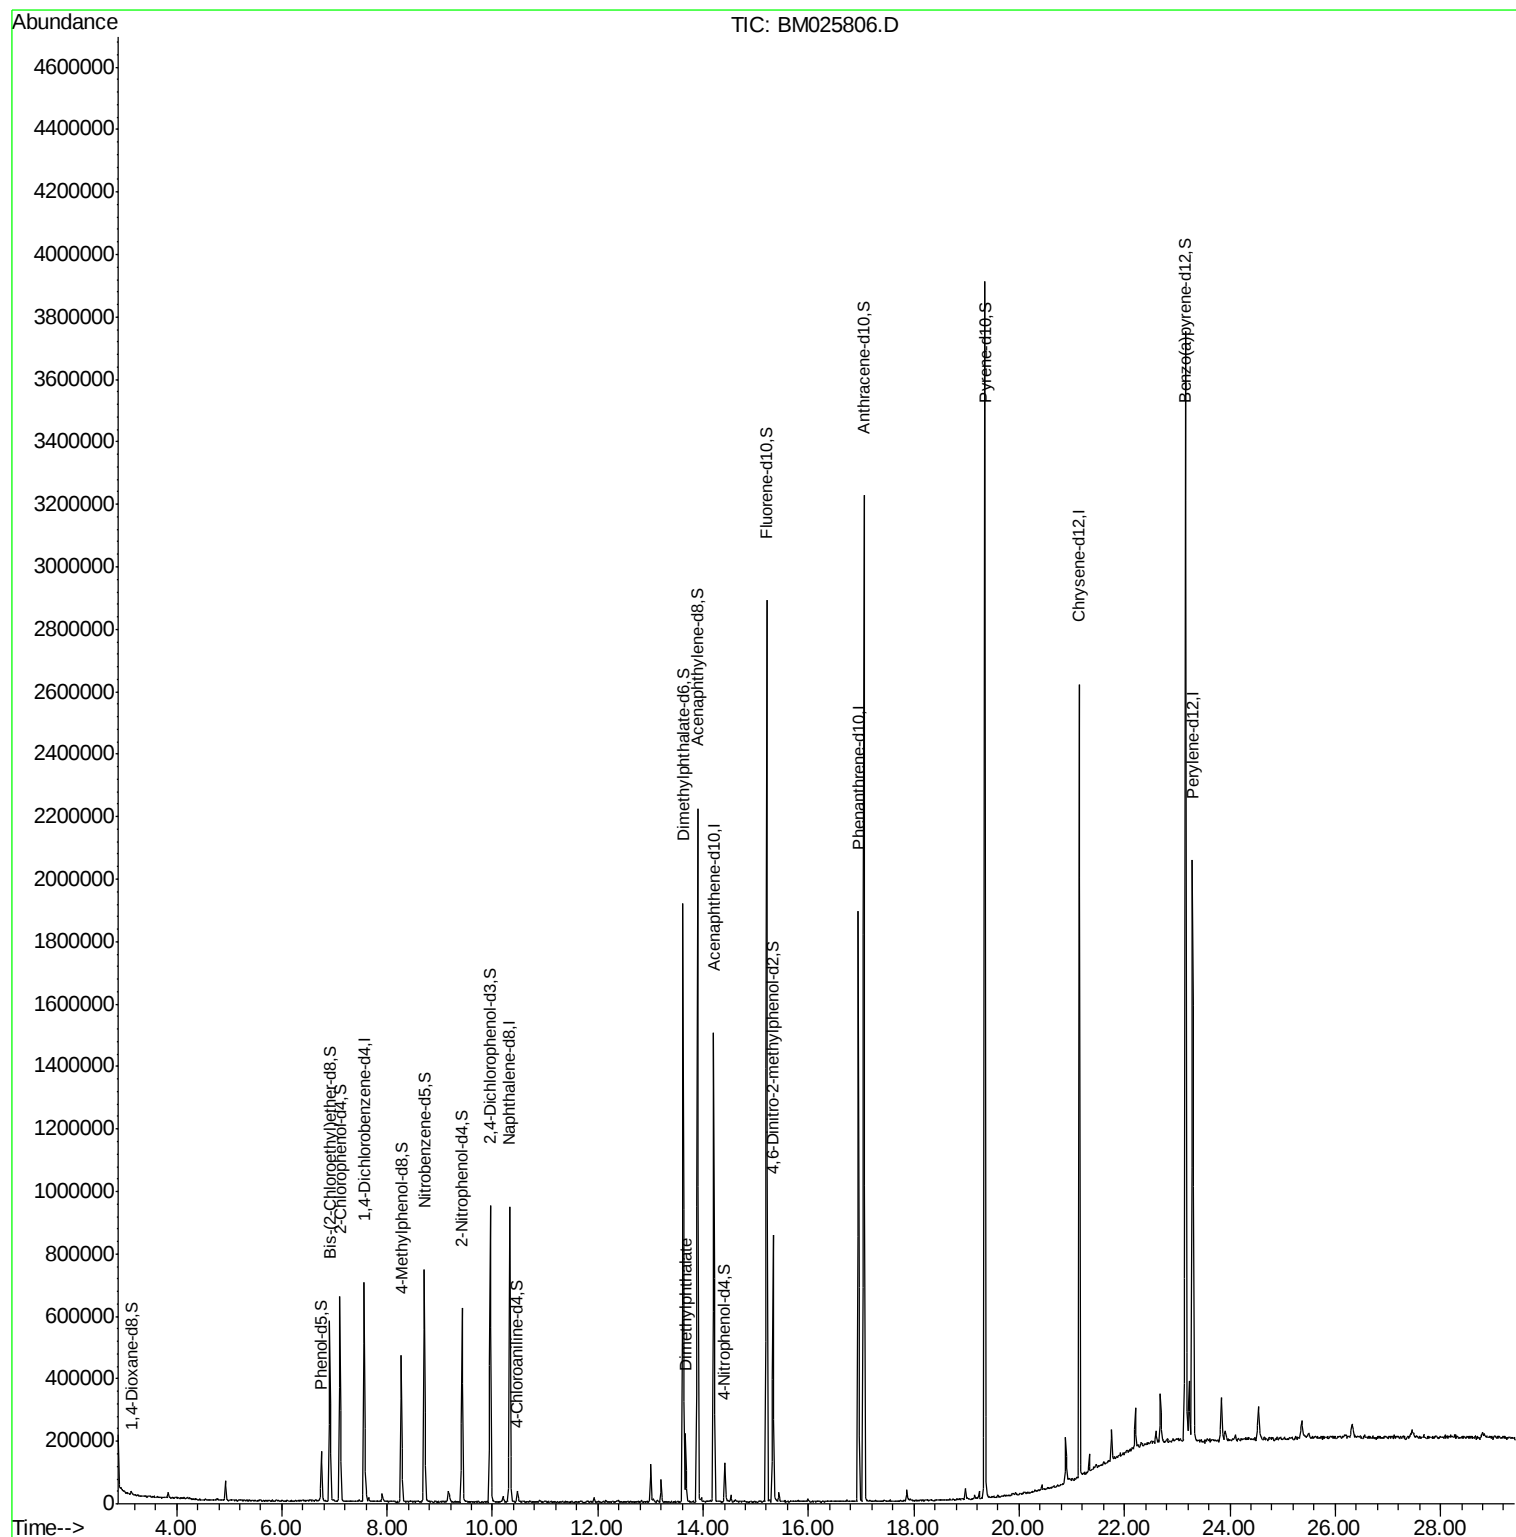

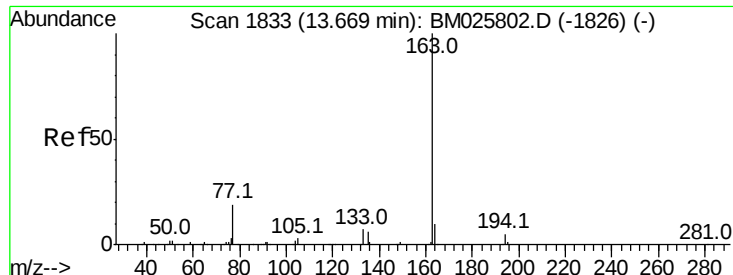

#45

Dimethylphthalate

Concen: 3.492 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM025806.D

Acq: 26 Mar 2020 18:52

Instrument :

BNA_M

ClientSampleId :

C0DC8

Tot Ion:163 Resp: 131178

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.7 8.2 12.4

