

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025814.D
 Acq On : 26 Mar 2020 23:42
 Operator : CG/JU
 Sample : L1968-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DD5

Manual Integrations
 APPROVED

mohammad
 3/30/2020 8:31:03 AM

Quant Time: Mar 27 02:05:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 27 00:56:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	190503	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	764513	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	470494	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1027018	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1138080	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	1277854	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	6324m	1.39	ng/uL	0.01
5) Phenol-d5	6.75	99	82026	5.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	241912	28.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	282418	23.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	164998	13.36	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	176561	31.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	190568	31.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	335481	27.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	16905	1.18	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1142437	31.95	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1362766	31.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	30939	4.54	ng/ul	0.00
58) Fluorene-d10	15.20	176	1048153	33.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	147639	23.56	ng/ul	0.00
71) Anthracene-d10	17.05	188	1706569	35.58	ng/ul	0.00
79) Pyrene-d10	19.35	212	1874038	34.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2358587	36.05	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	81227	2.182	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025814.D
Acq On : 26 Mar 2020 23:42
Operator : CG/JU
Sample : L1968-06
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0DD5

Manual Integrations
APPROVED

mohammad
3/30/2020 8:31:03 AM

Quant Time: Mar 27 02:05:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 27 00:56:05 2020
Response via : Initial Calibration

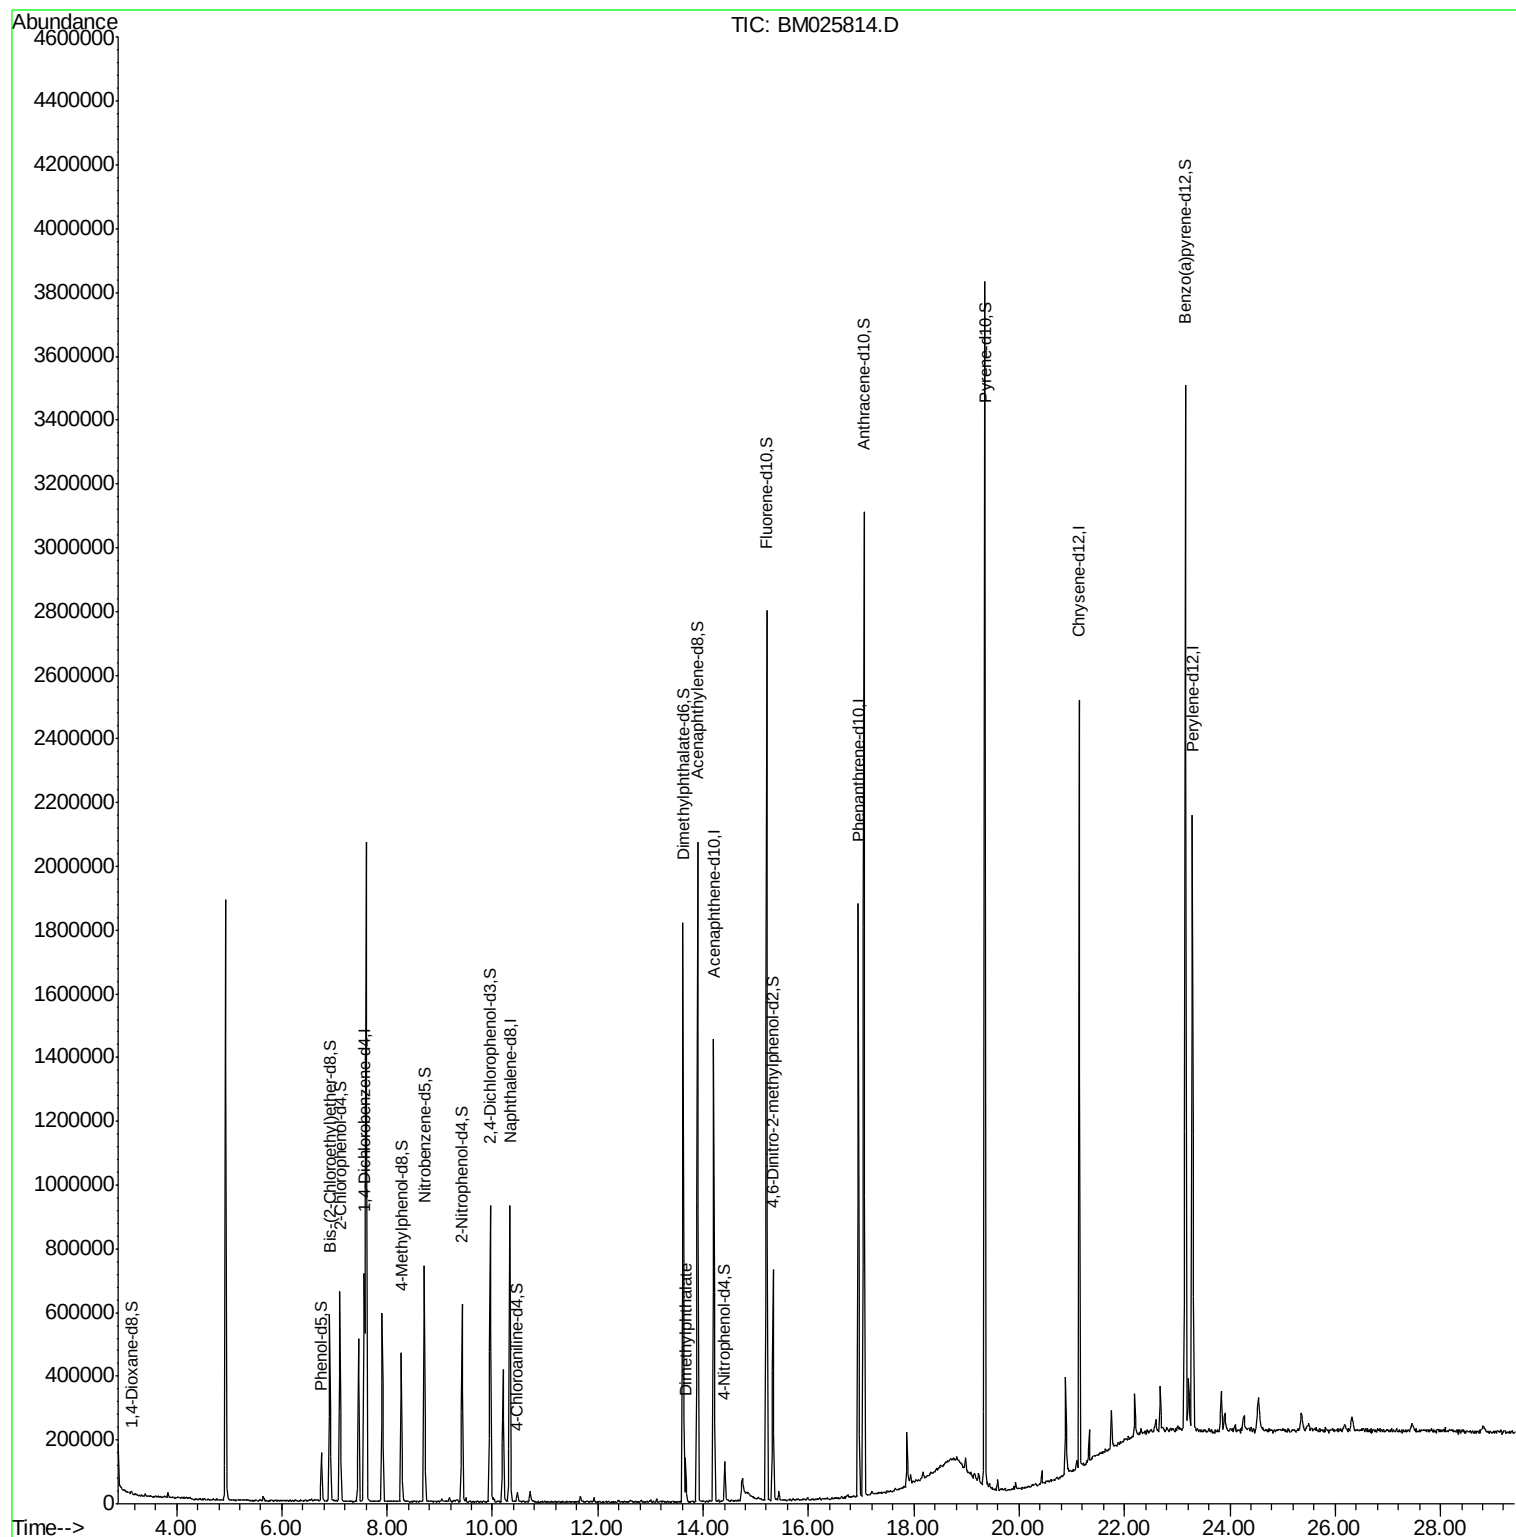

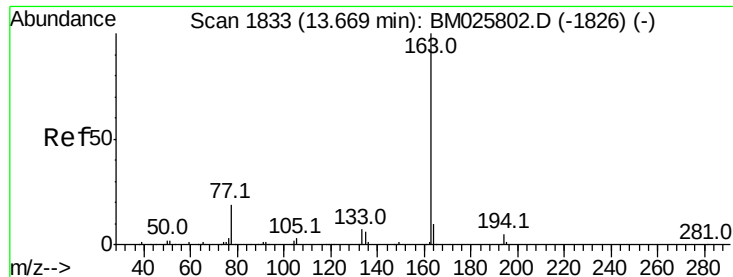

#45
 Dimethylphthalate
 Concen: 2.182 ng/ul
 RT: 13.67 min Scan# 1833
 Delta R.T. -0.00 min
 Lab File: BM025814.D
 Acq: 26 Mar 2020 23:42

Instrument :
 BNA_M
 ClientSampleId :
 C0DD5

Tot Ion:	163	Resp:	81227
Ion Ratio	Lower	Upper	
163	100		
194	4.8	3.5	5.3
164	10.0	8.2	12.4

Manual Integrations
 APPROVED

mohammad
 3/30/2020 8:31:03 AM

