

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025827.D
 Acq On : 27 Mar 2020 08:08
 Operator : CG/JU
 Sample : L2003-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0EK4

Quant Time: Mar 27 11:41:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 26 18:34:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	230938	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	958897	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	598861	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1326553	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1444183	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	1631554	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	6876	1.25	ng/uL	0.00
5) Phenol-d5	6.75	99	95723	5.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	281869	27.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	326686	22.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	190930	12.75	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	205979	28.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	221114	29.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	390456	25.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	23552	1.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1438406	31.60	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1689915	30.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	38450	4.44	ng/ul	0.00
58) Fluorene-d10	15.20	176	1320507	33.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	208017	25.70	ng/ul	0.00
71) Anthracene-d10	17.04	188	2201042	35.52	ng/ul	0.00
79) Pyrene-d10	19.34	212	2407112	34.70	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	3026301	36.23	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.67	163	126947	2.679	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025827.D
Acq On : 27 Mar 2020 08:08
Operator : CG/JU
Sample : L2003-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0EK4

Quant Time: Mar 27 11:41:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 26 18:34:50 2020
Response via : Initial Calibration

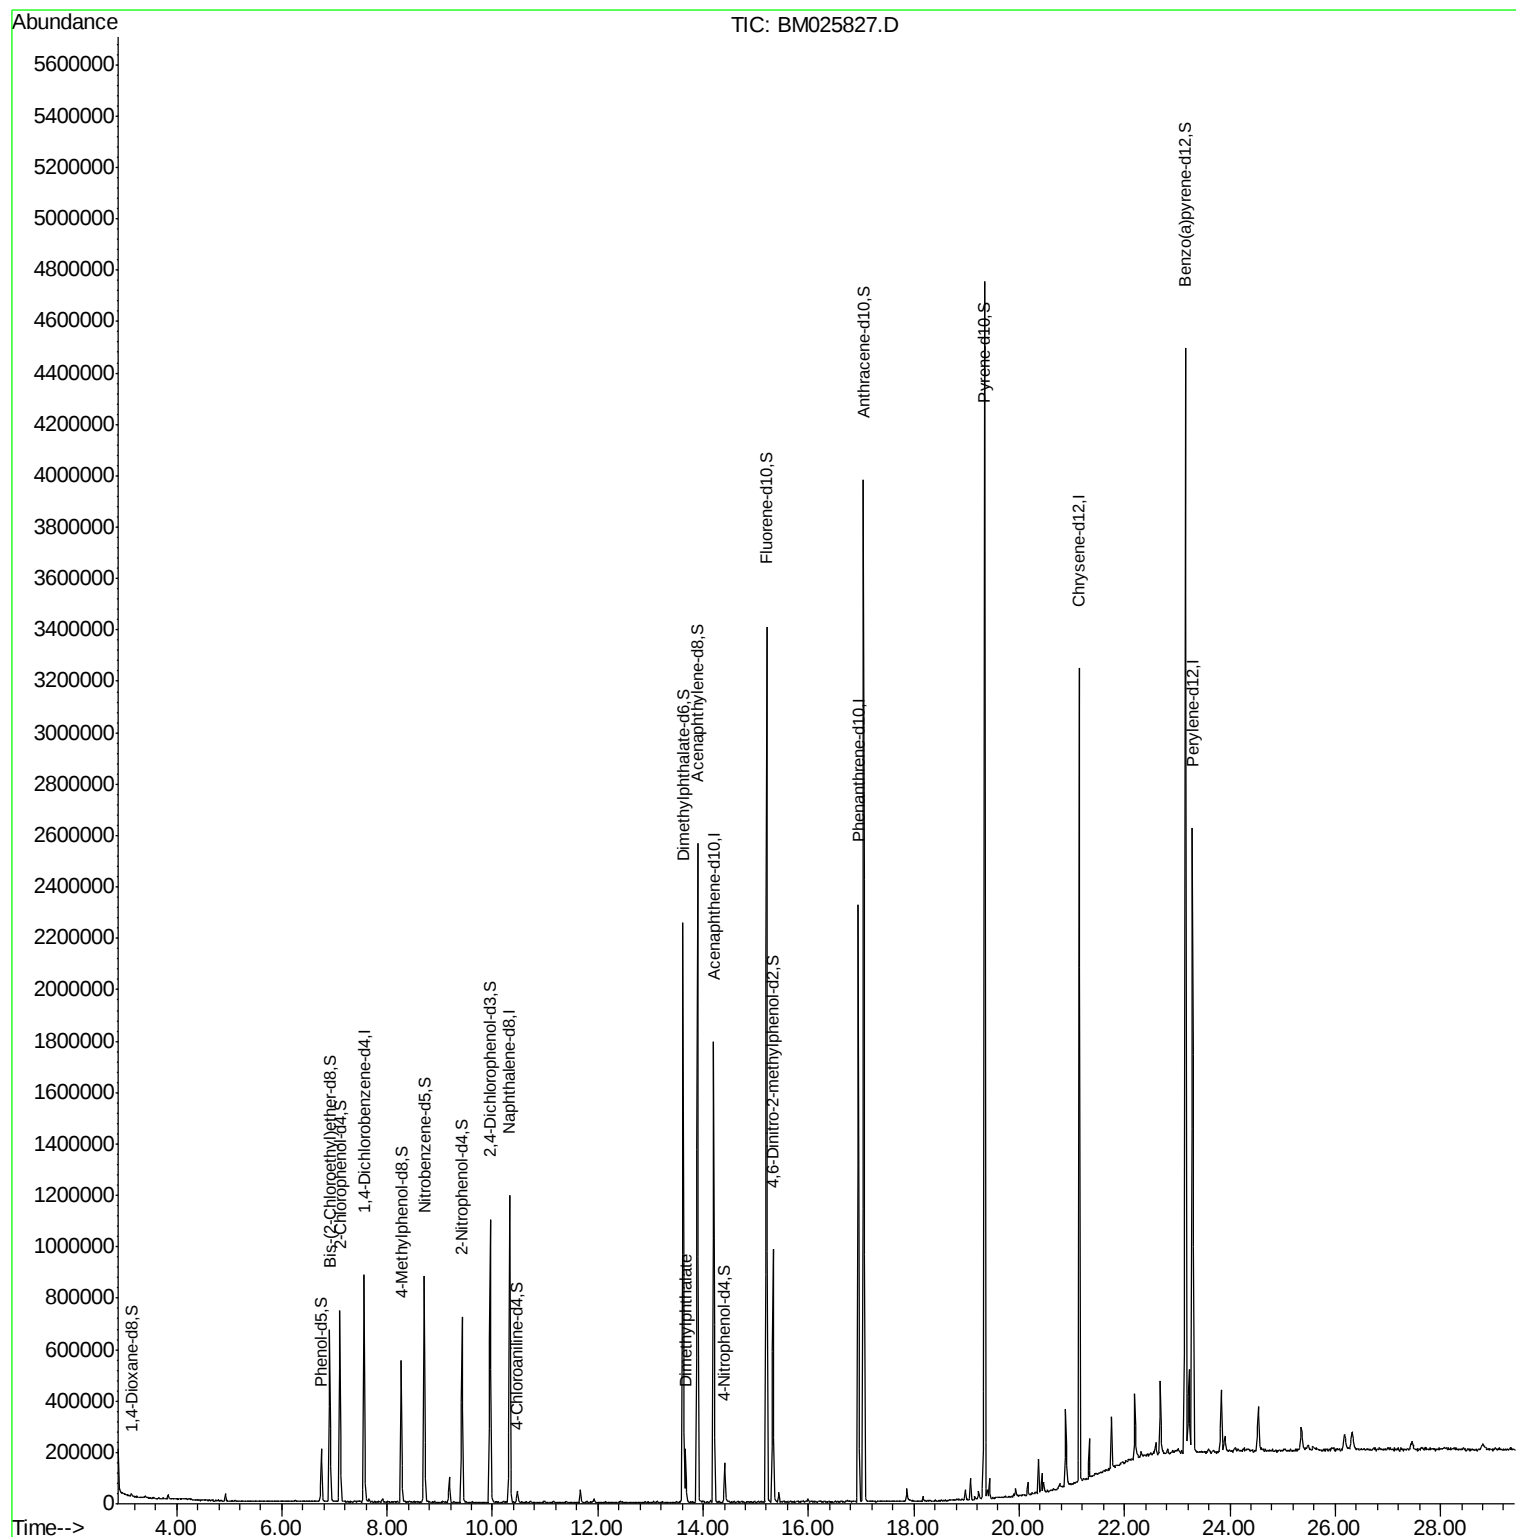

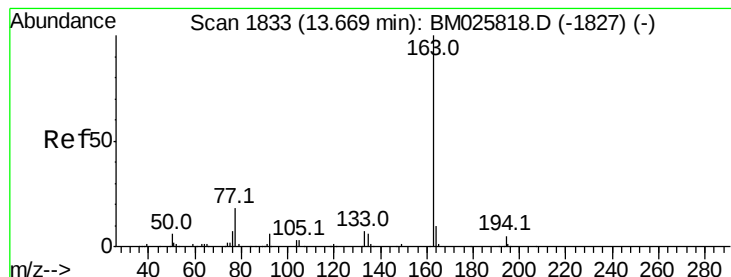

#45

Dimethylphthalate

Concen: 2.679 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM025827.D

Acq: 27 Mar 2020 08:08

Instrument :

BNA_M

ClientSampleId :

C0EK4


Tot Ion:163 Resp: 126947

Ion Ratio Lower Upper

163 100

194 3.7 3.5 5.3

164 11.0 8.2 12.4

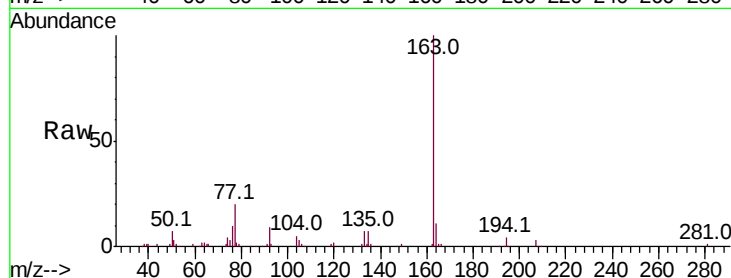

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

