

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025806.D
 Acq On : 26 Mar 2020 18:52
 Operator : CG/JU
 Sample : L1968-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	40	43	46	rBV3	11135	13085	0.22%	0.027%
2	3.699	136	138	142	rVB4	4306	6187	0.11%	0.013%
3	3.846	159	163	168	rBV	15410	19948	0.34%	0.041%
4	4.934	343	348	358	rVB	64500	96782	1.64%	0.197%
5	6.751	650	657	668	rVB	158955	249430	4.23%	0.507%
6	6.910	676	684	696	rBV	577068	879473	14.93%	1.787%
7	7.104	708	717	727	rBV	657771	1007580	17.10%	2.047%
8	7.563	789	795	806	rVV	700152	1136878	19.30%	2.310%
9	7.651	806	810	817	rVB3	12653	19279	0.33%	0.039%
10	7.910	850	854	862	rVB	25659	43820	0.74%	0.089%
11	8.269	909	915	926	rBV	467252	738681	12.54%	1.501%
12	8.710	981	990	997	rBV	741917	1220537	20.72%	2.480%
13	9.163	1061	1067	1076	rVB2	36670	84879	1.44%	0.172%
14	9.422	1105	1111	1121	rBV	621848	973786	16.53%	1.978%
15	9.957	1196	1202	1213	rBV	948203	1507074	25.58%	3.062%
16	10.198	1236	1243	1249	rVB3	18578	30183	0.51%	0.061%
17	10.328	1258	1265	1275	rVB	943759	1535403	26.06%	3.119%
18	10.475	1283	1290	1298	rBV2	37219	65712	1.12%	0.133%
19	10.716	1328	1331	1335	rVB5	5007	6623	0.11%	0.013%
20	10.892	1357	1361	1365	rBV5	5168	6661	0.11%	0.014%
21	11.927	1533	1537	1543	rBV2	14096	23602	0.40%	0.048%
22	12.386	1611	1615	1624	rVB4	6208	11096	0.19%	0.023%
23	12.822	1685	1689	1697	rVB4	6960	8228	0.14%	0.017%
24	13.010	1715	1721	1726	rBV3	122162	195014	3.31%	0.396%
25	13.057	1726	1729	1736	rVB6	10882	18560	0.32%	0.038%
26	13.133	1736	1742	1747	rBV5	5341	10640	0.18%	0.022%
27	13.204	1749	1754	1761	rVB	71691	106699	1.81%	0.217%
28	13.621	1816	1825	1830	rBV	1918163	2563940	43.52%	5.209%
29	13.669	1830	1833	1839	rVB	219882	295832	5.02%	0.601%
30	13.892	1864	1871	1879	rBV	2220235	3084247	52.35%	6.266%
31	13.963	1879	1883	1889	rVB6	15786	23836	0.40%	0.048%
32	14.139	1910	1913	1916	rVV2	5786	6996	0.12%	0.014%
33	14.204	1918	1924	1932	rVB	1499961	2093776	35.54%	4.254%
34	14.410	1954	1959	1967	rBV	125826	202333	3.43%	0.411%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025806.D
 Acq On : 26 Mar 2020 18:52
 Operator : CG/JU
 Sample : L1968-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	14.533	1975	1980	1983	rVB	22421	28134	0.48%	0.057%
36	15.104	2071	2077	2079	rVB5	3453	6442	0.11%	0.013%
37	15.204	2087	2094	2100	rBV	2885243	3910250	66.37%	7.944%
38	15.257	2100	2103	2107	rVB4	8157	12440	0.21%	0.025%
39	15.327	2109	2115	2123	rBV	850467	1104057	18.74%	2.243%
40	15.445	2130	2135	2139	rVB2	28401	38912	0.66%	0.079%
41	15.992	2225	2228	2233	rVB3	8716	10602	0.18%	0.022%
42	16.733	2350	2354	2357	rBV3	6945	10735	0.18%	0.022%
43	16.951	2385	2391	2401	rVB	1890857	2515031	42.69%	5.110%
44	17.051	2401	2408	2419	rBV	3222276	4434050	75.26%	9.008%
45	17.874	2544	2548	2555	rBV2	36098	44100	0.75%	0.090%
46	18.980	2732	2736	2740	rBV	34089	45167	0.77%	0.092%
47	19.162	2763	2767	2769	rBV4	11273	11695	0.20%	0.024%
48	19.239	2776	2780	2783	rVB2	24455	29854	0.51%	0.061%
49	19.351	2791	2799	2805	rBV	3896767	5219730	88.60%	10.604%
50	19.427	2811	2812	2819	rVB6	6217	9071	0.15%	0.018%
51	19.939	2896	2899	2901	rBV2	7648	6655	0.11%	0.014%
52	20.186	2937	2941	2943	rBV5	6912	11328	0.19%	0.023%
53	20.433	2981	2983	2986	rVB4	14332	12724	0.22%	0.026%
54	20.886	3056	3060	3066	rBV2	140274	193884	3.29%	0.394%
55	21.145	3099	3104	3111	rBV	2532288	3033613	51.49%	6.163%
56	21.333	3133	3136	3139	rBV2	56451	56315	0.96%	0.114%
57	21.756	3205	3208	3215	rVB2	96838	117618	2.00%	0.239%
58	22.203	3280	3284	3290	rBV	125178	157164	2.67%	0.319%
59	22.686	3363	3366	3371	rVB	148202	200841	3.41%	0.408%
60	23.162	3440	3447	3454	rBV	3540516	5891623	100.00%	11.969%
61	23.227	3454	3458	3463	rVV	184778	265716	4.51%	0.540%
62	23.291	3463	3469	3480	rVB	1855637	3315730	56.28%	6.736%
63	23.838	3558	3562	3569	rVB3	138178	242233	4.11%	0.492%


Sum of corrected areas: 49222514

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025806.D
Acq On : 26 Mar 2020 18:52
Operator : CG/JU
Sample : L1968-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DC8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

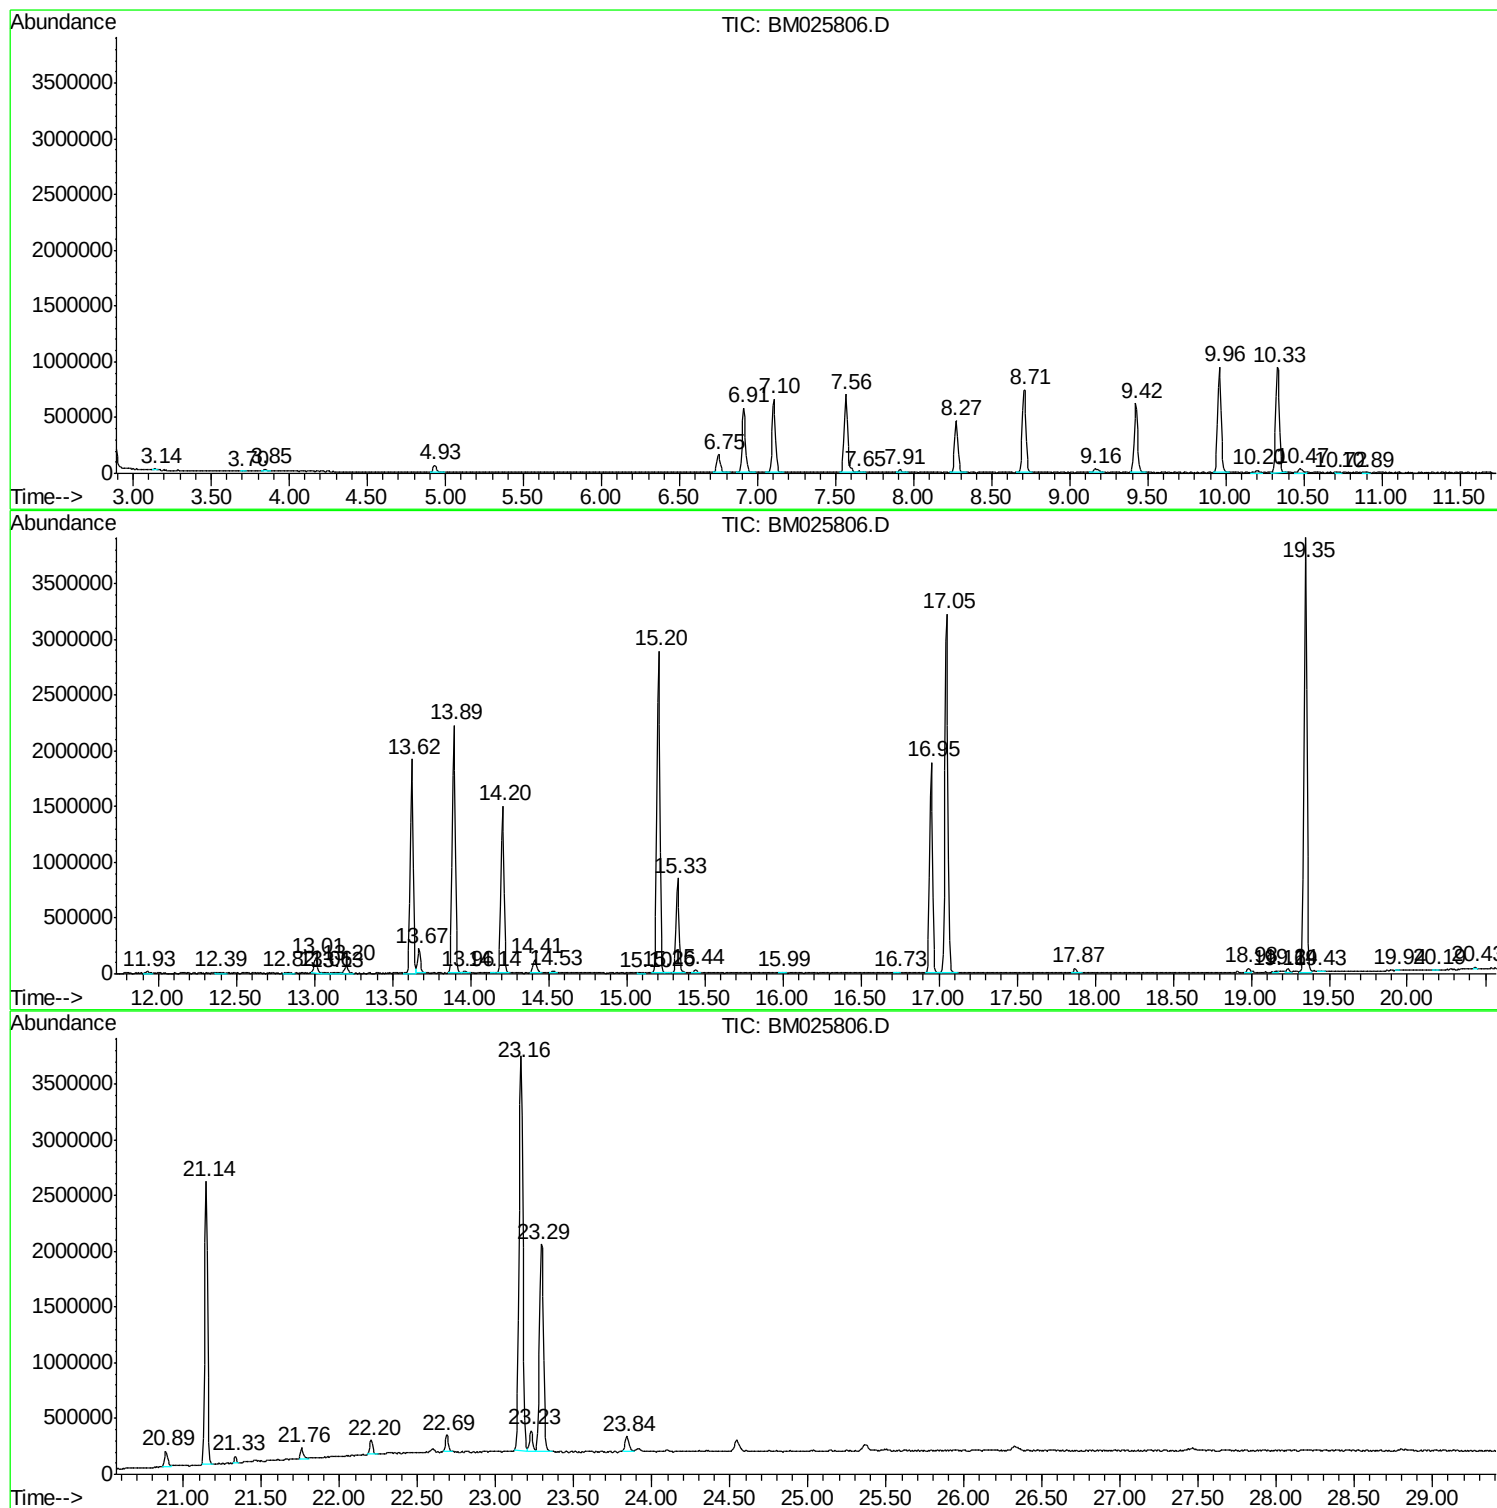

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025806.D
Acq On : 26 Mar 2020 18:52
Operator : CG/JU
Sample : L1968-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DC8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025806.D
Acq On : 26 Mar 2020 18:52
Operator : CG/JU
Sample : L1968-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DC8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc