

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025822.D
 Acq On : 27 Mar 2020 05:08
 Operator : CG/JU
 Sample : PB127838BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	39	42	48	rBV	43346	56762	1.17%	0.120%
2	3.846	159	163	166	rBV2	14269	18372	0.38%	0.039%
3	4.934	343	348	357	rVB	56089	88785	1.83%	0.188%
4	6.746	650	656	671	rVB	735220	1142030	23.51%	2.417%
5	6.910	677	684	695	rVB	560846	859414	17.69%	1.819%
6	7.104	710	717	724	rVB	768227	1195707	24.61%	2.531%
7	7.469	772	779	780	rBV6	2940	5465	0.11%	0.012%
8	7.563	789	795	808	rVB	643790	1010175	20.79%	2.138%
9	7.910	849	854	860	rVB2	28101	47734	0.98%	0.101%
10	8.269	909	915	925	rBV	931601	1433238	29.50%	3.034%
11	8.704	982	989	996	rBV	702529	1126497	23.19%	2.385%
12	9.422	1105	1111	1120	rBV	578117	900423	18.53%	1.906%
13	9.957	1195	1202	1212	rBV	971024	1495958	30.79%	3.167%
14	10.192	1238	1242	1249	rVB4	7794	13490	0.28%	0.029%
15	10.328	1259	1265	1274	rVB	857456	1372688	28.26%	2.906%
16	10.469	1281	1289	1298	rBV	933468	1549062	31.89%	3.279%
17	10.716	1326	1331	1334	rVB4	3693	5464	0.11%	0.012%
18	11.928	1532	1537	1542	rBV	13233	20948	0.43%	0.044%
19	13.622	1819	1825	1833	rBV	1750996	2248670	46.29%	4.760%
20	13.892	1863	1871	1879	rBV	2012645	2794450	57.52%	5.915%
21	14.204	1917	1924	1931	rBV	1305529	1875742	38.61%	3.971%
22	14.410	1952	1959	1972	rBV	726111	1045814	21.53%	2.214%
23	15.204	2087	2094	2100	rBV	2528135	3470616	71.44%	7.346%
24	15.327	2109	2115	2125	rBV	660322	909712	18.73%	1.926%
25	15.439	2129	2134	2140	rVB	25238	36163	0.74%	0.077%
26	15.986	2223	2227	2232	rVB4	7459	10777	0.22%	0.023%
27	16.739	2349	2355	2359	rBV4	6125	11083	0.23%	0.023%
28	16.951	2385	2391	2399	rBV	1693050	2260133	46.52%	4.784%
29	17.045	2401	2407	2415	rBV	2685838	3755113	77.30%	7.949%
30	17.327	2450	2455	2460	rVB5	3032	7016	0.14%	0.015%
31	18.174	2597	2599	2607	rBV8	6148	11927	0.25%	0.025%
32	18.374	2632	2633	2637	rBV4	4399	5091	0.10%	0.011%
33	18.980	2732	2736	2740	rVB2	23409	29641	0.61%	0.063%
34	19.074	2747	2752	2757	rBV2	45331	53189	1.09%	0.113%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025822.D
 Acq On : 27 Mar 2020 05:08
 Operator : CG/JU
 Sample : PB127838BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	19.233	2775	2779	2784	rVB	21894	30533	0.63%	0.065%
36	19.345	2789	2798	2804	rVV	3359650	4464544	91.90%	9.450%
37	19.398	2804	2807	2810	rVV4	17239	23481	0.48%	0.050%
38	19.433	2810	2813	2818	rVB2	42728	47046	0.97%	0.100%
39	19.939	2895	2899	2904	rBV4	13407	18262	0.38%	0.039%
40	20.156	2933	2936	2940	rBV3	22556	28782	0.59%	0.061%
41	20.362	2968	2971	2977	rBV2	65450	73598	1.51%	0.156%
42	20.433	2979	2983	2986	rVV	35416	40048	0.82%	0.085%
43	20.462	2986	2988	2993	rVB5	18350	20847	0.43%	0.044%
44	20.892	3059	3061	3064	rVB2	28771	24517	0.50%	0.052%
45	21.139	3098	3103	3112	rBV	2169336	2693237	55.44%	5.701%
46	21.333	3132	3136	3139	rBV	49388	51324	1.06%	0.109%
47	21.750	3205	3207	3211	rVB2	56820	55595	1.14%	0.118%
48	22.198	3280	3283	3288	rVB	108979	122870	2.53%	0.260%
49	22.686	3362	3366	3372	rVB	133215	186762	3.84%	0.395%
50	23.156	3439	3446	3453	rBV	2931457	4858099	100.00%	10.283%
51	23.221	3453	3457	3462	rVV	168876	270749	5.57%	0.573%
52	23.292	3462	3469	3478	rVB	1652247	2882790	59.34%	6.102%
53	23.833	3557	3561	3569	rVB	140301	251884	5.18%	0.533%
54	24.539	3676	3681	3687	rVB2	126795	229585	4.73%	0.486%


Sum of corrected areas: 47241902

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025822.D
Acq On : 27 Mar 2020 05:08
Operator : CG/JU
Sample : PB127838BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

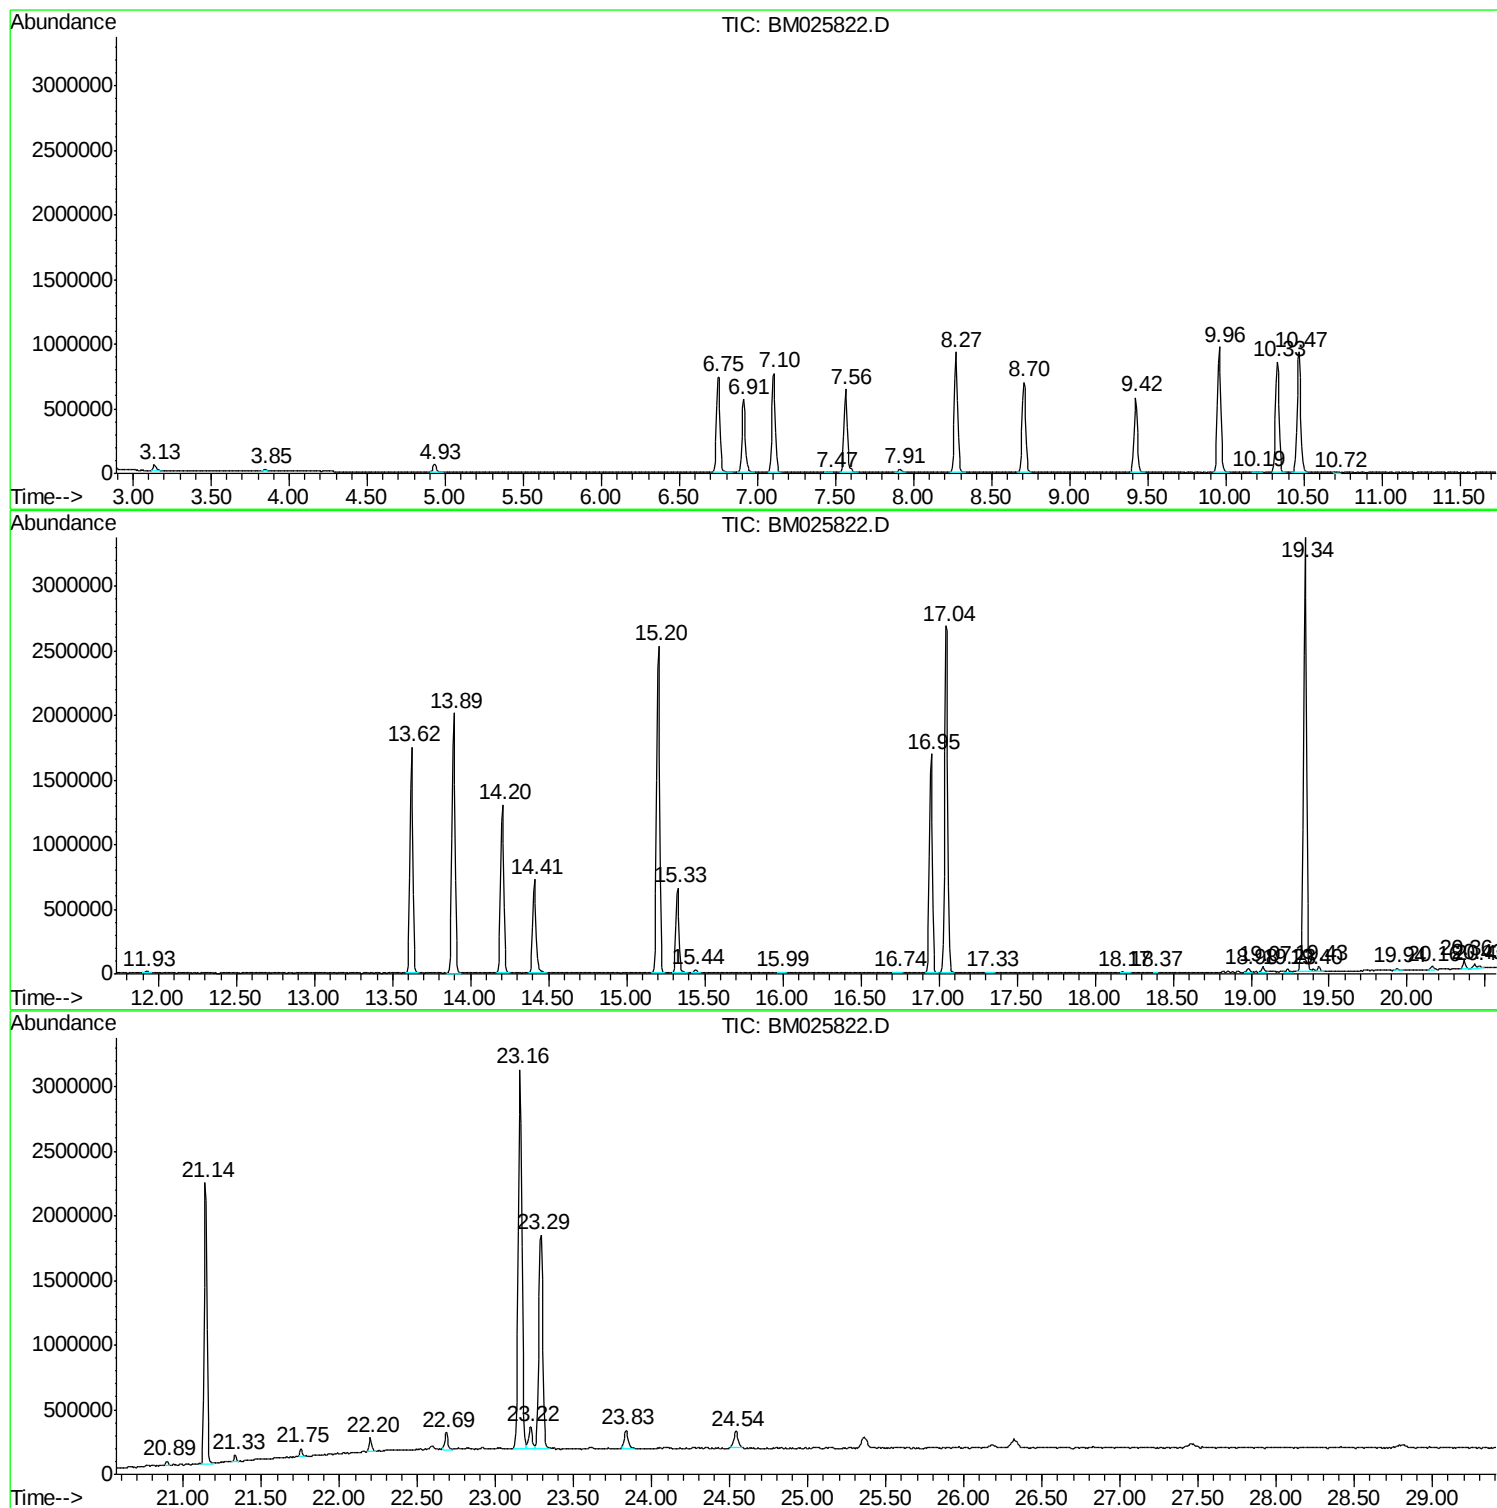

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025822.D
Acq On : 27 Mar 2020 05:08
Operator : CG/JU
Sample : PB127838BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025822.D
Acq On : 27 Mar 2020 05:08
Operator : CG/JU
Sample : PB127838BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc