

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025823.D
 Acq On : 27 Mar 2020 05:44
 Operator : CG/JU
 Sample : PB127721BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	39	42	56	rVB	48994	72640	1.46%	0.151%
2	3.846	159	163	166	rBV	14214	18094	0.36%	0.038%
3	4.069	198	201	204	rBV3	3272	5720	0.11%	0.012%
4	4.934	343	348	356	rVB	96954	137299	2.75%	0.286%
5	6.745	649	656	665	rBV	765198	1165906	23.36%	2.431%
6	6.910	677	684	700	rVB	580974	886068	17.75%	1.848%
7	7.104	710	717	726	rBV	807422	1228608	24.61%	2.562%
8	7.457	773	777	780	rVB6	6091	8338	0.17%	0.017%
9	7.563	789	795	808	rVB	650114	1057972	21.19%	2.206%
10	7.910	847	854	861	rVB2	42011	68915	1.38%	0.144%
11	8.269	909	915	928	rBV	951107	1470346	29.45%	3.066%
12	8.704	983	989	1000	rBV	722039	1152908	23.09%	2.404%
13	9.422	1105	1111	1120	rBV	584135	925012	18.53%	1.929%
14	9.957	1195	1202	1216	rBV	973299	1528632	30.62%	3.188%
15	10.198	1239	1243	1247	rVB4	11857	17017	0.34%	0.035%
16	10.327	1258	1265	1274	rBV	874734	1399575	28.04%	2.919%
17	10.469	1281	1289	1300	rBV	943607	1582677	31.70%	3.301%
18	11.933	1532	1538	1543	rVB	14873	25864	0.52%	0.054%
19	13.621	1819	1825	1833	rBV	1749372	2304028	46.15%	4.805%
20	13.692	1833	1837	1841	rVB5	3791	6235	0.12%	0.013%
21	13.892	1864	1871	1882	rBV	2005851	2847733	57.05%	5.939%
22	14.204	1917	1924	1932	rBV	1328290	1904983	38.16%	3.973%
23	14.286	1934	1938	1942	rVB5	2650	5641	0.11%	0.012%
24	14.410	1952	1959	1970	rBV	743224	1066844	21.37%	2.225%
25	15.204	2087	2094	2101	rBV	2545568	3569259	71.50%	7.443%
26	15.321	2109	2114	2125	rBV	677616	924556	18.52%	1.928%
27	15.439	2130	2134	2141	rVB2	24387	34815	0.70%	0.073%
28	15.986	2224	2227	2233	rVB5	8536	11800	0.24%	0.025%
29	16.627	2334	2336	2341	rBV5	3904	5734	0.11%	0.012%
30	16.739	2352	2355	2360	rVB2	6419	8503	0.17%	0.018%
31	16.951	2384	2391	2397	rBV	1675701	2295704	45.99%	4.788%
32	17.045	2401	2407	2417	rBV	2803138	3844173	77.01%	8.017%
33	18.980	2733	2736	2743	rVB	27279	33678	0.67%	0.070%
34	19.074	2748	2752	2756	rBV3	16323	20985	0.42%	0.044%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025823.D
 Acq On : 27 Mar 2020 05:44
 Operator : CG/JU
 Sample : PB127721BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	19.233	2775	2779	2782	rVB	24129	28131	0.56%	0.059%
36	19.345	2789	2798	2805	rBV	3339614	4467983	89.50%	9.318%
37	19.392	2805	2806	2810	rVV4	8286	9516	0.19%	0.020%
38	19.433	2810	2813	2816	rVV4	14196	16783	0.34%	0.035%
39	19.933	2896	2898	2902	rBV4	5095	6402	0.13%	0.013%
40	20.162	2933	2937	2941	rBV6	12822	22078	0.44%	0.046%
41	20.368	2968	2972	2974	rBV2	25584	28299	0.57%	0.059%
42	20.433	2980	2983	2986	rVB5	12660	14004	0.28%	0.029%
43	20.468	2987	2989	2991	rVB2	11503	8779	0.18%	0.018%
44	20.897	3059	3062	3065	rBV4	18255	22273	0.45%	0.046%
45	21.139	3098	3103	3111	rBV	2229545	2791938	55.93%	5.822%
46	21.333	3133	3136	3139	rVB3	28412	26143	0.52%	0.055%
47	21.756	3205	3208	3214	rVB3	38959	43738	0.88%	0.091%
48	22.197	3280	3283	3288	rVB2	69822	87714	1.76%	0.183%
49	22.685	3362	3366	3370	rVB2	92345	125494	2.51%	0.262%
50	23.156	3439	3446	3453	rBV	2981541	4992042	100.00%	10.411%
51	23.221	3453	3457	3462	rVV	138750	220162	4.41%	0.459%
52	23.291	3462	3469	3478	rVB	1776749	2997473	60.05%	6.251%
53	23.838	3557	3562	3567	rVB	113946	196081	3.93%	0.409%
54	24.538	3677	3681	3688	rVB3	104848	210522	4.22%	0.439%


Sum of corrected areas: 47951817

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025823.D
Acq On : 27 Mar 2020 05:44
Operator : CG/JU
Sample : PB127721BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

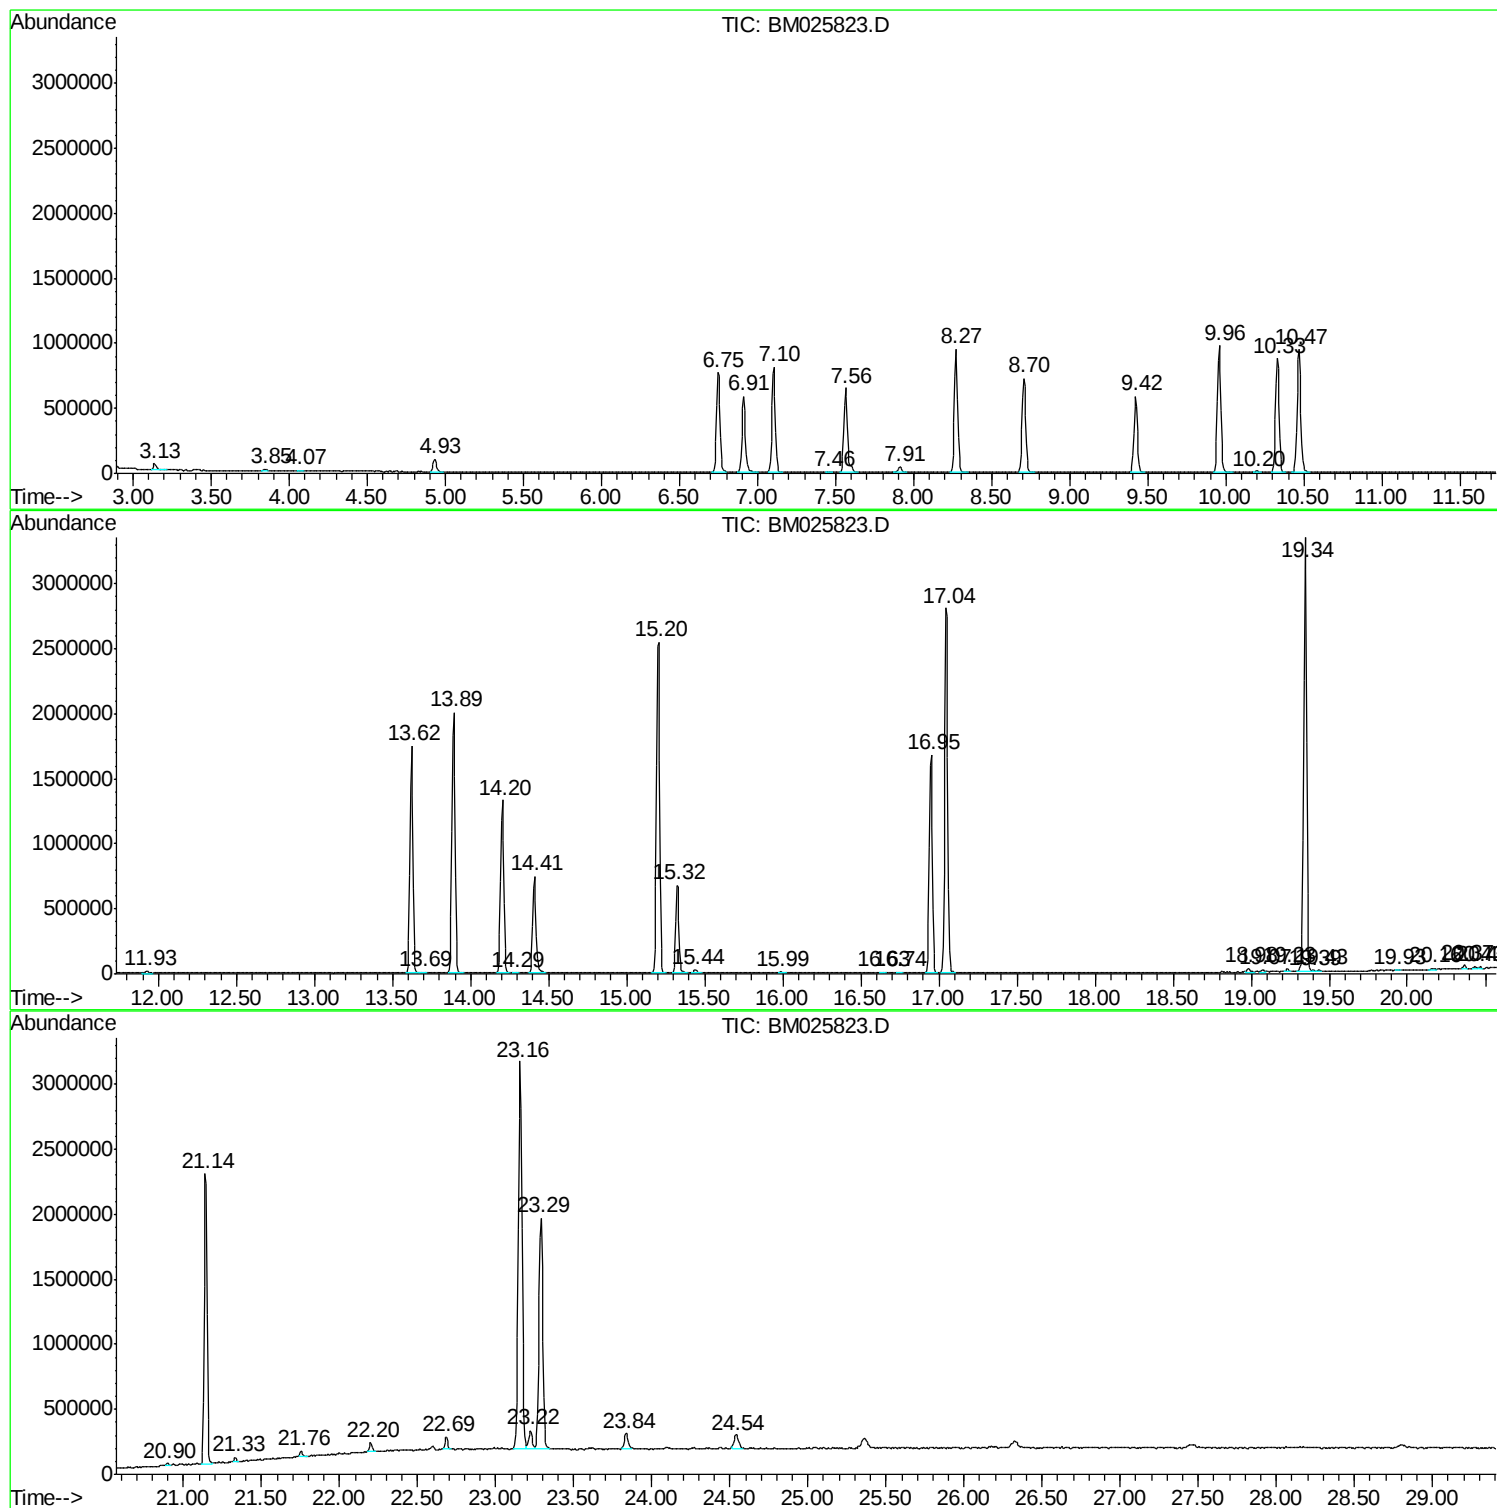

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025823.D
Acq On : 27 Mar 2020 05:44
Operator : CG/JU
Sample : PB127721BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025823.D
Acq On : 27 Mar 2020 05:44
Operator : CG/JU
Sample : PB127721BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc