

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025824.D
 Acq On : 27 Mar 2020 06:20
 Operator : CG/JU
 Sample : PB127720BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	39	42	50	rVB	51195	69201	1.19%	0.126%
2	3.846	159	163	168	rBV	15030	19419	0.34%	0.035%
3	4.934	341	348	356	rBV	194832	292724	5.05%	0.534%
4	6.746	651	656	668	rVB	821183	1273365	21.97%	2.323%
5	6.910	676	684	692	rBV	645728	963009	16.62%	1.757%
6	7.104	710	717	725	rBV	850464	1321931	22.81%	2.411%
7	7.457	771	777	781	rVB2	11058	17142	0.30%	0.031%
8	7.563	788	795	800	rBV	716344	1146470	19.78%	2.091%
9	7.910	846	854	861	rVB	96030	148851	2.57%	0.272%
10	8.269	909	915	926	rBV	1046320	1613800	27.85%	2.944%
11	8.704	981	989	997	rBV	809937	1276371	22.02%	2.328%
12	9.422	1105	1111	1118	rBV	664216	1018729	17.58%	1.858%
13	9.957	1194	1202	1210	rBV	1059948	1695222	29.25%	3.092%
14	10.198	1238	1243	1248	rBV2	30141	45218	0.78%	0.082%
15	10.328	1257	1265	1273	rBV	957406	1550272	26.75%	2.828%
16	10.469	1282	1289	1300	rBV	1056568	1757270	30.32%	3.205%
17	10.716	1327	1331	1336	rVB4	9958	13571	0.23%	0.025%
18	11.928	1532	1537	1544	rBV2	13886	23662	0.41%	0.043%
19	13.622	1819	1825	1832	rBV	1964835	2577168	44.47%	4.701%
20	13.892	1864	1871	1880	rBV	2283354	3149890	54.35%	5.746%
21	14.204	1917	1924	1933	rVB	1513810	2143264	36.98%	3.910%
22	14.410	1952	1959	1969	rBV	868939	1232864	21.27%	2.249%
23	14.939	2045	2049	2053	rBV4	3012	5954	0.10%	0.011%
24	15.204	2087	2094	2100	rBV	2828730	3978557	68.65%	7.257%
25	15.327	2109	2115	2127	rVV	796803	1086286	18.74%	1.982%
26	15.439	2130	2134	2139	rVB2	27271	37882	0.65%	0.069%
27	15.992	2221	2228	2232	rBV5	8507	14799	0.26%	0.027%
28	16.739	2351	2355	2358	rBV3	6213	9499	0.16%	0.017%
29	16.951	2384	2391	2397	rBV	1890605	2632204	45.42%	4.801%
30	17.045	2401	2407	2419	rVV	3175605	4348018	75.02%	7.931%
31	18.980	2732	2736	2742	rVB2	30586	37594	0.65%	0.069%
32	19.074	2749	2752	2757	rVB3	31871	33847	0.58%	0.062%
33	19.233	2773	2779	2783	rBV2	25494	34176	0.59%	0.062%
34	19.345	2789	2798	2805	rBV	3888958	5169195	89.19%	9.429%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025824.D
 Acq On : 27 Mar 2020 06:20
 Operator : CG/JU
 Sample : PB127720BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	19.398	2805	2807	2810	rVV4	13773	16883	0.29%	0.031%
36	19.433	2810	2813	2816	rVB3	33482	35458	0.61%	0.065%
37	19.933	2896	2898	2902	rBV3	9612	11148	0.19%	0.020%
38	20.157	2933	2936	2941	rBV4	19062	28495	0.49%	0.052%
39	20.362	2968	2971	2975	rBV2	43747	47075	0.81%	0.086%
40	20.433	2980	2983	2985	rVV	22714	22689	0.39%	0.041%
41	20.462	2985	2988	2992	rVV5	15870	16682	0.29%	0.030%
42	20.892	3059	3061	3065	rBV2	24711	24017	0.41%	0.044%
43	21.139	3098	3103	3109	rBV	2686360	3265610	56.35%	5.957%
44	21.333	3133	3136	3138	rBV3	43852	42672	0.74%	0.078%
45	21.751	3204	3207	3211	rBV3	62112	74354	1.28%	0.136%
46	22.198	3279	3283	3287	rBV	102685	126420	2.18%	0.231%
47	22.686	3362	3366	3370	rVB2	131185	170654	2.94%	0.311%
48	23.156	3439	3446	3453	rBV	3394412	5795608	100.00%	10.572%
49	23.221	3453	3457	3462	rVV	197727	320900	5.54%	0.585%
50	23.292	3462	3469	3478	rVB	2016775	3476630	59.99%	6.342%
51	23.833	3557	3561	3570	rVB	173301	294722	5.09%	0.538%
52	24.539	3677	3681	3691	rVB2	160610	313569	5.41%	0.572%


Sum of corrected areas: 54821010

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025824.D
Acq On : 27 Mar 2020 06:20
Operator : CG/JU
Sample : PB127720BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

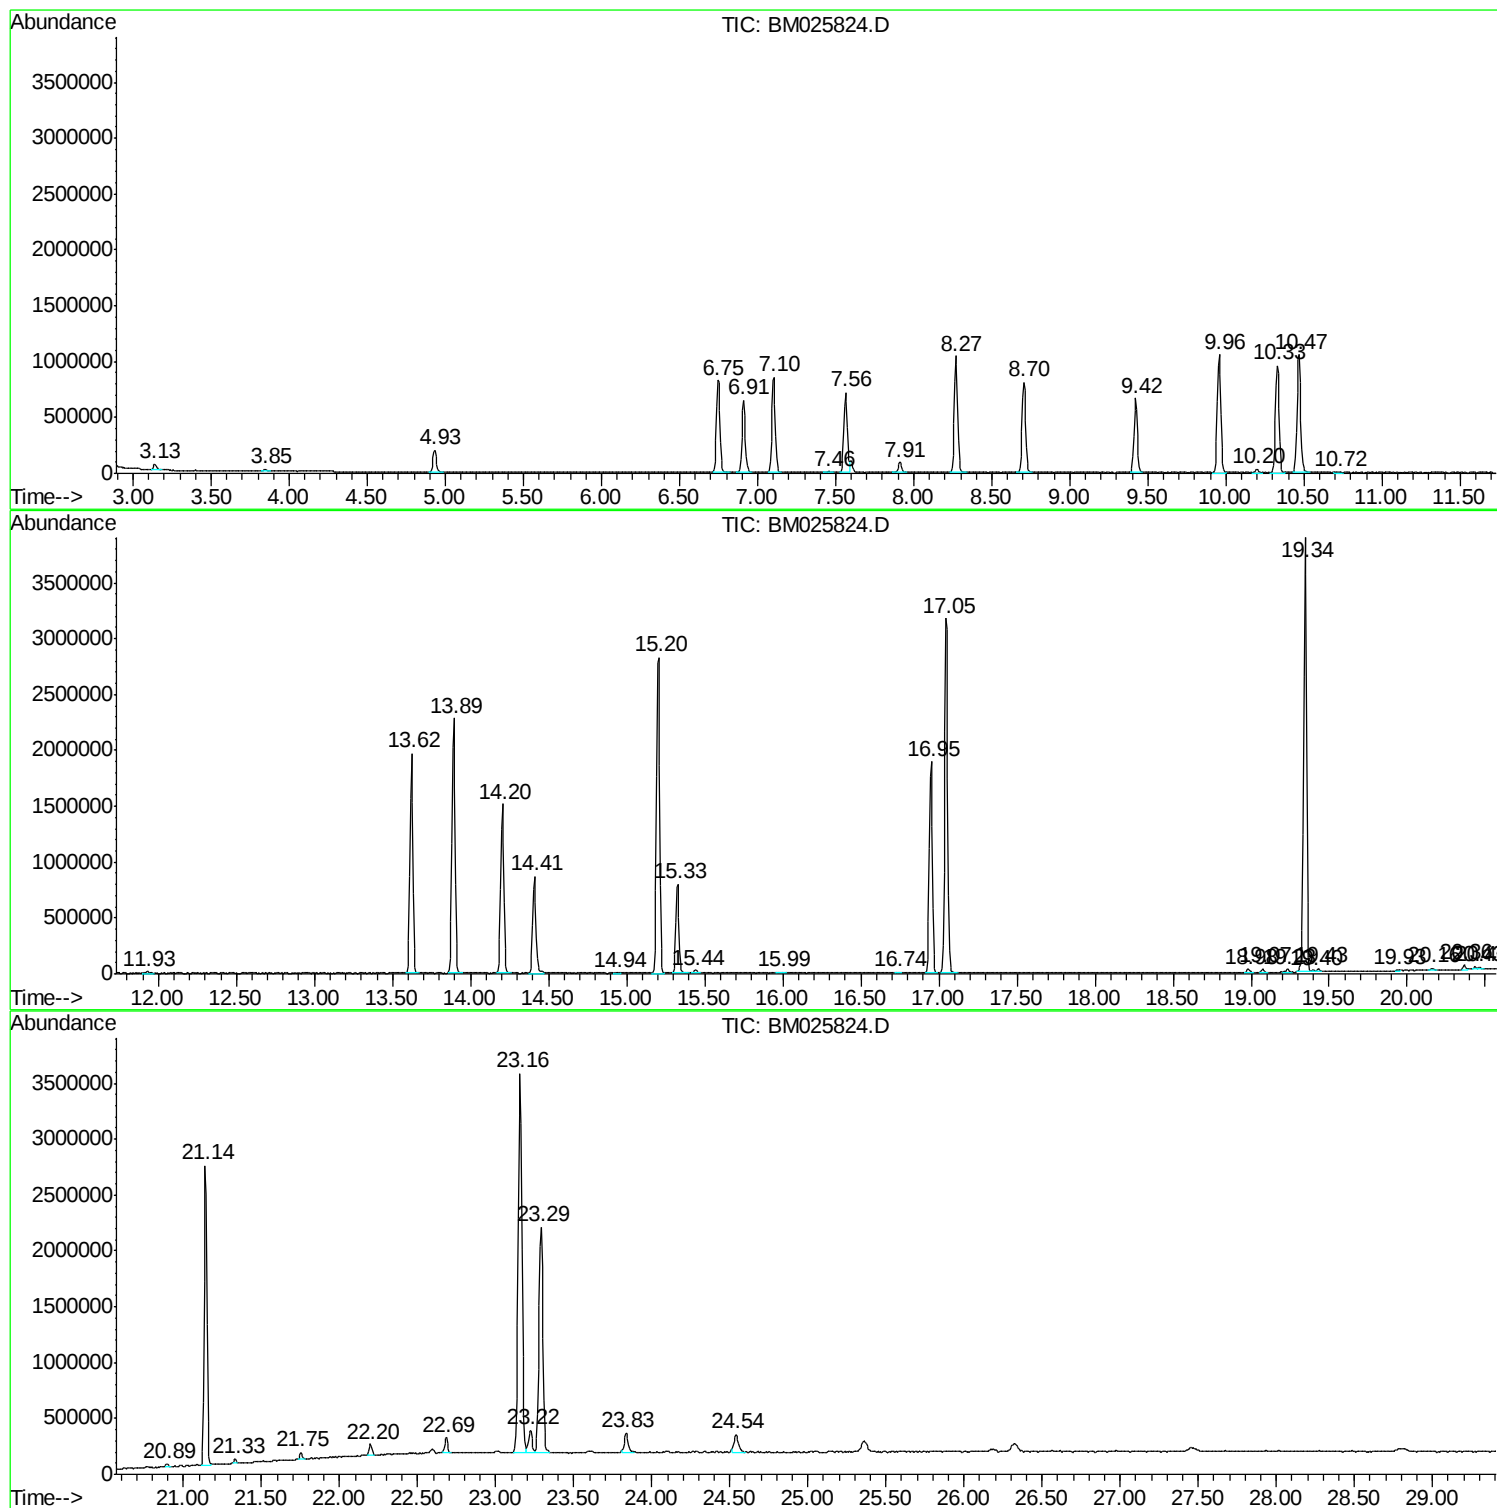

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025824.D
Acq On : 27 Mar 2020 06:20
Operator : CG/JU
Sample : PB127720BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025824.D
Acq On : 27 Mar 2020 06:20
Operator : CG/JU
Sample : PB127720BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc