

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025831.D
 Acq On : 27 Mar 2020 10:33
 Operator : CG/JU
 Sample : L2005-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CODE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	40	42	51	rVB6	14655	22528	0.26%	0.026%
2	3.846	159	163	167	rVB	17051	22568	0.26%	0.026%
3	4.928	341	347	359	rVB	2007019	2981842	34.04%	3.416%
4	6.745	651	656	666	rVB	191254	316098	3.61%	0.362%
5	6.910	678	684	693	rBV	755601	1143499	13.05%	1.310%
6	7.098	710	716	726	rBV	822245	1298629	14.83%	1.488%
7	7.457	771	777	787	rVB	387021	604858	6.91%	0.693%
8	7.563	789	795	798	rVV	906649	1492097	17.03%	1.709%
9	7.598	798	801	808	rVV	1750091	2494452	28.48%	2.858%
10	7.645	808	809	815	rVB2	18508	17501	0.20%	0.020%
11	7.910	847	854	863	rBV	1831811	2795331	31.91%	3.202%
12	8.269	909	915	923	rBV	640320	950244	10.85%	1.089%
13	8.704	982	989	1003	rBV	1012769	1592894	18.19%	1.825%
14	9.039	1040	1046	1053	rVB3	23320	40116	0.46%	0.046%
15	9.180	1064	1070	1077	rVB	38953	59124	0.67%	0.068%
16	9.275	1082	1086	1089	rVV	21328	29301	0.33%	0.034%
17	9.351	1089	1099	1104	rVB5	23429	68811	0.79%	0.079%
18	9.422	1104	1111	1118	rBV	826093	1282632	14.64%	1.469%
19	9.492	1118	1123	1128	rVB	24518	38325	0.44%	0.044%
20	9.722	1157	1162	1168	rBV5	6635	13765	0.16%	0.016%
21	9.957	1195	1202	1210	rBV	1232537	1995096	22.78%	2.286%
22	10.204	1235	1244	1256	rVV	5362524	8759144	100.00%	10.034%
23	10.327	1259	1265	1273	rVV	1207415	1959408	22.37%	2.245%
24	10.469	1282	1289	1298	rBV	51285	91507	1.04%	0.105%
25	10.716	1323	1331	1341	rBV	2156279	3392550	38.73%	3.886%
26	11.921	1530	1536	1544	rVB2	19512	33968	0.39%	0.039%
27	12.345	1602	1608	1610	rBV3	50956	76126	0.87%	0.087%
28	12.380	1610	1614	1621	rVB	127168	197563	2.26%	0.226%
29	12.616	1647	1654	1658	rBV3	25209	35493	0.41%	0.041%
30	12.992	1711	1718	1725	rBV	672198	969003	11.06%	1.110%
31	13.057	1725	1729	1733	rVB4	9234	13580	0.16%	0.016%
32	13.110	1733	1738	1742	rBV6	6102	10500	0.12%	0.012%
33	13.221	1751	1757	1763	rBV3	14342	25151	0.29%	0.029%
34	13.274	1763	1766	1772	rVB4	15776	21895	0.25%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
 Data File : BM025831.D
 Acq On : 27 Mar 2020 10:33
 Operator : CG/JU
 Sample : L2005-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CODE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	13.498	1801	1804	1810	rBV5	7166	11124	0.13%	0.013%
36	13.621	1816	1825	1830	rBV	2454475	3321696	37.92%	3.805%
37	13.668	1830	1833	1839	rVB	330194	419488	4.79%	0.481%
38	13.892	1864	1871	1880	rBV	2851753	4065623	46.42%	4.658%
39	14.010	1888	1891	1900	rVB7	6716	13038	0.15%	0.015%
40	14.139	1910	1913	1916	rVB3	9186	12968	0.15%	0.015%
41	14.204	1917	1924	1931	rBV	1869488	2685234	30.66%	3.076%
42	14.410	1954	1959	1972	rBV	180039	283636	3.24%	0.325%
43	14.527	1975	1979	1986	rVB	53619	69497	0.79%	0.080%
44	14.692	2003	2007	2010	rVV4	13942	18350	0.21%	0.021%
45	15.104	2071	2077	2081	rBV6	14977	25371	0.29%	0.029%
46	15.204	2087	2094	2102	rBV	3691055	5182865	59.17%	5.937%
47	15.327	2109	2115	2128	rBV	1181744	1610794	18.39%	1.845%
48	15.439	2128	2134	2139	rVB2	41468	60453	0.69%	0.069%
49	15.986	2224	2227	2231	rVB3	13024	16774	0.19%	0.019%
50	16.739	2350	2355	2361	rBV5	10993	19604	0.22%	0.022%
51	16.951	2384	2391	2398	rVB	2377675	3266012	37.29%	3.741%
52	17.051	2401	2408	2418	rVV	4142495	5870711	67.02%	6.725%
53	17.868	2543	2547	2552	rBV2	45026	60900	0.70%	0.070%
54	18.174	2596	2599	2605	rVB8	6822	10063	0.11%	0.012%
55	18.980	2728	2736	2742	rBV	48528	67284	0.77%	0.077%
56	19.162	2763	2767	2770	rBV4	17546	22594	0.26%	0.026%
57	19.233	2775	2779	2783	rVV2	39976	51611	0.59%	0.059%
58	19.345	2792	2798	2805	rBV	5187786	6960471	79.47%	7.974%
59	19.597	2837	2841	2844	rBV3	6024	9950	0.11%	0.011%
60	19.862	2884	2886	2889	rBV3	11910	11131	0.13%	0.013%
61	20.886	3056	3060	3067	rBV	170542	234905	2.68%	0.269%
62	21.144	3098	3104	3111	rBV	3309448	4100145	46.81%	4.697%
63	21.333	3132	3136	3139	rBV2	52813	58992	0.67%	0.068%
64	21.756	3205	3208	3214	rVB3	87606	102839	1.17%	0.118%
65	22.197	3280	3283	3288	rBV2	128709	158433	1.81%	0.181%
66	22.685	3362	3366	3371	rVB	175399	227895	2.60%	0.261%
67	23.162	3439	3447	3453	rBV	4697257	8033467	91.72%	9.203%
68	23.227	3454	3458	3462	rVV	227355	348452	3.98%	0.399%
69	23.291	3462	3469	3480	rVB2	2488735	4457681	50.89%	5.107%
70	23.832	3557	3561	3568	rVB	178504	299789	3.42%	0.343%
71	24.544	3677	3682	3689	rVB3	145117	276277	3.15%	0.316%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025831.D
Acq On : 27 Mar 2020 10:33
Operator : CG/JU
Sample : L2005-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CODE8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 87291716

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032620\
Data File : BM025831.D
Acq On : 27 Mar 2020 10:33
Operator : CG/JU
Sample : L2005-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
CODE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

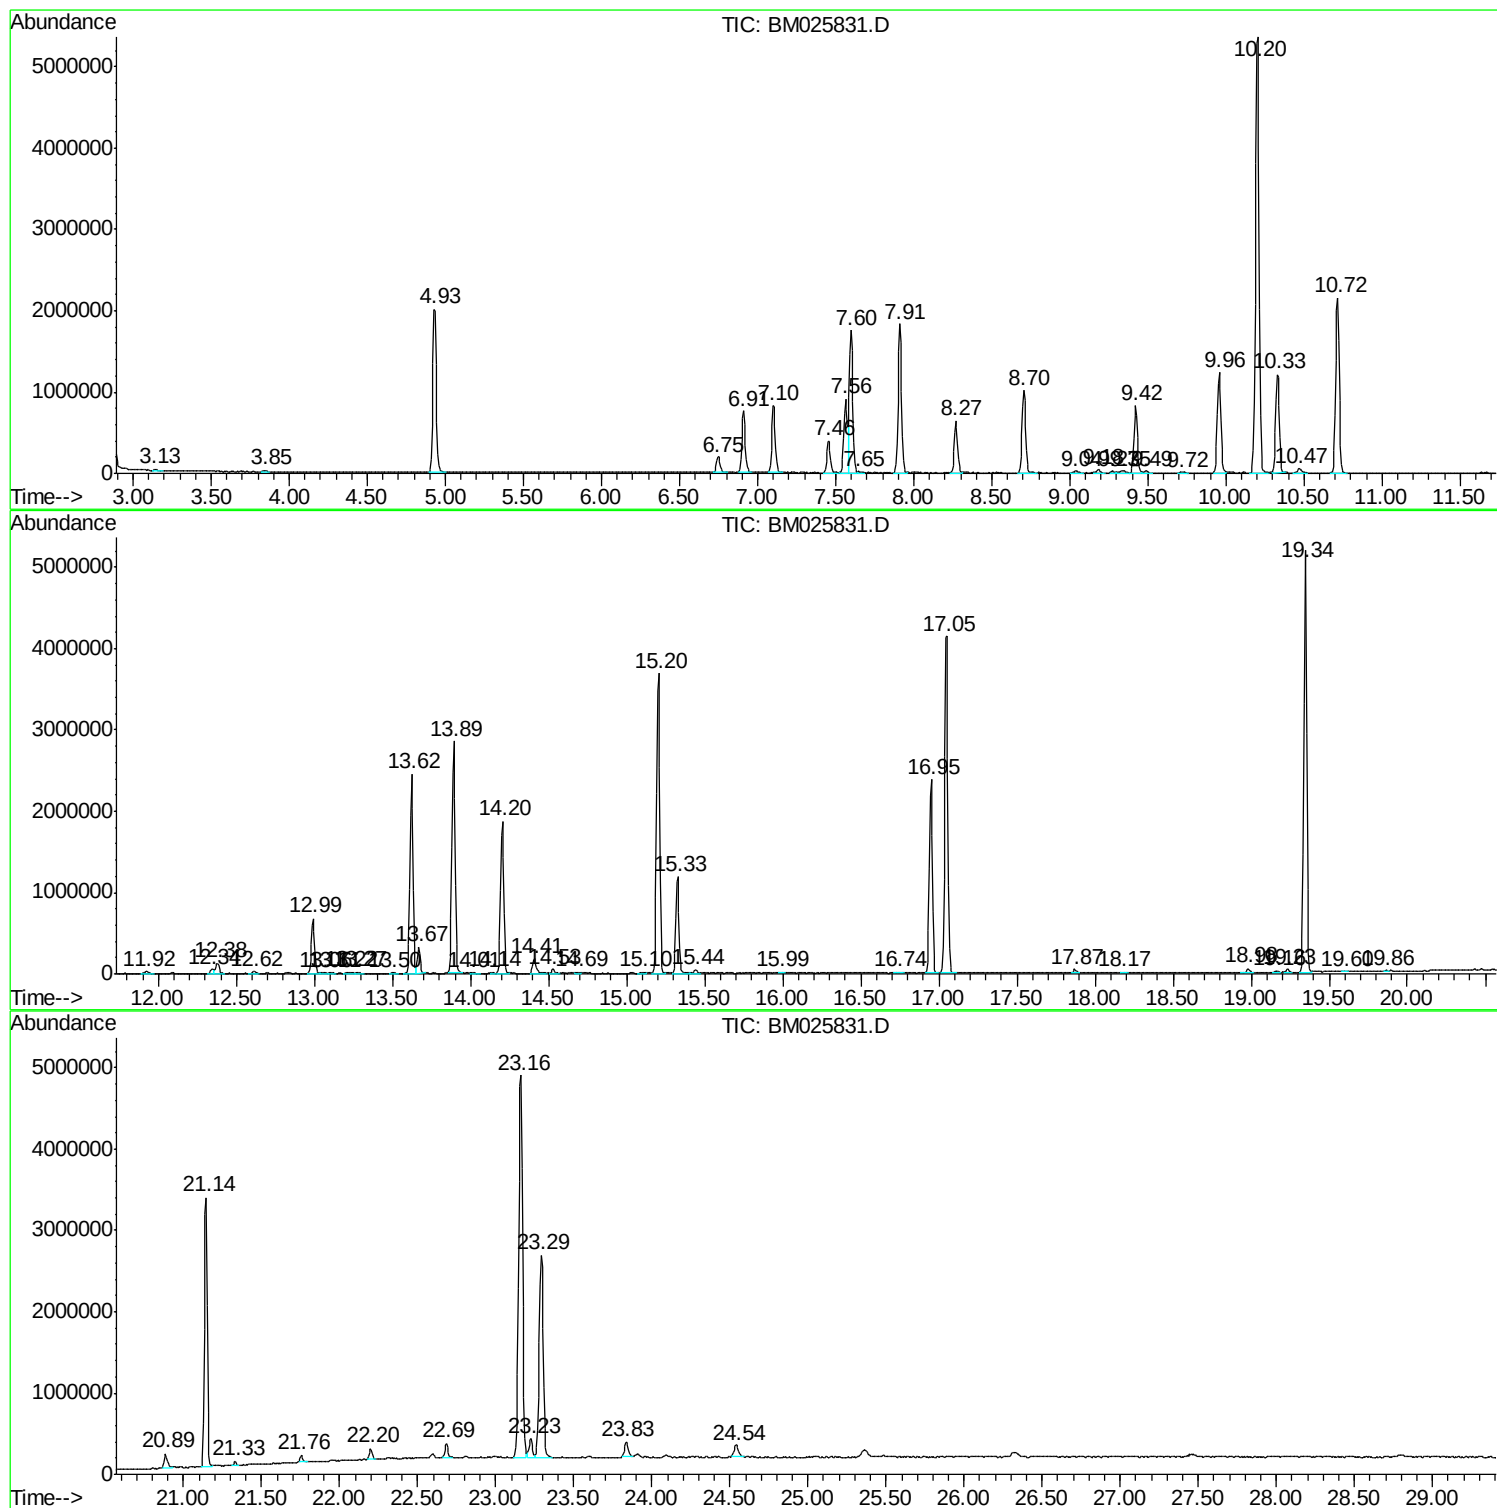

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025831.D
Acq On : 27 Mar 2020 10:33
Operator : CG/JU
Sample : L2005-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CODE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032620\
Data File : BM025831.D
Acq On : 27 Mar 2020 10:33
Operator : CG/JU
Sample : L2005-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CODE8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc