

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
 Data File : BM019516.D
 Acq On : 27 Mar 2019 21:57
 Operator : JU/SJ
 Sample : K2052-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VILLAGE-WELL02-01

Quant Time: Mar 28 05:13:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 28 05:07:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	104791	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.37	136	457462	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.24	164	263940	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.00	188	578862	20.00	ng/ul	-0.01
78) Chrysene-d12	21.21	240	675068	20.00	ng/ul	-0.01
86) Perylene-d12	23.42	264	796966	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	10873	4.06	ng/uL	-0.01
5) Phenol-d5	6.87	99	714	0.08	ng/ul	0.09
7) Bis-(2-Chloroethyl)ether-d	6.94	67	200884	32.15	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.13	132	29820	4.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	19696	2.81	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	123577	37.87	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.47	143	74531	20.52	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.00	165	169559	24.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	1497	0.18	ng/ul	-0.01
44) Dimethylphthalate-d6	13.67	166	860922	40.42	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	1598	0.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	373	0.11	ng/ul	0.09
58) Fluorene-d10	15.24	176	339816	18.52	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.40	200	45038	11.77	ng/ul	0.00
71) Anthracene-d10	17.10	188	3525	0.13	ng/ul	-0.01
79) Pyrene-d10	19.42	212	1420	0.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	2377	0.06	ng/ul	-0.01

Target Compounds


					Qvalue
8) Bis(2-Chloroethyl)ether	7.00	93	941839	126.428 ng/ul#	44
30) 4-Chloroaniline	10.52	127	11623	1.341 ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
Data File : BM019516.D
Acq On : 27 Mar 2019 21:57
Operator : JU/SJ
Sample : K2052-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VILLAGE-WELL02-01

Quant Time: Mar 28 05:13:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 05:07:19 2019
Response via : Initial Calibration




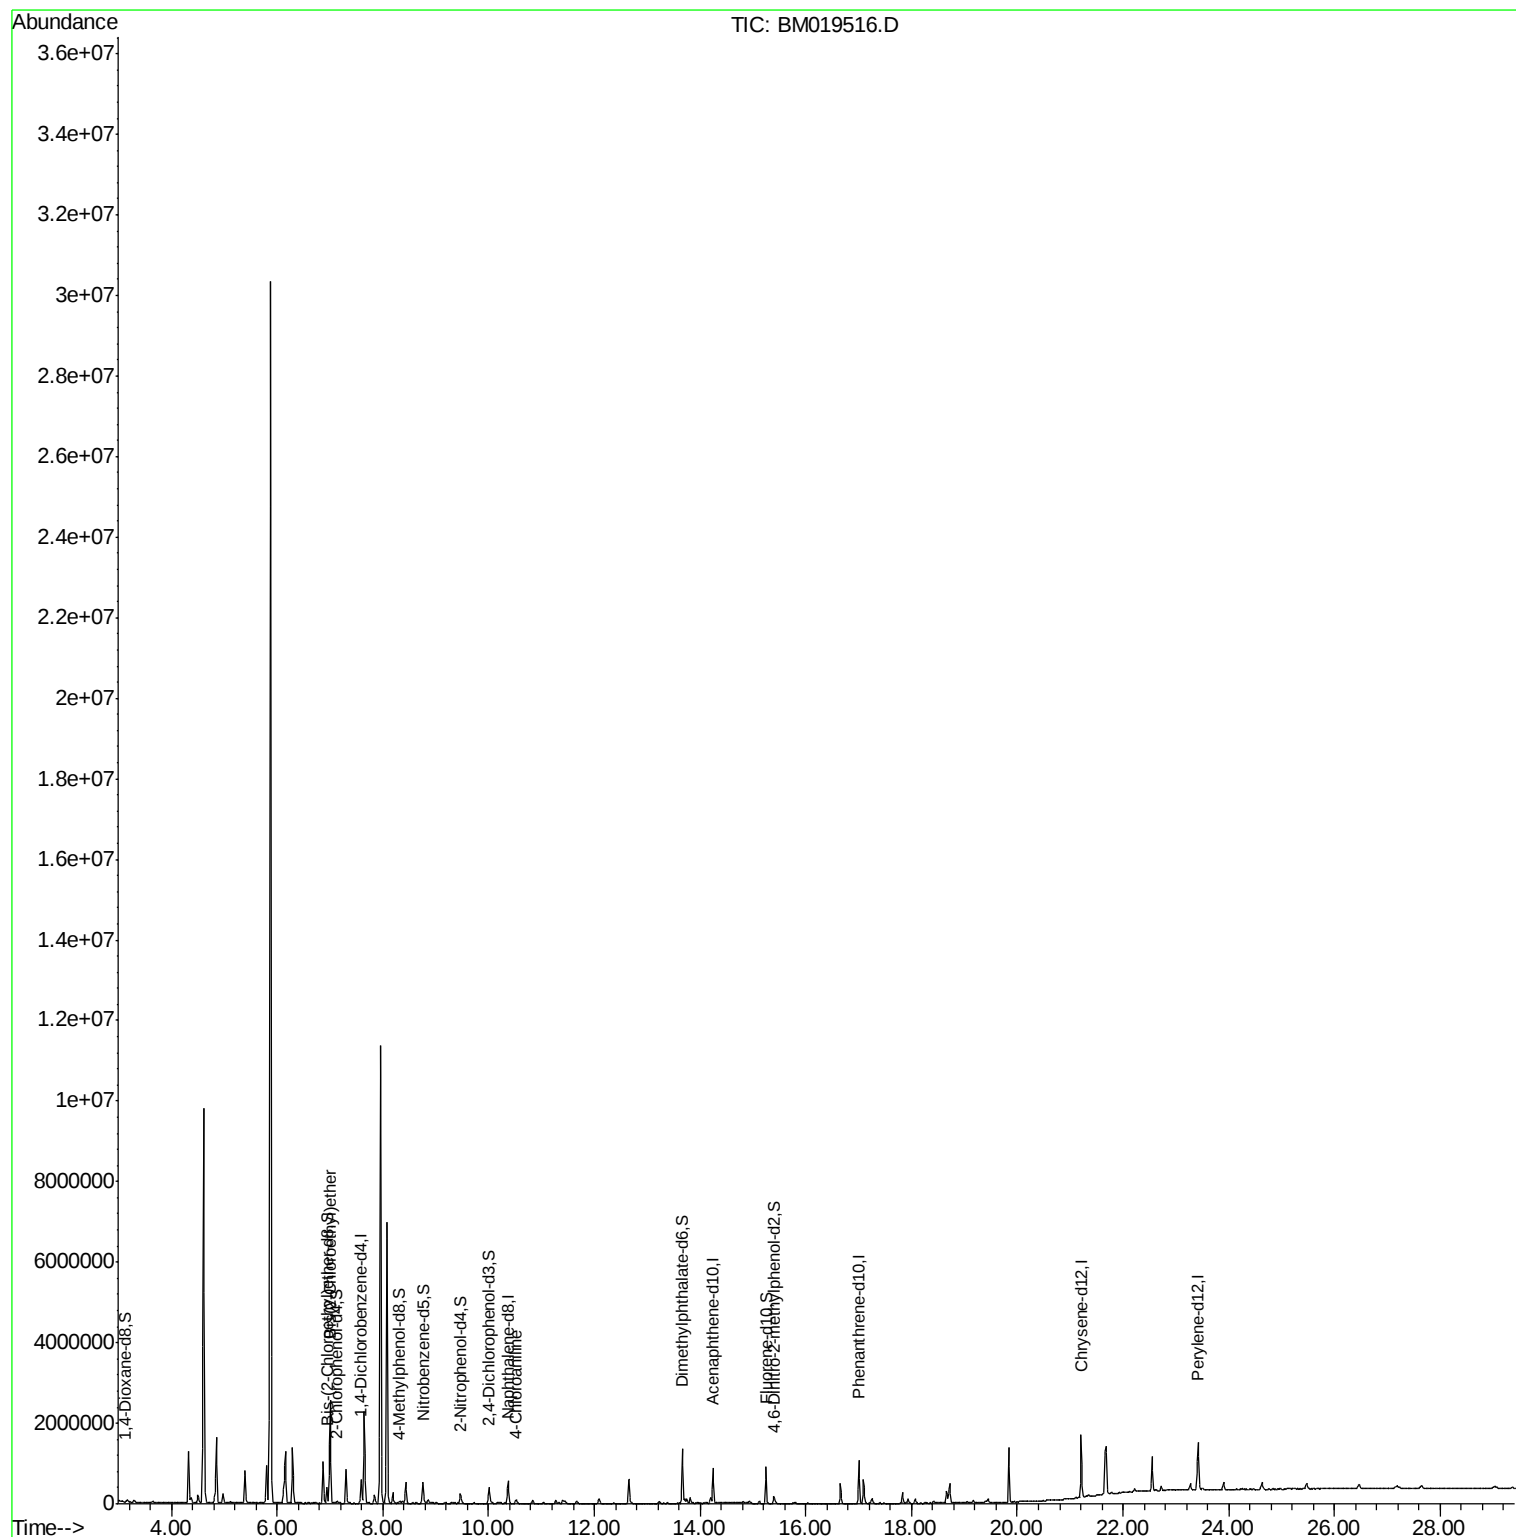


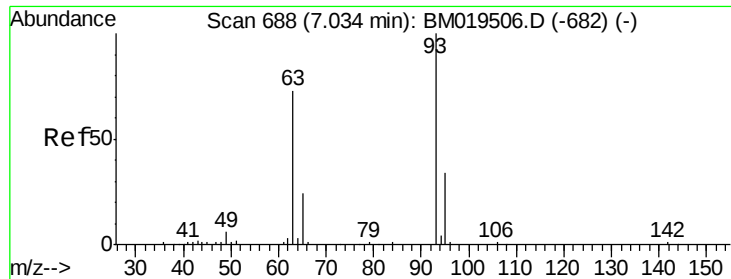

#8
 Bis(2-Chloroethyl)ether
 Concen: 126.428 ng/ul
 RT: 7.00 min Scan# 683
 Delta R.T. -0.04 min
 Lab File: BM019516.D
 Acq: 27 Mar 2019 21:57

Instrument :
 BNA_M
 ClientSampleId :
 VILLAGE-WELL02-01

Tgt Ion:	93	Resp:	941839
Ion	Ratio	Lower	Upper
93	100		
63	6.2	59.4	89.2#
95	31.7	26.4	39.6

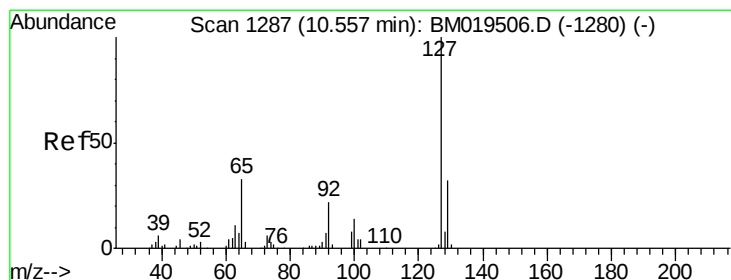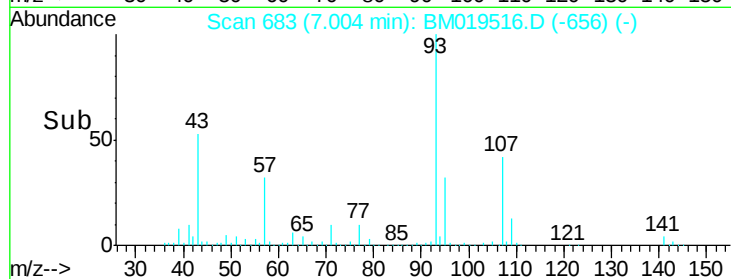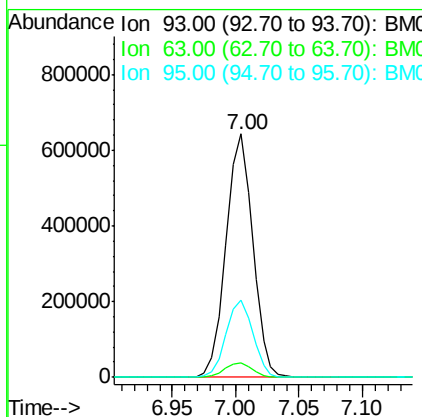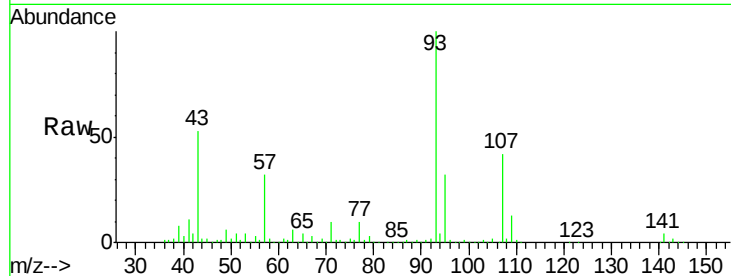

#30
 4-Chloroaniline
 Concen: 1.341 ng/ul
 RT: 10.52 min Scan# 1280
 Delta R.T. -0.05 min
 Lab File: BM019516.D
 Acq: 27 Mar 2019 21:57

Tgt Ion:	127	Resp:	11623
Ion	Ratio	Lower	Upper
127	100		
129	72.2	24.6	37.0#

