

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
 Data File : BM019525.D
 Acq On : 28 Mar 2019 03:31
 Operator : JU/SJ
 Sample : K2063-07MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 DB6R7MSD

Manual Integrations
 APPROVED

Sohil
 3/28/2019 3:18:37 PM

Quant Time: Mar 28 08:11:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 28 05:07:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	92594	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.37	136	402497	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.24	164	241665	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.00	188	541481	20.00	ng/ul	-0.01
78) Chrysene-d12	21.21	240	697366	20.00	ng/ul	-0.01
86) Perylene-d12	23.41	264	921316	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	7740	3.27	ng/uL	-0.01
5) Phenol-d5	6.79	99	91478	11.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	172309	31.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	167707	26.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	121614	19.65	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	149585	52.10	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.47	143	113275	35.45	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.00	165	190483	31.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	3989	0.55	ng/ul	0.03
44) Dimethylphthalate-d6	13.67	166	625145	32.06	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	762033	31.25	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.51	143	30546m	9.99	ng/ul	0.01
58) Fluorene-d10	15.24	176	516589	30.75	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.39	200	107136	29.92	ng/ul	-0.01
71) Anthracene-d10	17.10	188	835500	32.15	ng/ul	-0.01
79) Pyrene-d10	19.41	212	965537	29.97	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.28	264	1408847	28.84	ng/ul	-0.01

Target Compounds

					Qvalue	
6) Phenol	6.82	94	109431	12.718	ng/ul#	1
10) 2-Chlorophenol	7.16	128	169201	26.634	ng/ul	96
11) 2-Methylphenol	8.05	108	39327	6.554	ng/ul	97
14) Acetophenone	8.42	105	276464	27.428	ng/ul	91
15) N-Nitroso-di-n-propylamine	8.40	70	197437	34.953	ng/ul#	90
16) 4-Methylphenol	8.37	108	34420	5.230	ng/ul	91
24) 2,4-Dimethylphenol	9.57	107	80954	10.569	ng/ul#	68
28) Naphthalene	10.43	128	13729951	658.477	ng/ul	97
33) 4-Chloro-3-methylphenol	11.69	107	264016	41.108	ng/ul#	87
34) 2-Methylnaphthalene	12.04	142	2590169	177.282	ng/ul	99
35) 1-Methylnaphthalene	12.26	142	1244016	90.177	ng/ul	97
41) 1,1'-Biphenyl	13.07	154	38968	1.893	ng/ul#	93
50) Acenaphthene	14.31	153	516143	30.326	ng/ul	98
53) 4-Nitrophenol	14.52	109	24996	10.449	ng/ul#	74
55) 2,4-Dinitrotoluene	14.64	165	190610	35.838	ng/ul	88
57) Diethylphthalate	15.08	149	22139	1.150	ng/ul	98
69) Pentachlorophenol	16.66	266	139570	37.501	ng/ul	98
80) Pyrene	19.44	202	1270301	30.278	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
Data File : BM019525.D
Acq On : 28 Mar 2019 03:31
Operator : JU/SJ
Sample : K2063-07MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DB6R7MSD

Manual Integrations
APPROVED

Sohil
3/28/2019 3:18:37 PM

Quant Time: Mar 28 08:11:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 05:07:19 2019
Response via : Initial Calibration

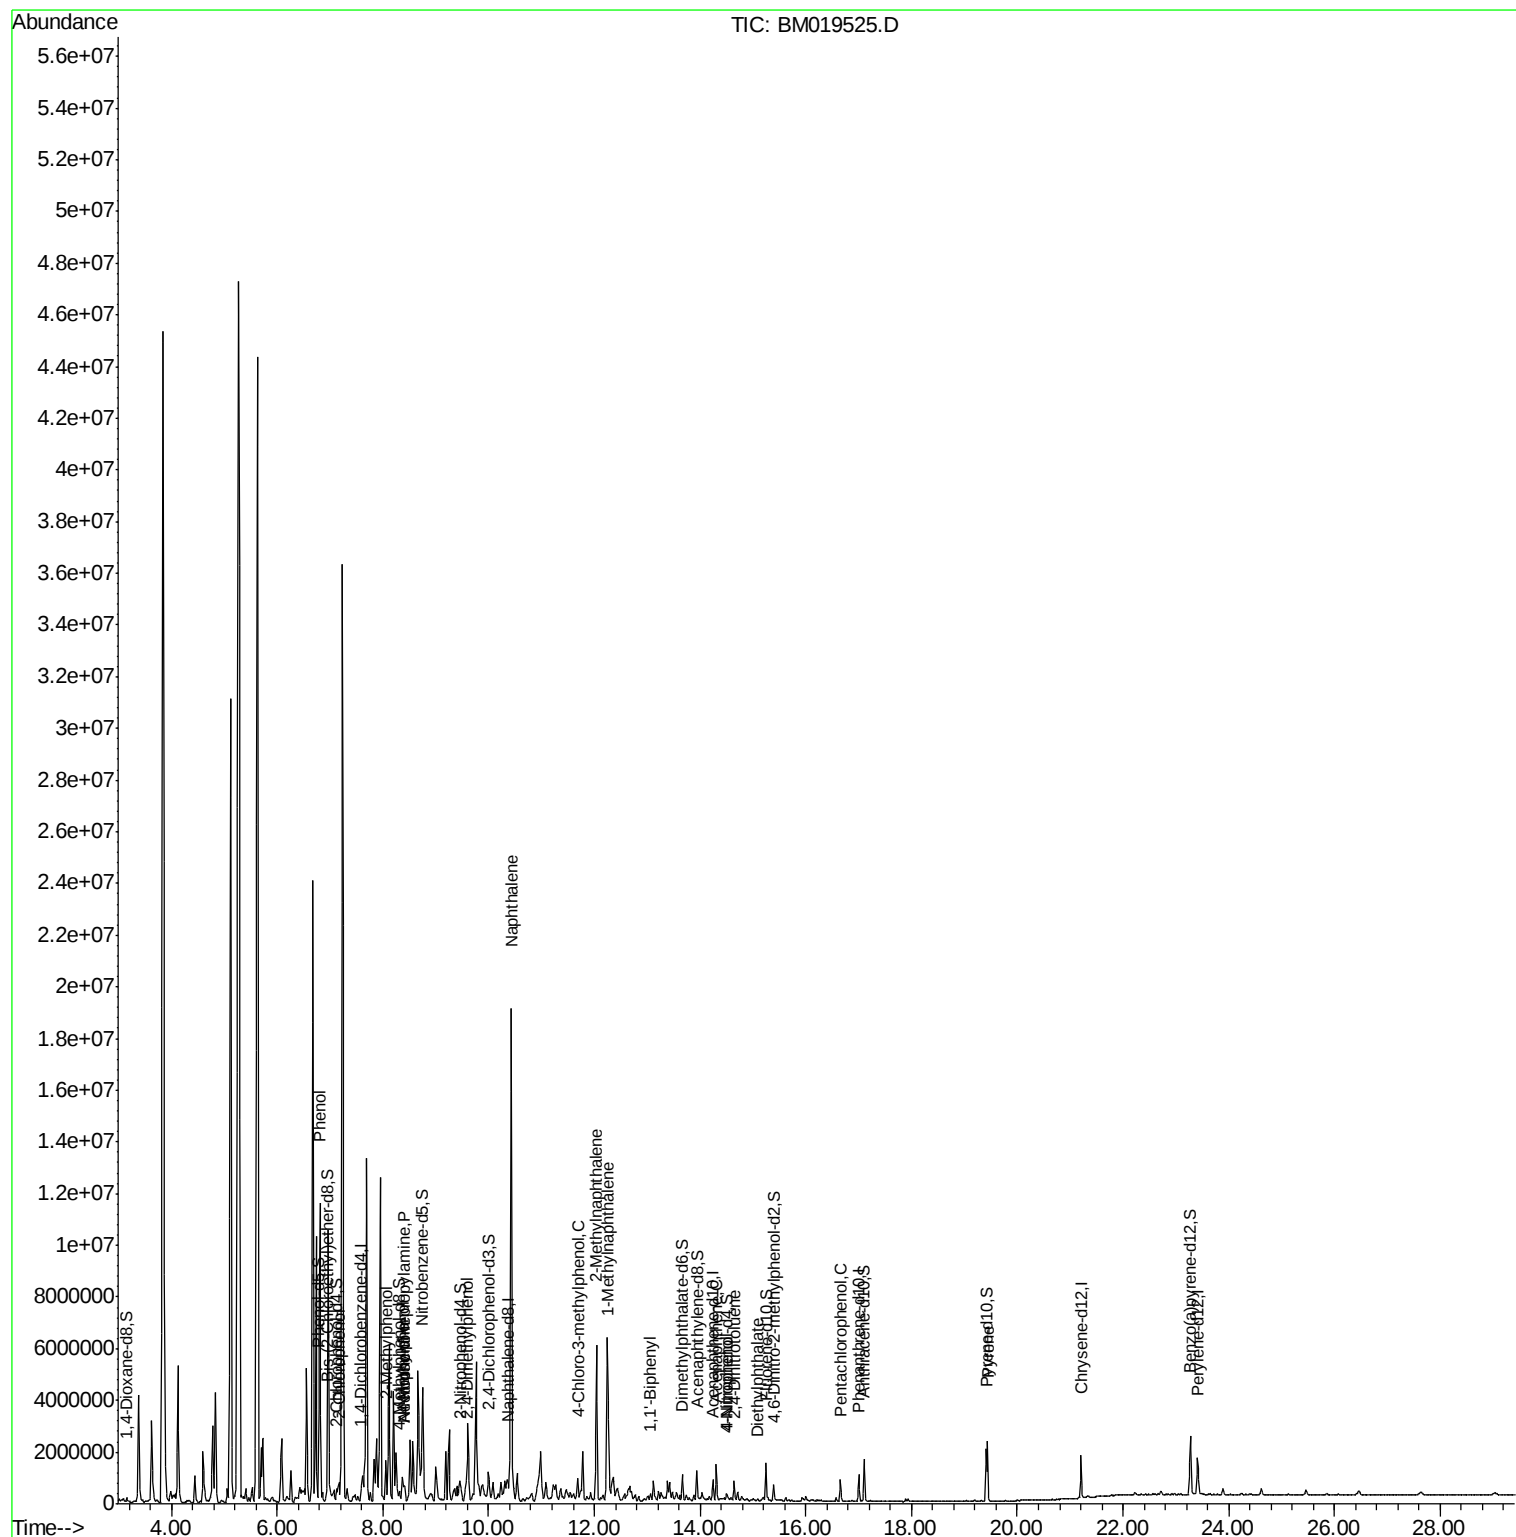

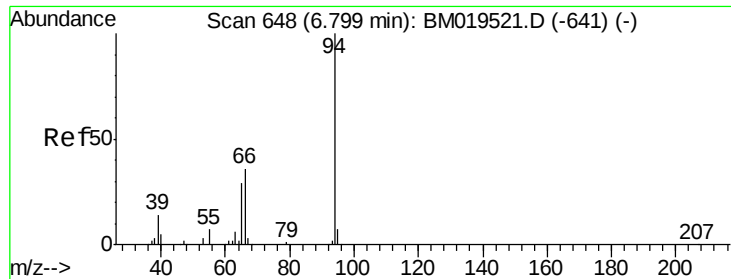

#6

Phenol

Concen: 12.718 ng/ul

RT: 6.82 min Scan# 651

Delta R.T. 0.01 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Instrument :

BNA_M





ClientSampleId :

DB6R7MSD

Tgt Ion:	94	Resp:	109431
Ion Ratio	Lower	Upper	
94	100		
65	227.1	23.0	34.6#
66	61.1	30.4	45.6#

Manual Integrations
APPROVED

Sohil
3/28/2019 3:18:37 PM

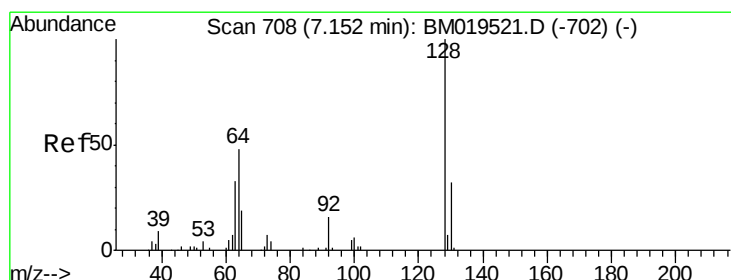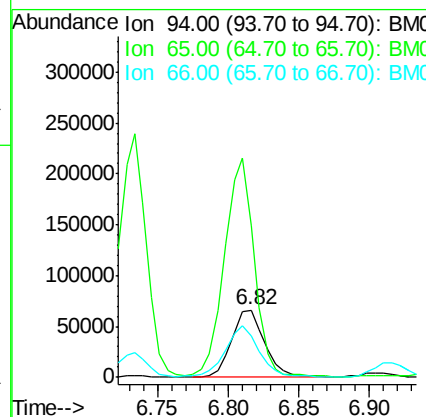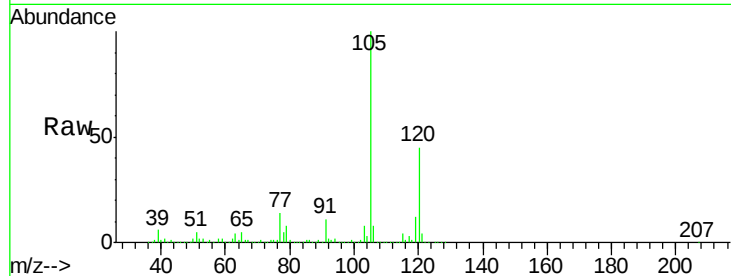

#10

2-Chlorophenol

Concen: 26.634 ng/ul




RT: 7.16 min Scan# 710


Delta R.T. -0.00 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Tgt Ion:	128	Resp:	169201
Ion Ratio	Lower	Upper	
128	100		
64	53.4	39.8	59.6
130	33.7	25.8	38.8

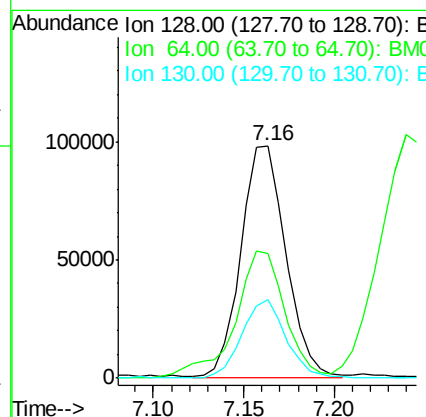

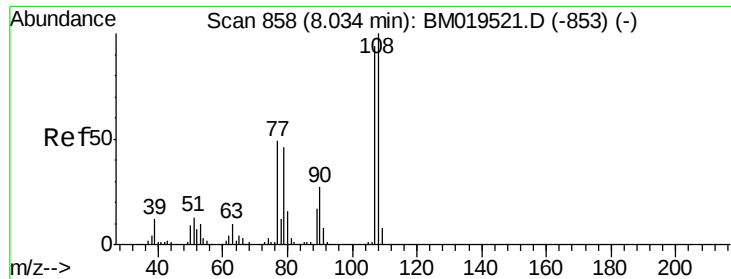





#11
2-Methylphenol
Concen: 6.554 ng/ul
RT: 8.05 min Scan# 861
Delta R.T. 0.01 min
Lab File: BM019525.D
Acq: 28 Mar 2019 03:31

Instrument :
BNA_M
ClientSampled :
DB6R7MSD

Tgt Ion:108 Resp: 39327
Ion Ratio Lower Upper
108 100
107 95.0 74.1 111.1




Manual Integrations
APPROVED


Sohil
3/28/2019 3:18:37 PM

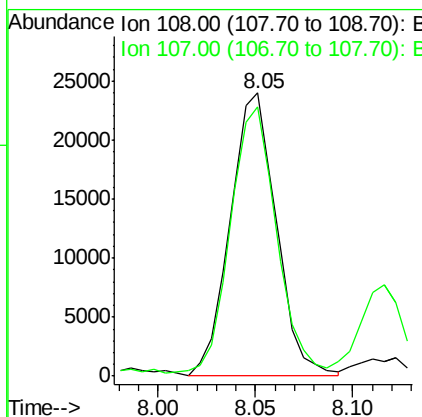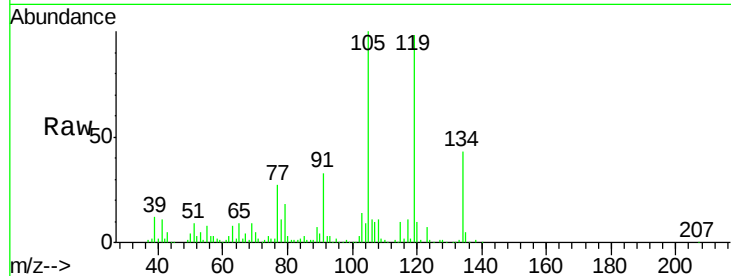

#14
Acetophenone
Concen: 27.428 ng/ul
RT: 8.42 min Scan# 924
Delta R.T. -0.01 min
Lab File: BM019525.D
Acq: 28 Mar 2019 03:31

Tgt Ion:105 Resp: 276464
Ion Ratio Lower Upper
105 100
77 87.2 63.2 94.8
51 20.1 19.8 29.8

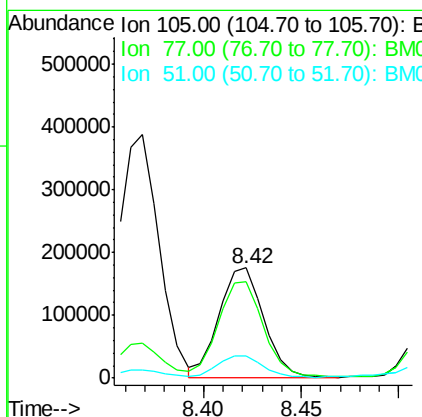

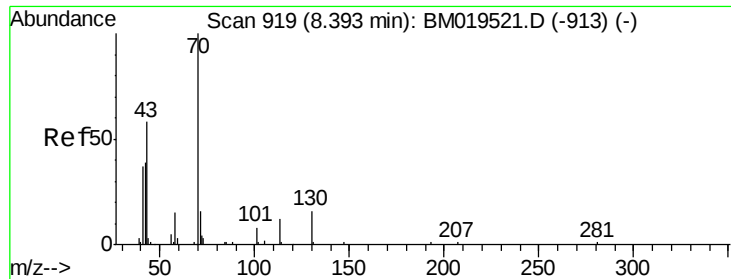

#15

N-Nitroso-di-n-propylamine

Concen: 34.953 ng/ul

RT: 8.40 min Scan# 920

Delta R.T. -0.01 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Instrument :

BNA_M





ClientSampleId :

DB6R7MSD

Tgt Ion	Ratio	Lower	Upper
70	100		
42	43.3	40.2	60.4
101	8.1	7.7	11.5
130	17.0	17.8	26.6

Manual Integrations
APPROVED

Sohil
3/28/2019 3:18:37 PM

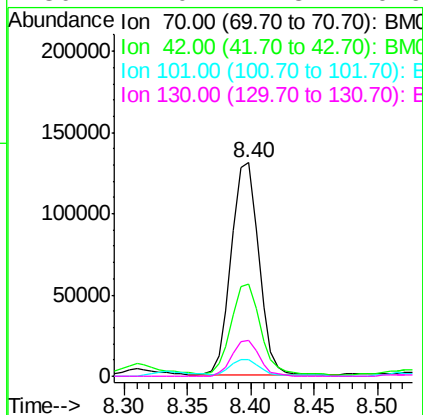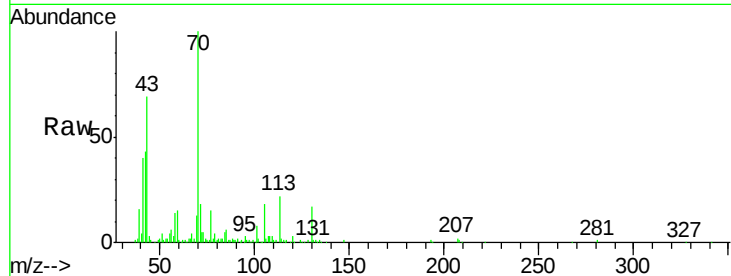

#16

4-Methylphenol

Concen: 5.230 ng/ul




RT: 8.37 min Scan# 916


Delta R.T. -0.00 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Lower	Upper
108	100		
107	127.2	93.6	140.4

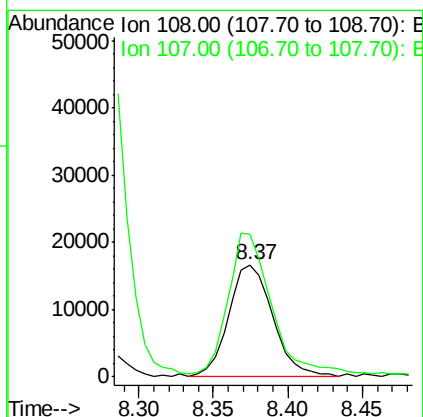

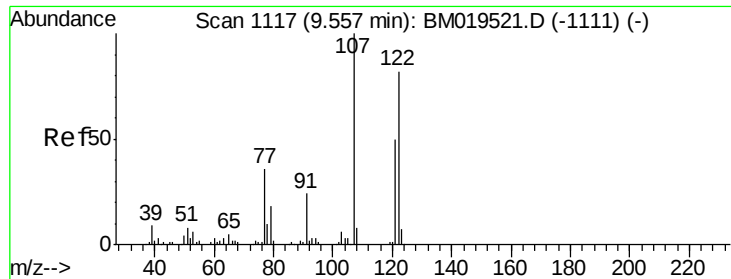

#24

2,4-Dimethylphenol

Concen: 10.569 ng/ul

RT: 9.57 min Scan# 1120

Delta R.T. 0.01 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Instrument :

BNA_M





ClientSampled :

DB6R7MSD

Tgt Ion	Ratio	Resp	Lower	Upper
107	100	80954		
121	21.0	38.1	57.1#	
122	55.6	63.8	95.8#	

Manual Integrations
APPROVED

Sohil
3/28/2019 3:18:37 PM

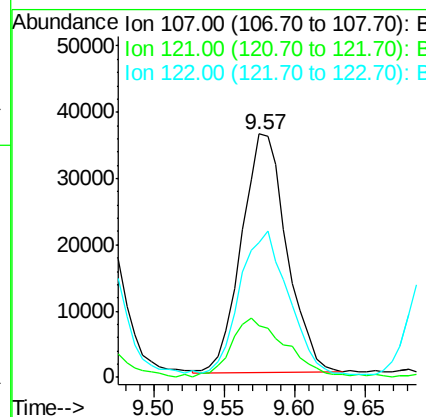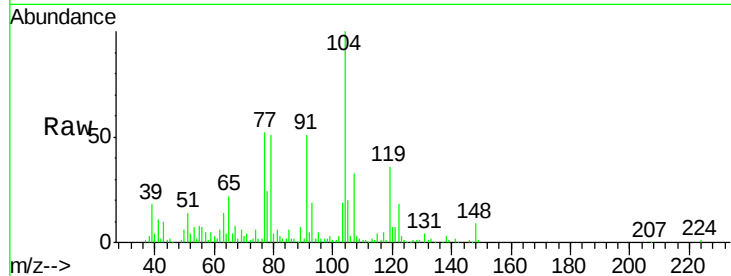

#28

Naphthalene

Concen: 658.477 ng/ul




RT: 10.43 min Scan# 1265


Delta R.T. -0.00 min

Lab File: BM019525.D

Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	13729951		
129	12.1	8.3	12.5	
127	14.2	10.8	16.2	

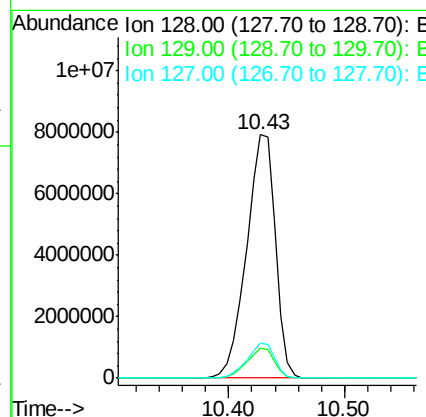

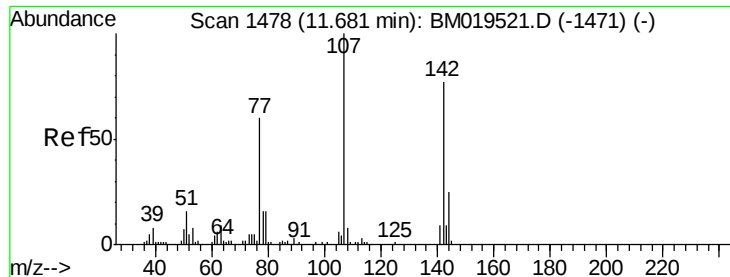





#33
 4-Chloro-3-methylphenol
 Concen: 41.108 ng/ul
 RT: 11.69 min Scan# 1479
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MSD

Tgt Ion	Ratio	Lower	Upper
107	100		
144	19.6	21.1	31.7#
142	63.6	60.1	90.1




Manual Integrations
 APPROVED


Sohil
 3/28/2019 3:18:37 PM

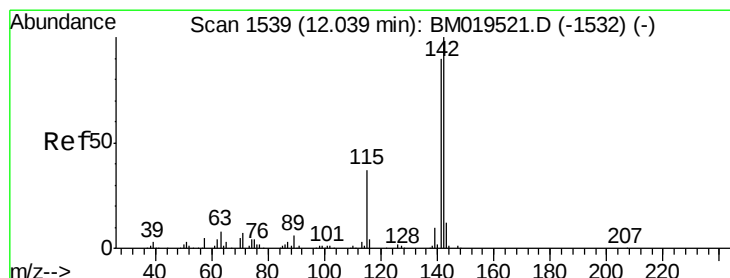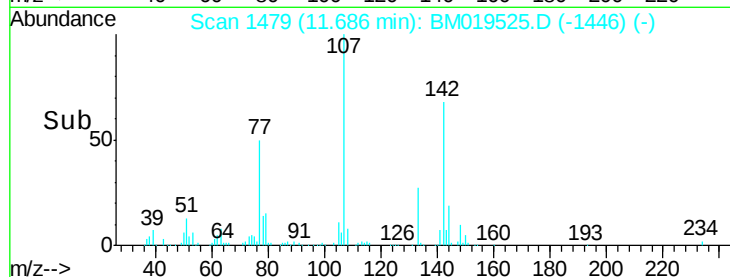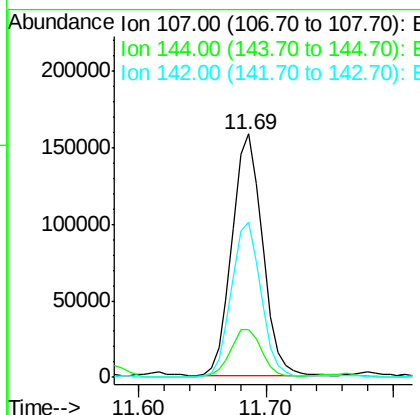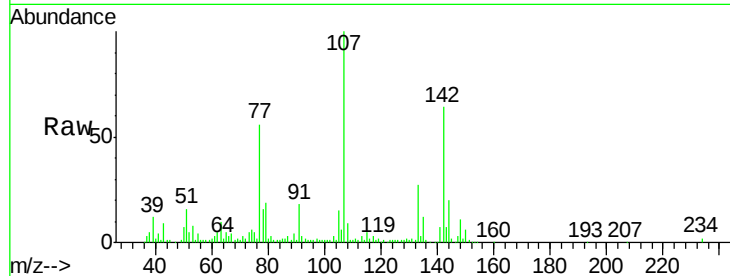

#34
 2-Methylnaphthalene
 Concen: 177.282 ng/ul
 RT: 12.04 min Scan# 1539
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.5	71.4	107.2

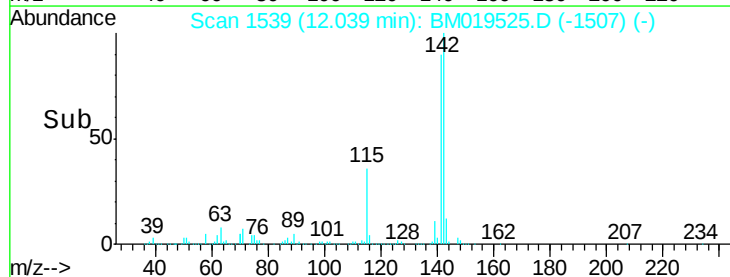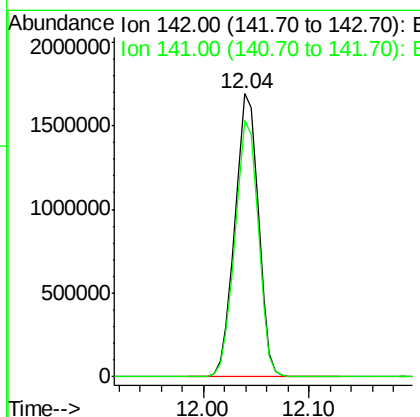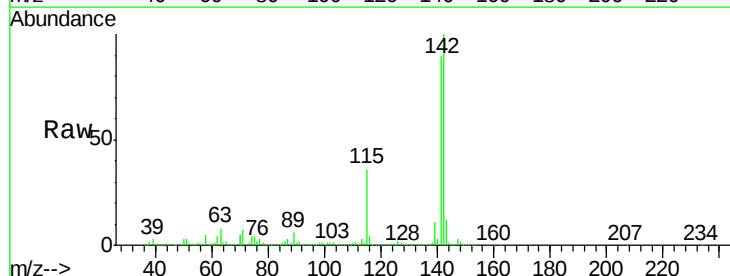







#35
 1-Methylnaphthalene
 Concen: 90.177 ng/ul
 RT: 12.26 min Scan# 1577
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Instrument :
 BNA_M
 ClientSampled :
 DB6R7MSD

Tgt Ion	Ratio	Lower	Upper
142	100		
141	92.5	76.6	115.0
116	4.3	3.6	5.4




Manual Integrations
 APPROVED


Sohil
 3/28/2019 3:18:37 PM

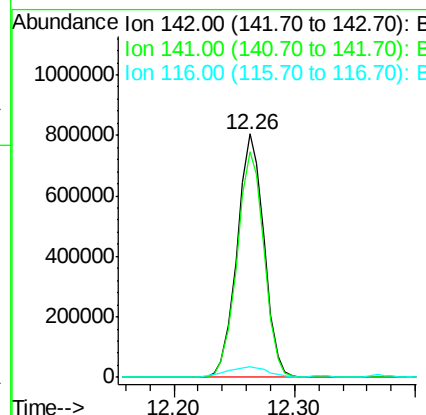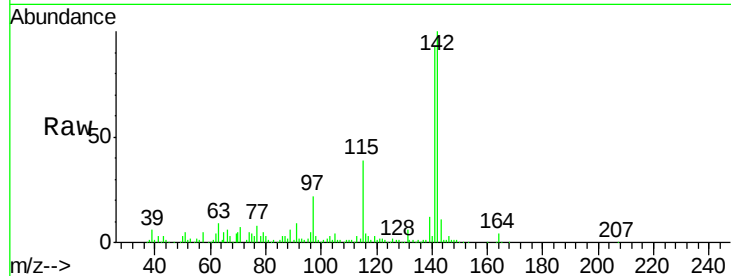

#41
 1,1'-Biphenyl
 Concen: 1.893 ng/ul
 RT: 13.07 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Lower	Upper
154	100		
153	43.1	34.0	51.0
76	22.0	8.4	12.6

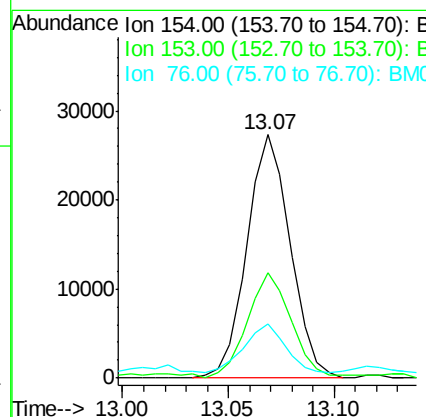

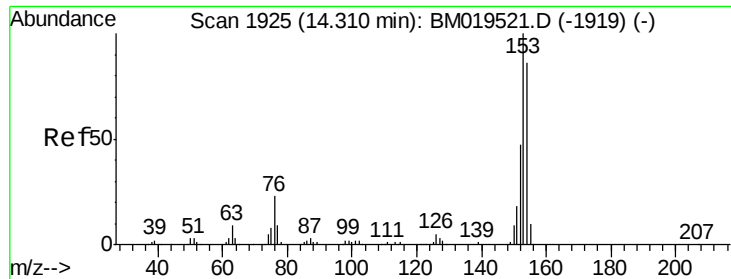





#50
Acenaphthene
Concen: 30.326 ng/ul
RT: 14.31 min Scan# 1925
Delta R.T. -0.01 min
Lab File: BM019525.D
Acq: 28 Mar 2019 03:31

Instrument :
BNA_M
ClientSampleId :
DB6R7MSD

Tgt Ion	Ratio	Lower	Upper
153	100		
152	46.8	37.9	56.9
154	85.1	69.8	104.6




Manual Integrations
APPROVED


Sohil
3/28/2019 3:18:37 PM

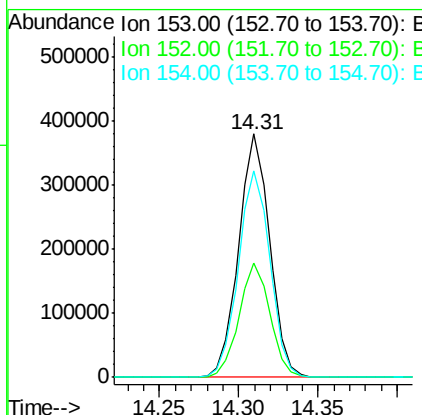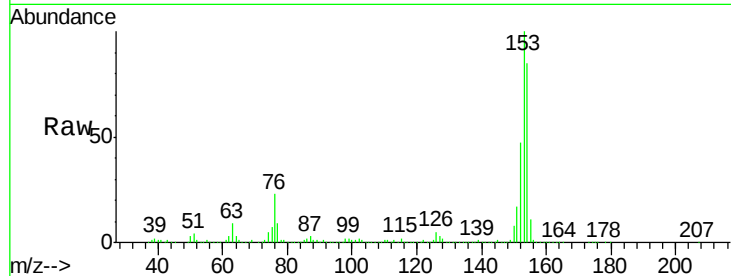

#53
4-Nitrophenol
Concen: 10.449 ng/ul
RT: 14.52 min Scan# 1961
Delta R.T. 0.01 min
Lab File: BM019525.D
Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Lower	Upper
109	100		
139	121.9	91.2	136.8
65	163.7	92.6	139.0#

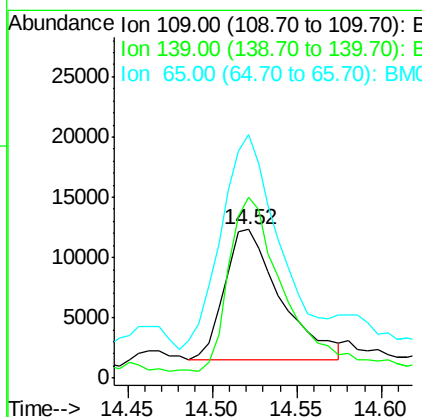

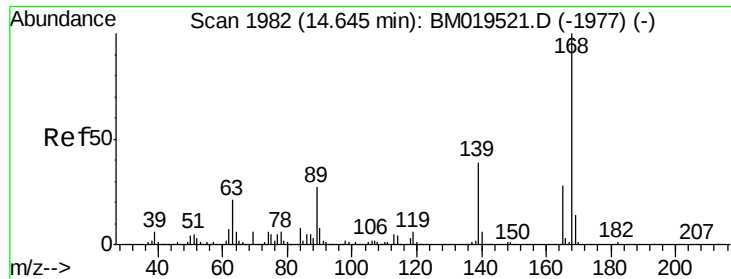





#55
 2,4-Dinitrotoluene
 Concen: 35.838 ng/ul
 RT: 14.64 min Scan# 1982
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MSD

Tgt Ion	Ratio	Resp	Lower	Upper
165	100	190610		
63	46.9	31.4	47.0	
182	2.8	2.7	4.1	




Manual Integrations
 APPROVED


Sohil
 3/28/2019 3:18:37 PM

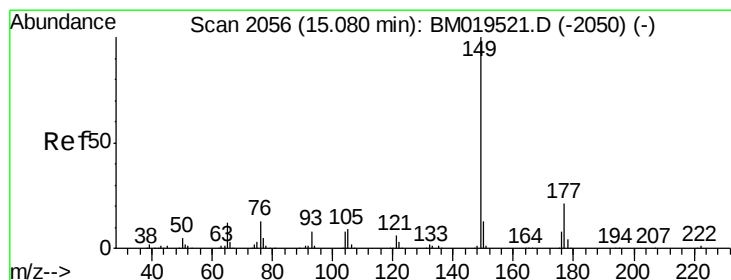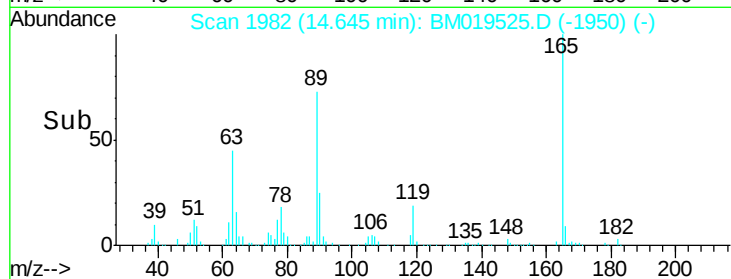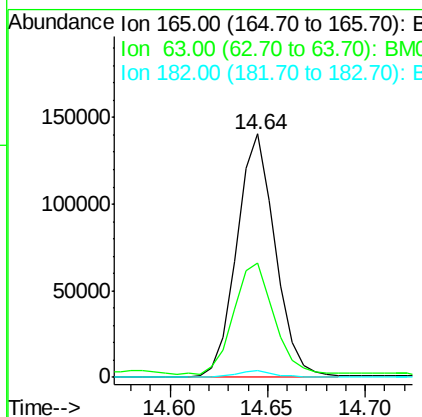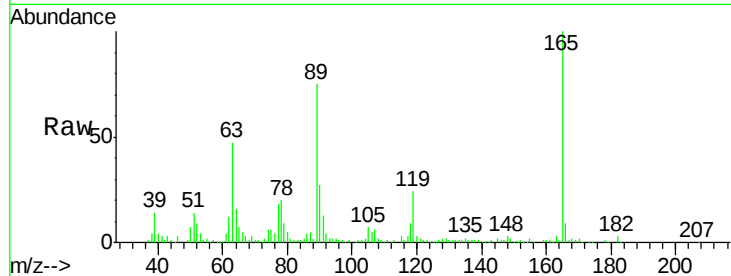

#57
 Diethylphthalate
 Concen: 1.150 ng/ul
 RT: 15.08 min Scan# 2056
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	22139		
177	22.3	19.3	28.9	
150	13.1	10.6	15.8	

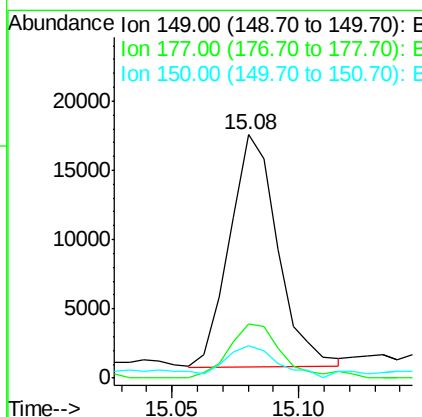

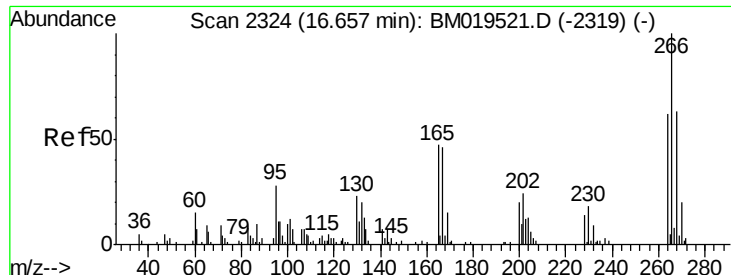





#69
 Pentachlorophenol
 Concen: 37.501 ng/ul
 RT: 16.66 min Scan# 2324
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MSD

Tgt Ion	Ratio	Resp	Lower	Upper
266	100	139570		
264	60.8	48.2	72.4	
268	62.1	52.3	78.5	

Manual Integrations
 APPROVED

Sohil
 3/28/2019 3:18:37 PM

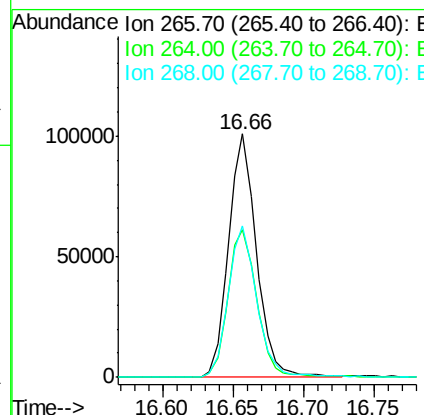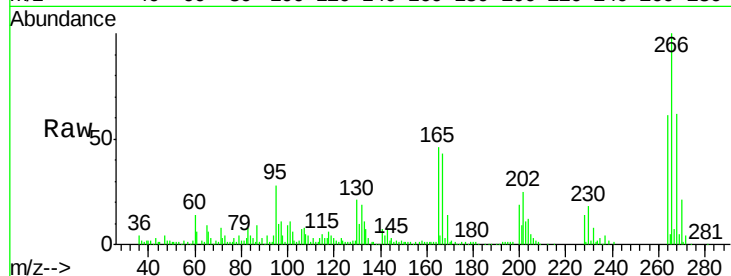

#80
 Pyrene
 Concen: 30.278 ng/ul
 RT: 19.44 min Scan# 2797
 Delta R.T. -0.01 min
 Lab File: BM019525.D
 Acq: 28 Mar 2019 03:31

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	1270301		
101	16.1	6.9	10.3#	
100	13.1	5.6	8.4#	

