

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
 Data File : BM019509.D
 Acq On : 27 Mar 2019 17:41
 Operator : JU/SJ
 Sample : K2063-06MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	59	67	76	rVB	4600156	6916226	4.31%	0.695%
2	3.634	102	110	121	rVB	3412959	6135523	3.82%	0.616%
3	3.863	137	149	153	rBV3	46804276	149040947	92.84%	14.966%
4	3.993	165	171	175	rBV2	539463	1019826	0.64%	0.102%
5	4.128	189	194	209	rVB	5702931	8600656	5.36%	0.864%
6	4.440	242	247	259	rBV	1260736	2250091	1.40%	0.226%
7	4.604	270	275	285	rBV	2180089	3826061	2.38%	0.384%
8	4.781	300	305	309	rVV	3112660	5064131	3.15%	0.509%
9	4.834	309	314	329	rVB	4570291	8331490	5.19%	0.837%
10	5.063	345	353	356	rBV	562697	914243	0.57%	0.092%
11	5.128	356	364	372	rVB2	31838252	59991285	37.37%	6.024%
12	5.281	377	390	397	rVV2	46667920	160530763	100.00%	16.120%
13	5.410	409	412	417	rVB	550207	787213	0.49%	0.079%
14	5.540	427	434	439	rBV2	581886	1089502	0.68%	0.109%
15	5.640	439	451	455	rBV3	43337067	96422289	60.06%	9.682%
16	5.704	455	462	464	rVV	2125084	2934396	1.83%	0.295%
17	5.734	464	467	472	rVB	2633694	3565448	2.22%	0.358%
18	6.081	517	526	539	rBV2	2945496	5956996	3.71%	0.598%
19	6.263	552	557	565	rVB	1377527	2115607	1.32%	0.212%
20	6.434	580	586	589	rBV3	533810	972972	0.61%	0.098%
21	6.563	603	608	618	rVB	6278898	9441677	5.88%	0.948%
22	6.687	618	629	633	rBV	25549842	42721486	26.61%	4.290%
23	6.740	633	638	644	rVB	12154918	16489719	10.27%	1.656%
24	6.816	644	651	656	rBV	13203706	19331196	12.04%	1.941%
25	6.975	666	678	683	rBV	12251680	18743079	11.68%	1.882%
26	7.134	701	705	708	rBV	362762	600138	0.37%	0.060%
27	7.175	708	712	716	rVB5	573400	895290	0.56%	0.090%
28	7.251	716	725	733	rVB2	35865380	71324363	44.43%	7.162%
29	7.322	733	737	747	rVB2	566879	1088044	0.68%	0.109%
30	7.622	778	788	791	rBV4	1234378	2962583	1.85%	0.297%
31	7.657	791	794	795	rBV	612893	626314	0.39%	0.063%
32	7.698	795	801	807	rVB	14835607	23287937	14.51%	2.339%
33	7.763	807	812	819	rVB	399219	637502	0.40%	0.064%
34	7.840	819	825	828	rBV	1807632	3028138	1.89%	0.304%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
 Data File : BM019509.D
 Acq On : 27 Mar 2019 17:41
 Operator : JU/SJ
 Sample : K2063-06MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	7.881	828	832	838	rVB	2089383	3122600	1.95%	0.314%
36	7.957	838	845	850	rBV	13750920	22025484	13.72%	2.212%
37	8.063	857	863	867	rBV2	1834056	2820182	1.76%	0.283%
38	8.116	867	872	878	rVV	6783088	10158525	6.33%	1.020%
39	8.210	882	888	892	rBV	4994846	7507328	4.68%	0.754%
40	8.257	892	896	903	rVB	1863216	2951702	1.84%	0.296%
41	8.369	910	915	918	rBV	1128906	1788224	1.11%	0.180%
42	8.522	930	941	945	rBV	2814723	4783180	2.98%	0.480%
43	8.575	945	950	959	rVB	2485258	3839565	2.39%	0.386%
44	8.675	960	967	976	rBV	5563424	11029933	6.87%	1.108%
45	8.757	976	981	986	rBV2	3656375	6048689	3.77%	0.607%
46	8.928	1004	1010	1017	rVB8	363391	920451	0.57%	0.092%
47	9.004	1017	1023	1027	rBV	1254774	2304186	1.44%	0.231%
48	9.192	1049	1055	1060	rVB	2329393	3404109	2.12%	0.342%
49	9.251	1060	1065	1072	rVB	3476441	5173378	3.22%	0.519%
50	9.363	1072	1084	1087	rBV6	609638	1678225	1.05%	0.169%
51	9.404	1087	1091	1095	rVB	516176	686982	0.43%	0.069%
52	9.451	1095	1099	1101	rBV2	725279	1138672	0.71%	0.114%
53	9.616	1112	1127	1135	rBV	3578668	7657266	4.77%	0.769%
54	9.763	1139	1152	1160	rBV2	6526798	12801730	7.97%	1.286%
55	9.886	1166	1173	1181	rBV4	527062	1668796	1.04%	0.168%
56	10.004	1188	1193	1199	rVB2	1141602	2047131	1.28%	0.206%
57	10.086	1199	1207	1215	rVB2	648998	1420744	0.89%	0.143%
58	10.239	1228	1233	1238	rBV2	642689	1172308	0.73%	0.118%
59	10.316	1242	1246	1249	rBV2	619902	871682	0.54%	0.088%
60	10.351	1249	1252	1258	rVV2	543776	994046	0.62%	0.100%
61	10.439	1258	1267	1272	rVV	19324412	35376455	22.04%	3.552%
62	10.545	1279	1285	1295	rVB2	1287069	2539268	1.58%	0.255%
63	10.828	1320	1333	1339	rVB7	368709	1204669	0.75%	0.121%
64	11.010	1339	1364	1370	rBV4	2028327	8031620	5.00%	0.807%
65	11.092	1371	1378	1385	rVV2	753662	1793348	1.12%	0.180%
66	11.269	1395	1408	1419	rVV5	1058066	3261075	2.03%	0.327%
67	11.386	1419	1428	1435	rVV4	475723	1524062	0.95%	0.153%
68	11.469	1435	1442	1452	rVV4	515350	1731149	1.08%	0.174%
69	11.557	1452	1457	1462	rVV2	384066	835537	0.52%	0.084%
70	11.610	1462	1466	1471	rVV2	317365	655124	0.41%	0.066%
71	11.692	1471	1480	1485	rVV4	989021	1990564	1.24%	0.200%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
 Data File : BM019509.D
 Acq On : 27 Mar 2019 17:41
 Operator : JU/SJ
 Sample : K2063-06MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

72	11.751	1485	1490	1492	rVV2	488393	929863	0.58%	0.093%
73	11.786	1492	1496	1503	rVV	2176389	3591296	2.24%	0.361%
74	11.939	1517	1522	1531	rVV2	341387	714965	0.45%	0.072%
75	12.045	1533	1540	1549	rVV	7311591	11352183	7.07%	1.140%
76	12.251	1566	1575	1584	rVV2	7026078	16419877	10.23%	1.649%
77	12.369	1584	1595	1601	rVV3	1213114	3810998	2.37%	0.383%
78	12.445	1601	1608	1617	rVB7	629516	1679713	1.05%	0.169%
79	12.575	1622	1630	1635	rBV3	309207	635123	0.40%	0.064%
80	12.645	1635	1642	1644	rBV4	482046	898872	0.56%	0.090%
81	13.122	1719	1723	1734	rVB2	863944	1420463	0.88%	0.143%
82	13.222	1734	1740	1744	rBV	381871	613820	0.38%	0.062%
83	13.392	1764	1769	1772	rBV2	835749	1280142	0.80%	0.129%
84	13.427	1772	1775	1780	rVV2	711671	1070988	0.67%	0.108%
85	13.563	1789	1798	1803	rBV	302113	624176	0.39%	0.063%
86	13.669	1811	1816	1822	rVB	1304427	1782589	1.11%	0.179%
87	13.939	1857	1862	1870	rBV	1451354	2121006	1.32%	0.213%
88	14.251	1906	1915	1920	rBV2	904186	1521392	0.95%	0.153%
89	14.316	1920	1926	1932	rBV	1654715	2330765	1.45%	0.234%
90	14.645	1977	1982	1990	rVV	788547	1235672	0.77%	0.124%
91	15.251	2079	2085	2090	rBV	1800629	2547904	1.59%	0.256%
92	15.398	2104	2110	2123	rBV	698534	1064844	0.66%	0.107%
93	16.657	2319	2324	2334	rVB	963863	1460190	0.91%	0.147%
94	17.010	2378	2384	2389	rBV	1052952	1539046	0.96%	0.155%
95	17.104	2395	2400	2408	rVB	1993387	2888735	1.80%	0.290%
96	19.415	2787	2793	2796	rBV	2508494	3769842	2.35%	0.379%
97	19.445	2796	2798	2806	rVB	2870908	3116096	1.94%	0.313%
98	21.215	3094	3099	3105	rBV	1662071	2045617	1.27%	0.205%
99	23.286	3444	3451	3463	rVB2	2323296	4382773	2.73%	0.440%
100	23.427	3469	3475	3488	rVB2	1242547	2392678	1.49%	0.240%


Sum of corrected areas: 995842748

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032719\
Data File : BM019509.D
Acq On : 27 Mar 2019 17:41
Operator : JU/SJ
Sample : K2063-06MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DB6R7MS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

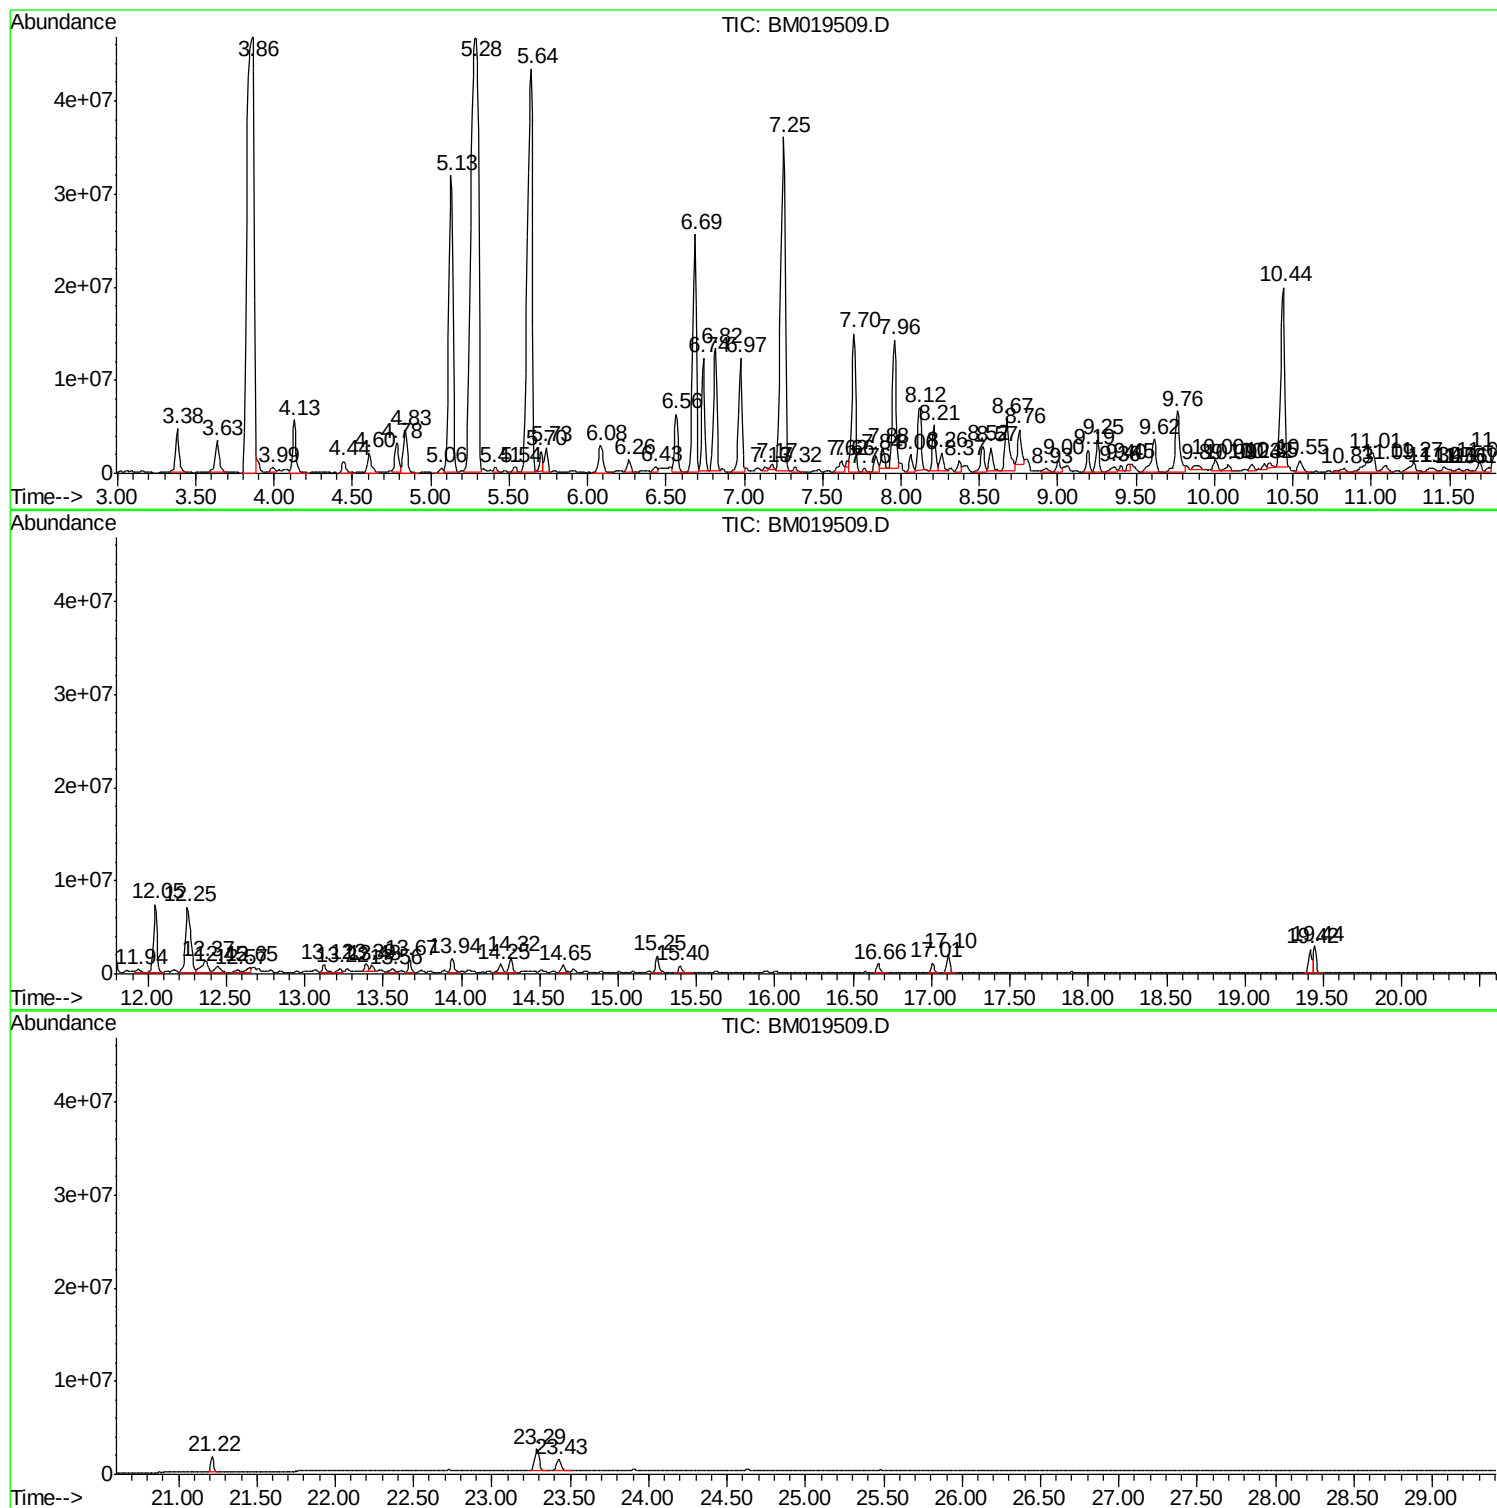

DbaaaPath::ZZ\SS0088RVNPE00001BBA\AMNDATA\B000322199\
 DbaaaFile::B00099009DD
 AcqQOn :227Mar2009 17441
 Operator::JUUSJ
 Sample::K00030000S
 Misc :
 ASSVal :55 SampleMultiplier:11

Instrument :
 BNA_M
 ClientSampleId :
 DB6R7MS

QcandMebdd::ZZ\SS0088RVNPE00001BBA\AMNDATA\B000322199\AMM
 QcandTitle::SS00ACALIBRATION

TICLibrary :CC\DATA\BASIS\SS002LL
 TICIntegrationParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
