

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032724\
 Data File : BM044785.D
 Acq On : 27 Mar 2024 18:44
 Operator : MA/JU
 Sample : P1830-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-206

Quant Time: Mar 28 01:00:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 14 02:28:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	172484	20.000	ng	-0.02
21) Naphthalene-d8	10.463	136	632544	20.000	ng	-0.02
39) Acenaphthene-d10	14.333	164	326274	20.000	ng	-0.02
64) Phenanthrene-d10	17.086	188	565699	20.000	ng	-0.02
76) Chrysene-d12	21.286	240	500509	20.000	ng	-0.02
86) Perylene-d12	23.539	264	594973	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.299	112	1560549	129.902	ng	0.00
7) Phenol-d6	6.869	99	1735601	112.299	ng	-0.01
23) Nitrobenzene-d5	8.851	82	1310803	99.833	ng	-0.01
42) 2,4,6-Tribromophenol	15.833	330	531993	147.830	ng	-0.01
45) 2-Fluorobiphenyl	12.945	172	2357632	99.517	ng	-0.02
79) Terphenyl-d14	19.733	244	2685273	93.854	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032724\
Data File : BM044785.D
Acq On : 27 Mar 2024 18:44
Operator : MA/JU
Sample : P1830-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-206

Quant Time: Mar 28 01:00:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration




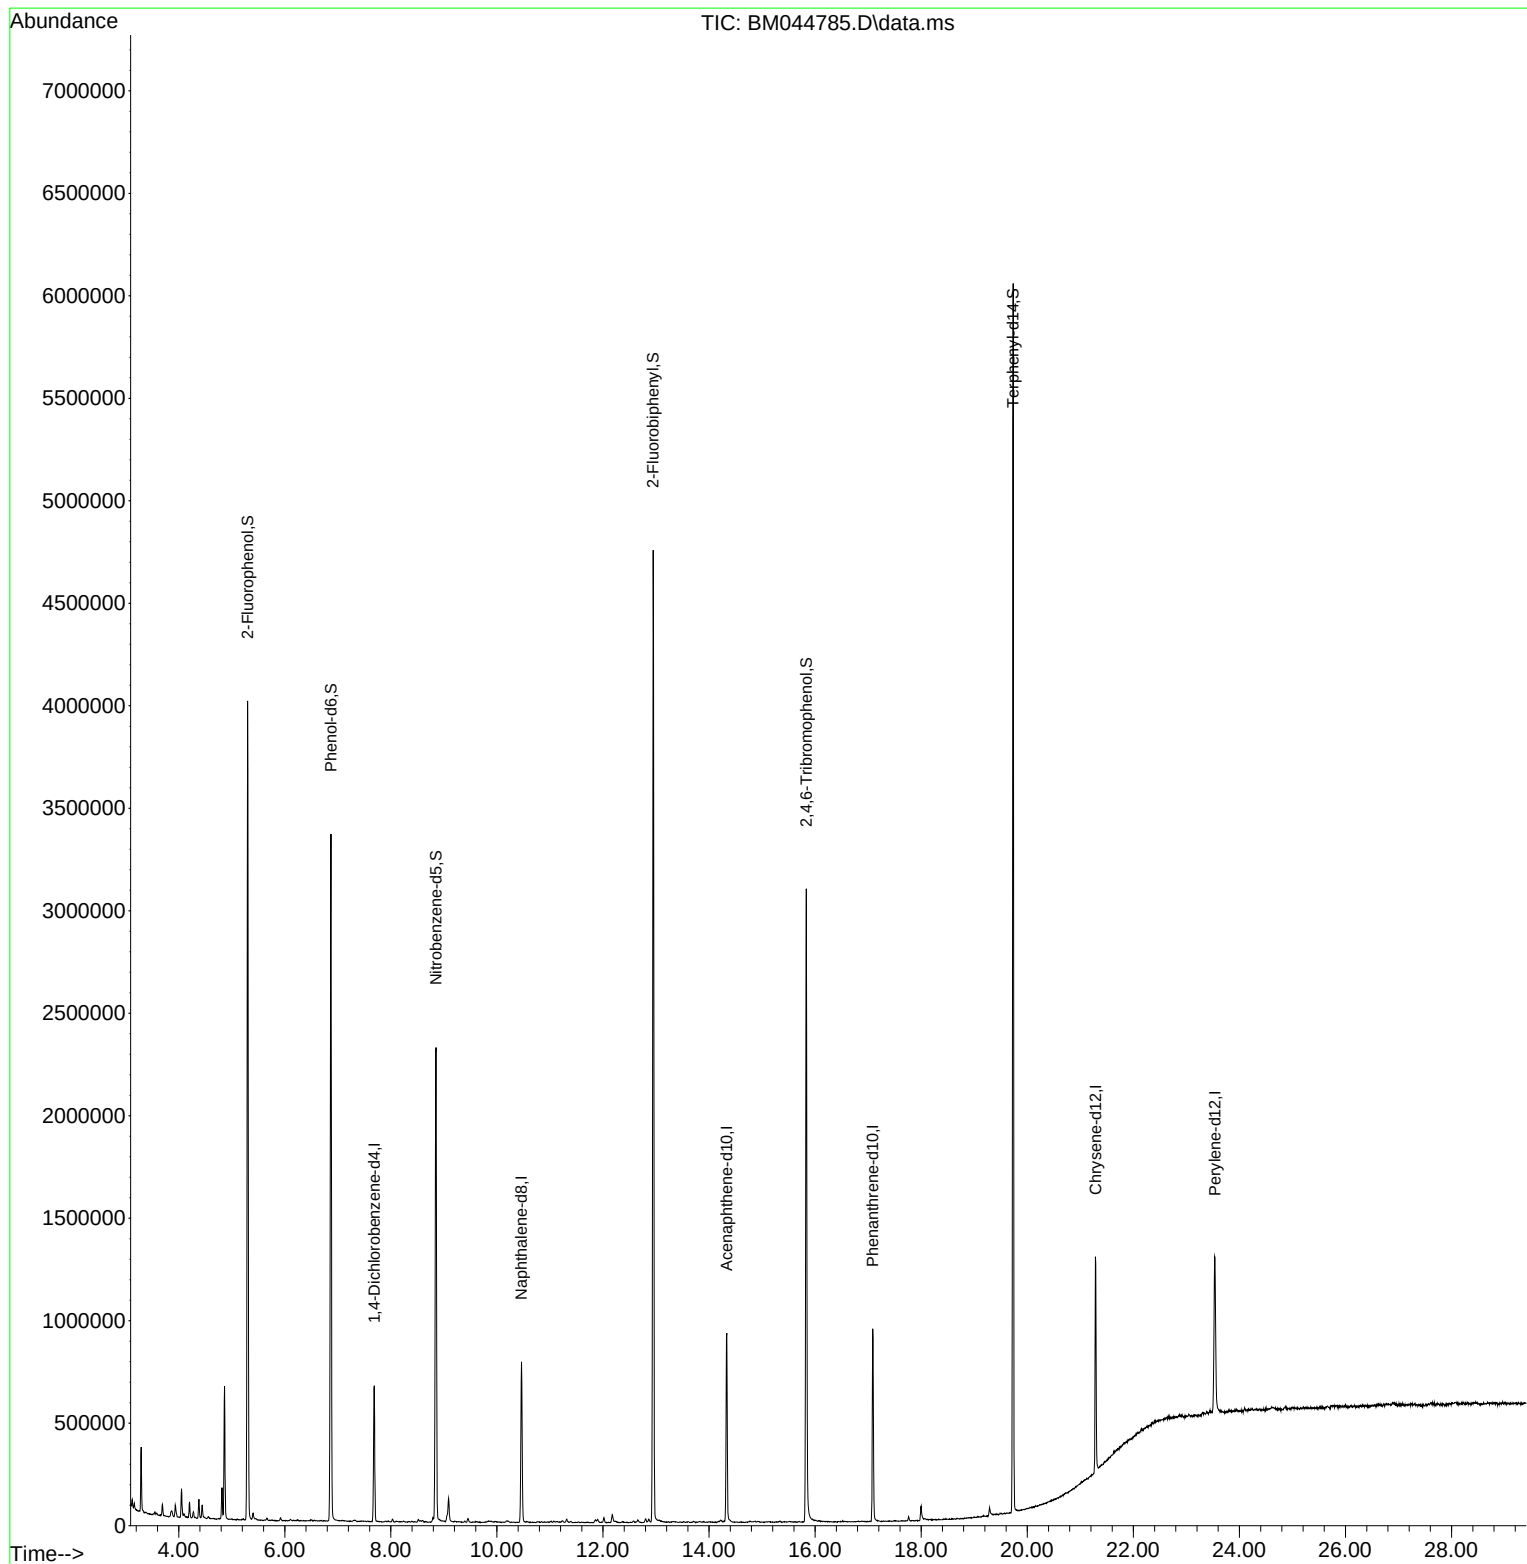


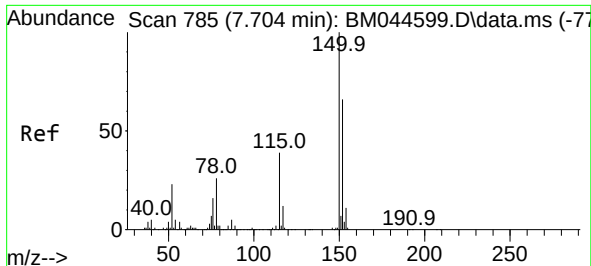

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.687 min Scan# 71
 Delta R.T. -0.017 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44




Instrument :
 BNA_M
 ClientSampleId :
 VNJ-206


Tgt Ion:152 Resp: 172484
 Ion Ratio Lower Upper
 152 100
 150 156.2 121.9 182.9
 115 58.2 47.1 70.7

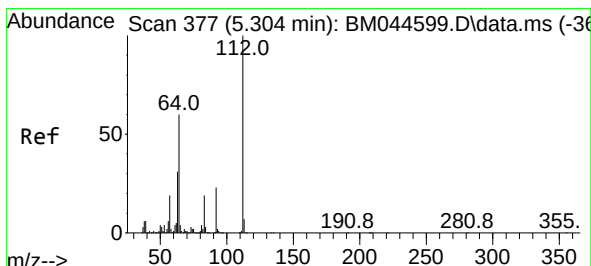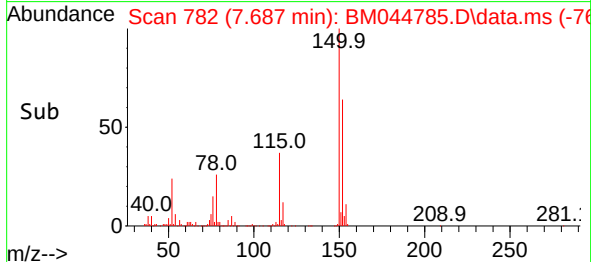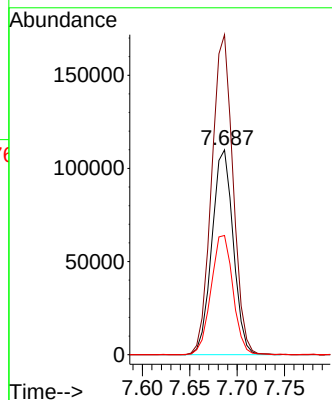

#5
 2-Fluorophenol
 Concen: 129.902 ng
 RT: 5.299 min Scan# 376
 Delta R.T. -0.006 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44

Tgt Ion:112 Resp: 1560549
 Ion Ratio Lower Upper
 112 100
 64 60.8 47.9 71.9
 63 34.4 25.0 37.4


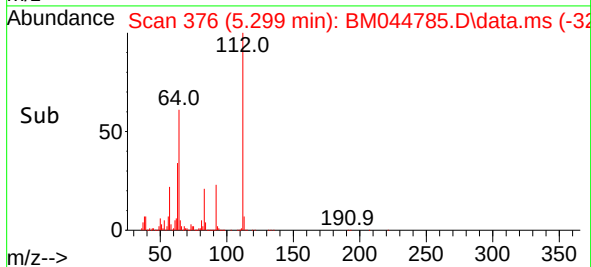
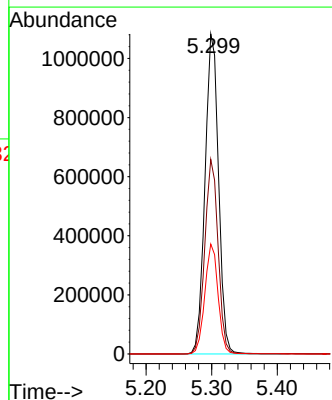
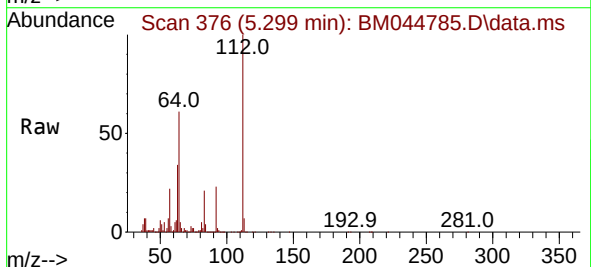


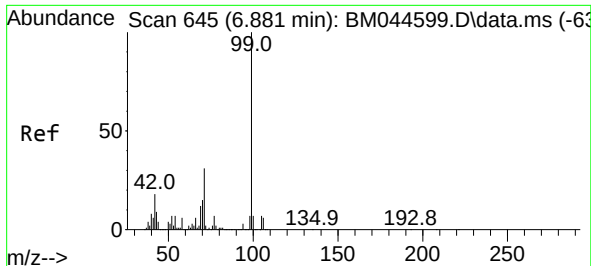

#7
Phenol-d6
Concen: 112.299 ng
RT: 6.869 min Scan# 64
Delta R.T. -0.012 min
Lab File: BM044785.D
Acq: 27 Mar 2024 18:44




Instrument :
BNA_M
ClientSampleId :
VNJ-206


Tgt Ion: 99 Resp: 1735601
Ion Ratio Lower Upper
99 100
42 22.0 14.3 21.5#
71 35.0 24.5 36.7

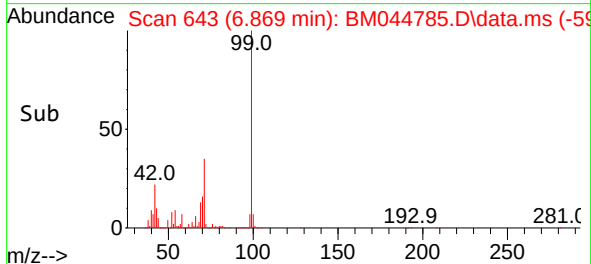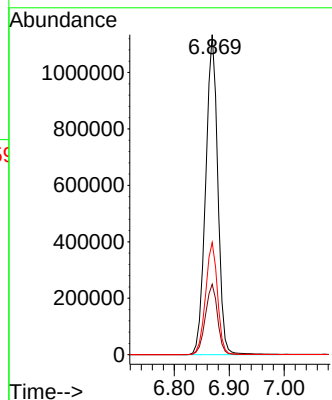

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.463 min Scan# 1254
Delta R.T. -0.023 min
Lab File: BM044785.D
Acq: 27 Mar 2024 18:44

Tgt Ion:136 Resp: 632544
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 8.8 6.6 10.0
68 5.8 5.0 7.4


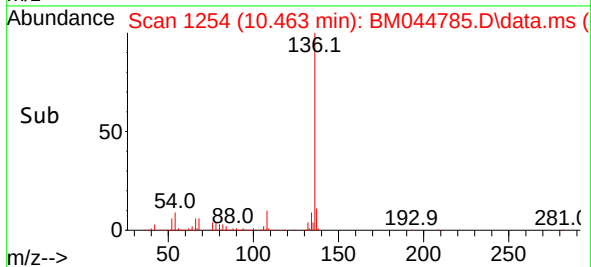
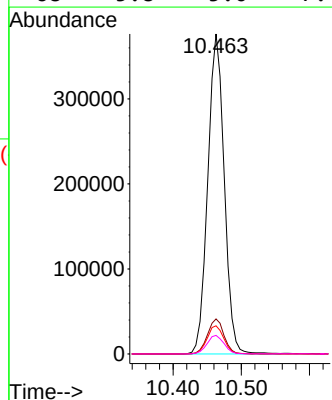
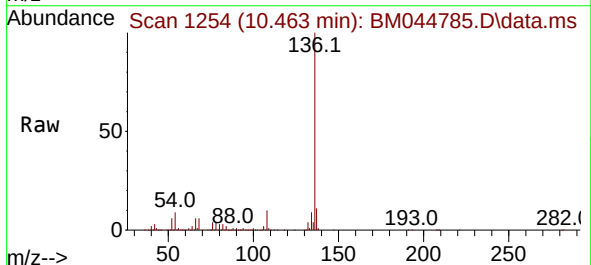


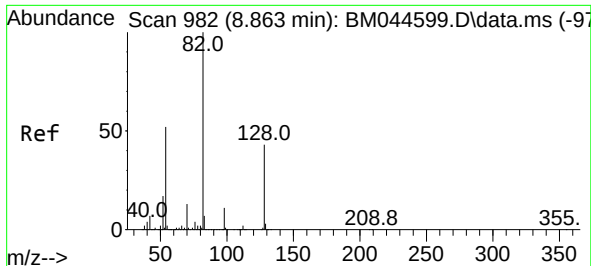

#23
 Nitrobenzene-d5
 Concen: 99.833 ng
 RT: 8.851 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44




Instrument :
 BNA_M
 ClientSampleId :
 VNJ-206


Tgt Ion: 82 Resp: 1310803
 Ion Ratio Lower Upper
 82 100
 128 43.6 34.2 51.4
 54 54.9 41.3 61.9

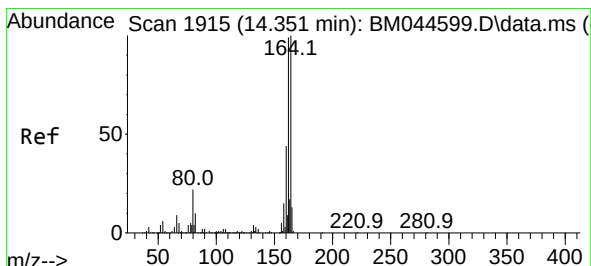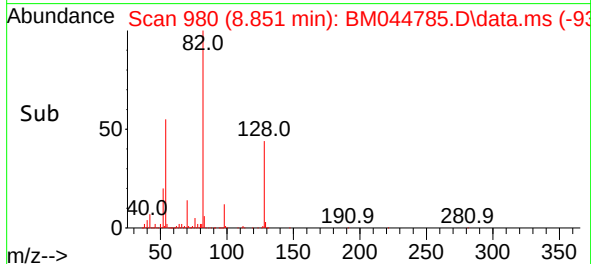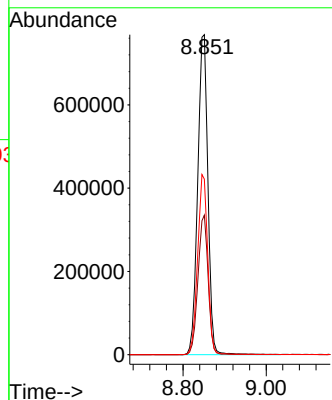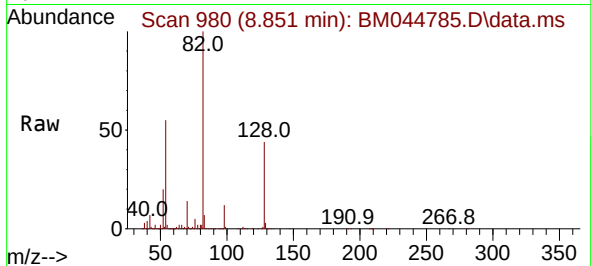

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.333 min Scan# 1912
 Delta R.T. -0.018 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44

Tgt Ion:164 Resp: 326274
 Ion Ratio Lower Upper
 164 100
 162 100.0 79.3 118.9
 160 43.7 35.2 52.8


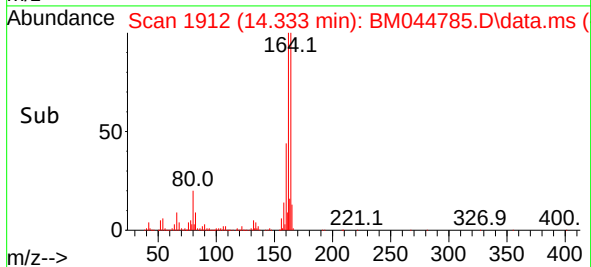
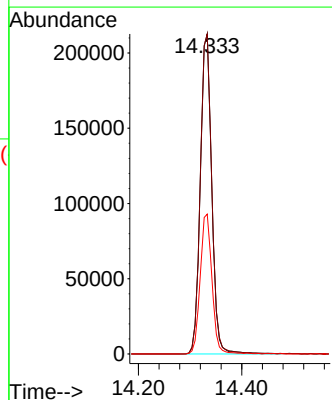
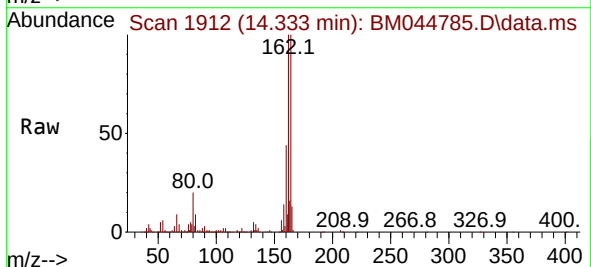




#42
2,4,6-Tribromophenol
Concen: 147.830 ng
RT: 15.833 min Scan# 2167
Delta R.T. -0.012 min
Lab File: BM044785.D
Acq: 27 Mar 2024 18:44




Instrument :
BNA_M
ClientSampleId :
VNJ-206


Tgt Ion:330 Resp: 531993
Ion Ratio Lower Upper
330 100
332 97.1 77.8 116.8
141 42.5 33.4 50.0

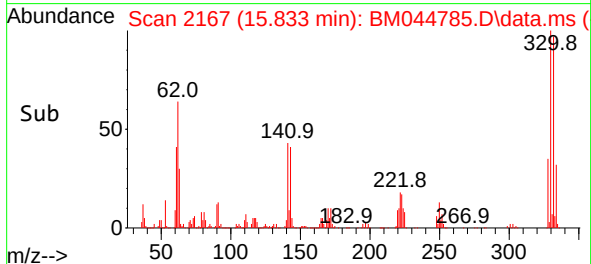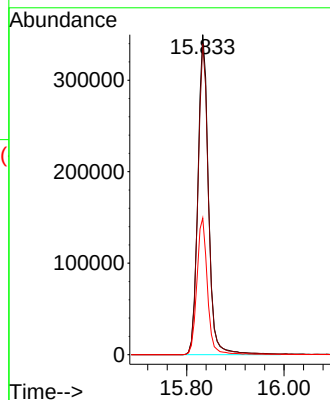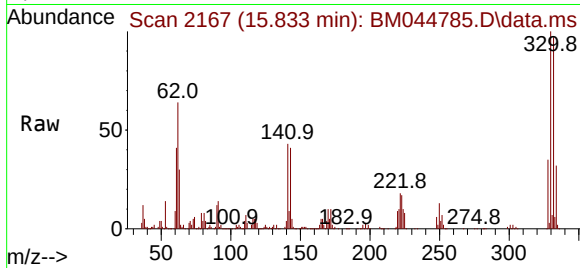

#45
2-Fluorobiphenyl
Concen: 99.517 ng
RT: 12.945 min Scan# 1676
Delta R.T. -0.023 min
Lab File: BM044785.D
Acq: 27 Mar 2024 18:44

Tgt Ion:172 Resp: 2357632
Ion Ratio Lower Upper
172 100
171 35.2 28.2 42.2
170 23.7 19.0 28.6

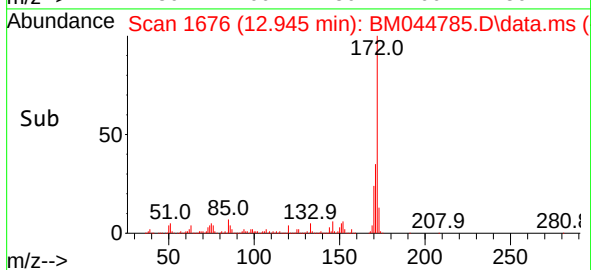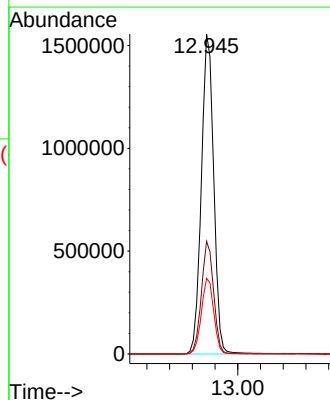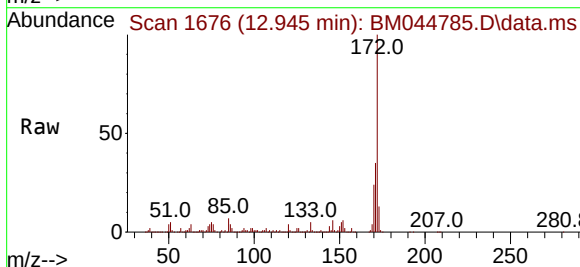



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.086 min Scan# 21

Delta R.T. -0.018 min

Lab File: BM044785.D

Acq: 27 Mar 2024 18:44

Instrument :

BNA_M

ClientSampleId :

VNJ-206





Tgt Ion:188 Resp: 565699

Ion Ratio Lower Upper

188 100

94 9.9 8.4 12.6

80 10.6 9.4 14.0

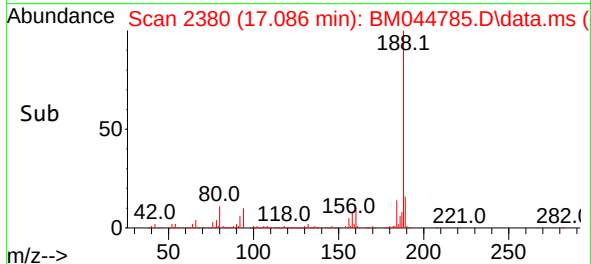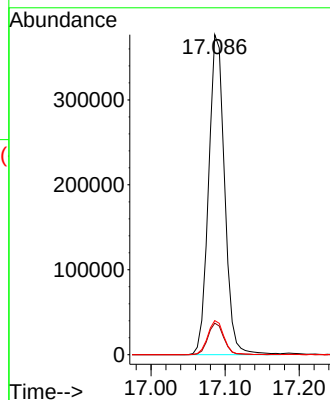

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.286 min Scan# 3094

Delta R.T. -0.018 min

Lab File: BM044785.D

Acq: 27 Mar 2024 18:44




Tgt Ion:240 Resp: 500509


Ion Ratio Lower Upper

240 100

120 12.9 9.7 14.5

236 26.3 21.0 31.4


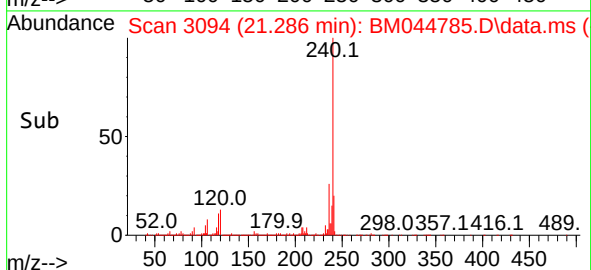
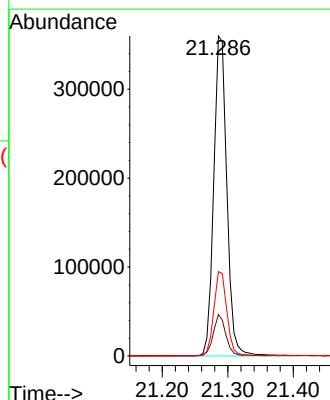
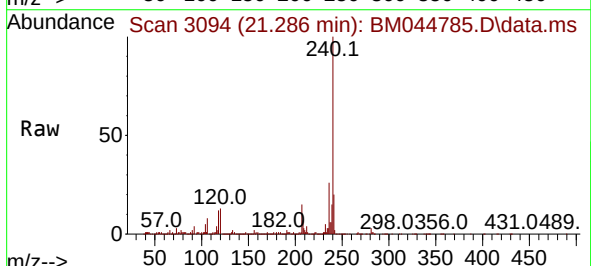


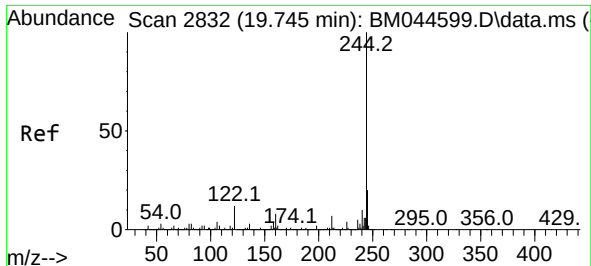

#79
 Terphenyl-d14
 Concen: 93.854 ng
 RT: 19.733 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-206

Tgt Ion:244 Resp: 2685273
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.5 8.3
 122 10.7 9.7 14.5

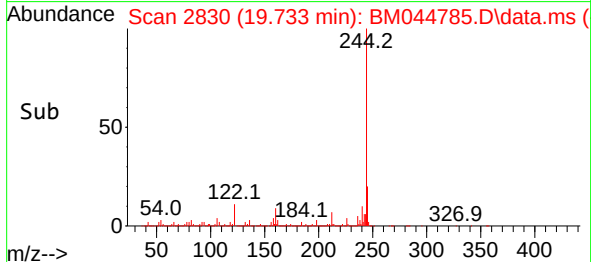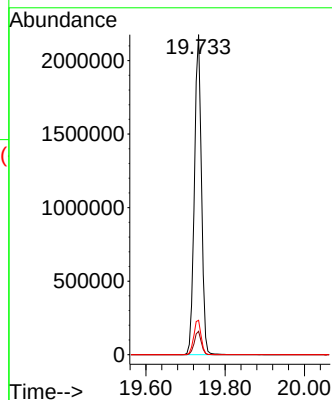

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.539 min Scan# 3477
 Delta R.T. -0.012 min
 Lab File: BM044785.D
 Acq: 27 Mar 2024 18:44

Tgt Ion:264 Resp: 594973
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.3 27.5
 265 22.7 17.5 26.3

