


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032724\
Data File : BM044776.D
Acq On : 27 Mar 2024 13:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 02:28:24 2024

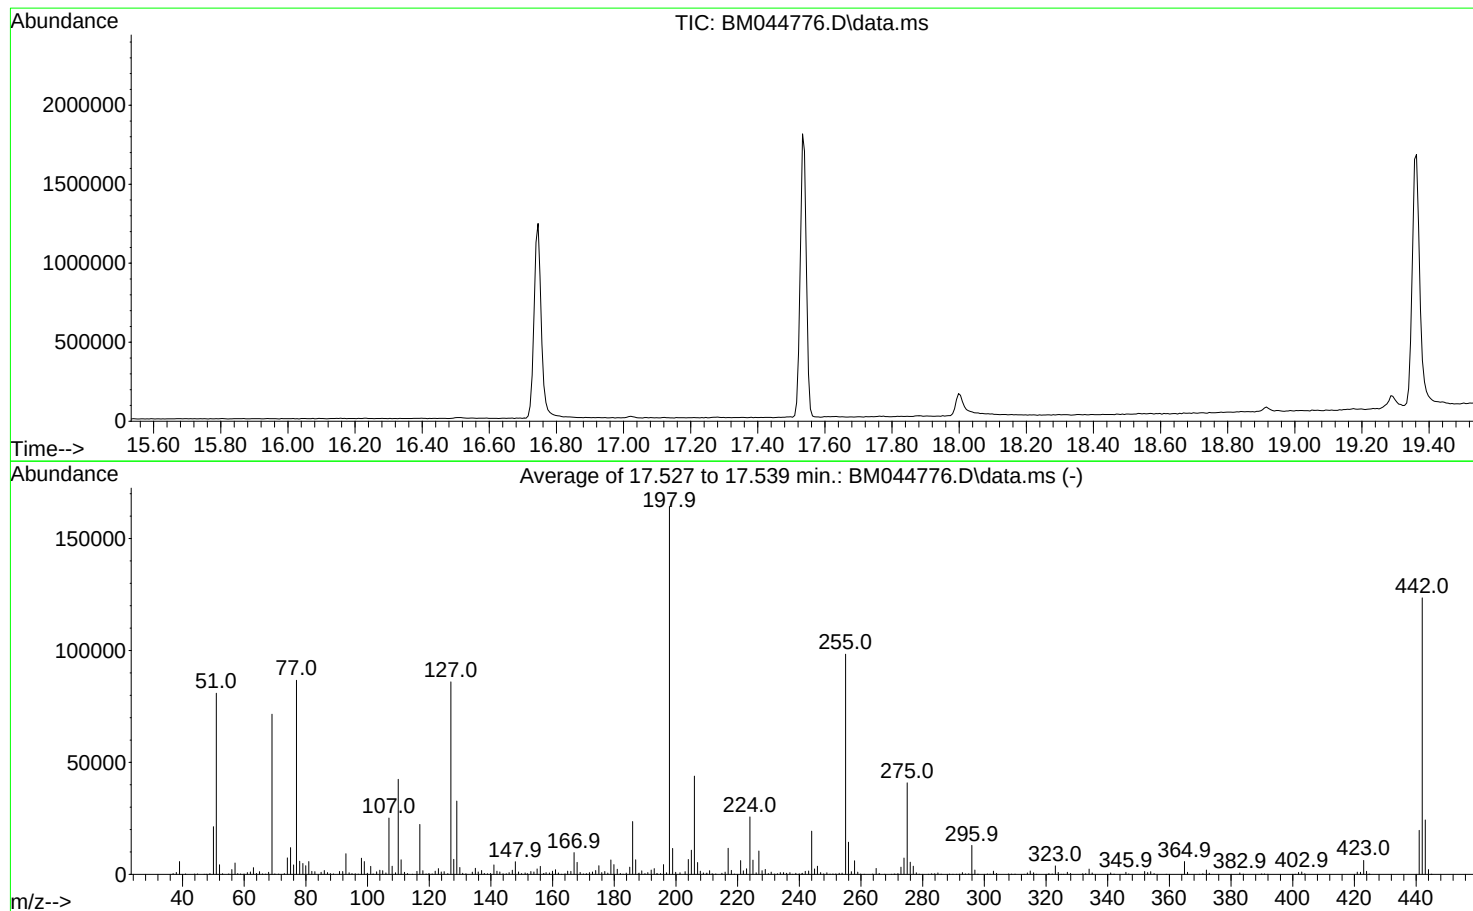




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	80879	PASS
68	69	0.00	2	1.3	962	PASS
69	198	0.00	100	43.5	71531	PASS
70	69	0.00	2	0.4	252	PASS
127	198	10	80	52.3	85965	PASS
197	198	0.00	2	0.4	719	PASS
198	198	100	100	100.0	164315	PASS
199	198	5	9	7.1	11614	PASS
275	198	10	60	24.9	40880	PASS
365	198	1	100	3.5	5703	PASS
441	198	0.01	100	11.9	19626	PASS
442	442	50	100	100.0	123491	PASS
443	442	15	24	19.7	24314	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032724\
Data File : BM044776.D
Acq On : 27 Mar 2024 13:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 28 02:58:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

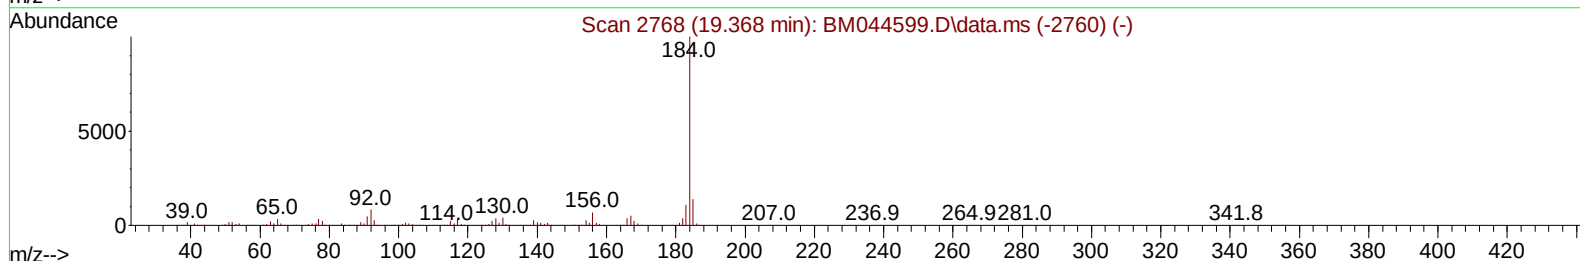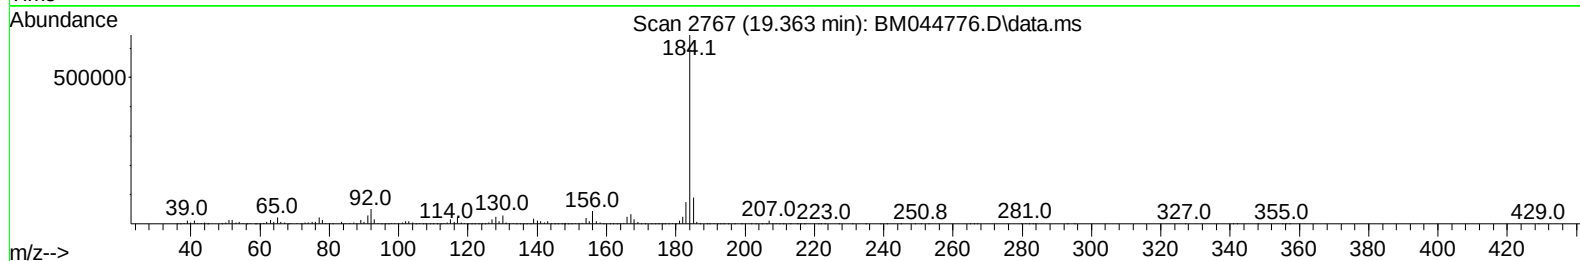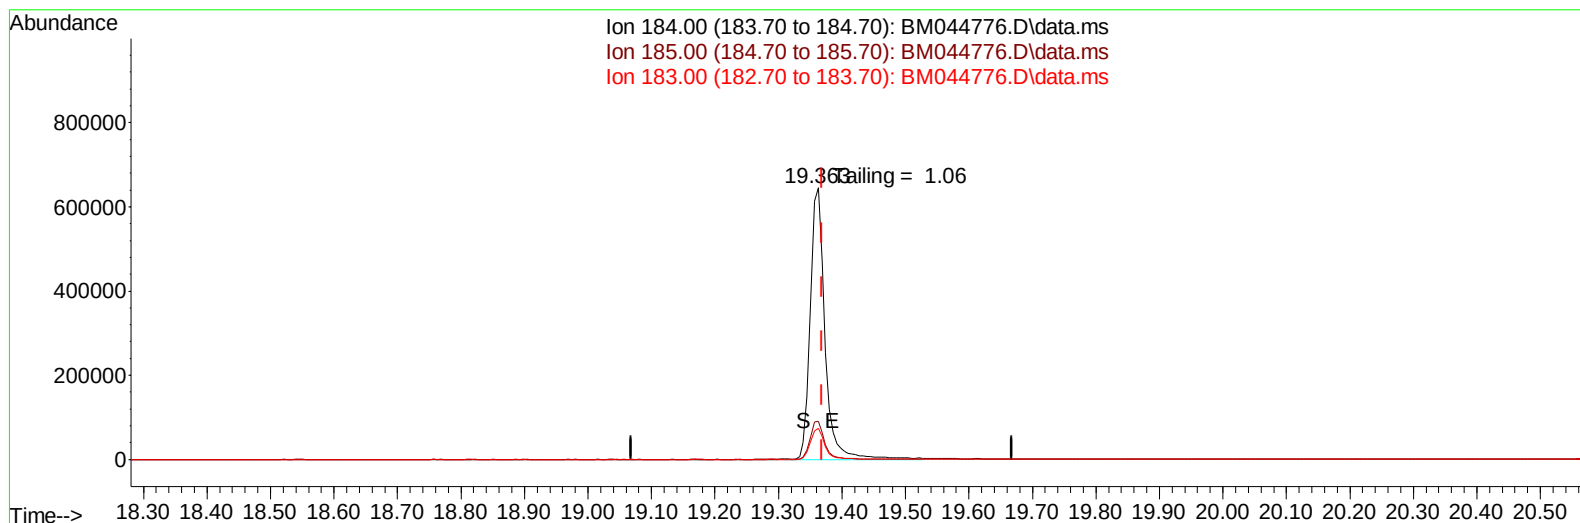

TIC: BM044776.D\data.ms

(77) Benzidine

19.363min (-0.005) 29574.93 ng

response 1047952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.02
183.00	10.90	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/27/2024	BNA_M	<u>BM044776.D</u>
Compound Name	Response	Retention Time
DDT	505101	20.592
DDD	37360	20.151
DDE	1891	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39251	544352	7.21

Instrument :
BNA_M
ClientSampleId :
DFTPP