

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032819\
 Data File : BM019564.D
 Acq On : 29 Mar 2019 05:15
 Operator : JU/SJ
 Sample : K2063-04DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB6R6DL

Quant Time: Mar 29 06:55:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 06:50:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	117347	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	518156	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	307264	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	686815	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	818077	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1027808	20.00	ng/ul	0.00

System Monitoring Compounds


3) 1,4-Dioxane-d8	3.16	96	259	0.09	ng/uL	0.04
5) Phenol-d5	6.78	99	7695	0.74	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.94	67	22906	3.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	21579	2.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	13167	1.68	ng/ul	0.02
19) Nitrobenzene-d5	8.76	128	16337	4.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	11804	2.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	21162	2.73	ng/ul	0.02
29) 4-Chloroaniline-d4	10.56	131	369	0.04	ng/ul	0.04
44) Dimethylphthalate-d6	13.66	166	83390	3.36	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	97925	3.16	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.24	176	75486	3.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	7580	1.67	ng/ul	0.01
71) Anthracene-d10	17.10	188	108778	3.30	ng/ul	0.00
79) Pyrene-d10	19.41	212	125759	3.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	170983	3.14	ng/ul	0.00

Target Compounds

					Qvalue	
4) Benzaldehyde	6.72	77	80989	10.820	ng/ul#	1
14) Acetophenone	8.43	105	14259	1.116	ng/ul	96
17) Hexachloroethane	8.66	117	58629	17.327	ng/ul#	1
28) Naphthalene	10.41	128	1157343	43.116	ng/ul	99
34) 2-Methylnaphthalene	12.03	142	195697	10.405	ng/ul	98
35) 1-Methylnaphthalene	12.25	142	102871	5.792	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032819\
Data File : BM019564.D
Acq On    : 29 Mar 2019   05:15
Operator  : JU/SJ
Sample    : K2063-04DL 10X
Misc      :
ALS Vial  : 26      Sample Multiplier: 1
```

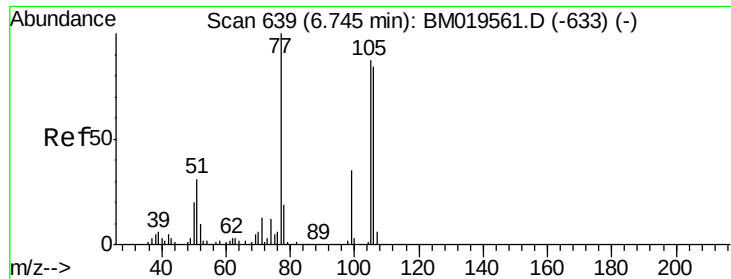

#4

Benzaldehyde

Concen: 10.820 ng/ul

RT: 6.72 min Scan# 635

Delta R.T. -0.02 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15

Instrument :

BNA_M

ClientSampleId :

DB6R6DL





Tgt Ion: 77 Resp: 80989

Ion Ratio Lower Upper

77 100

105 777.5 71.0 106.6#

106 69.6 69.5 104.3

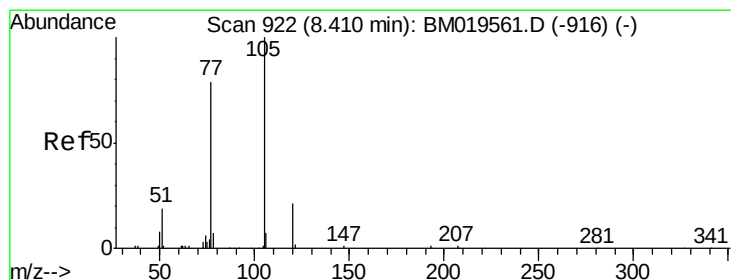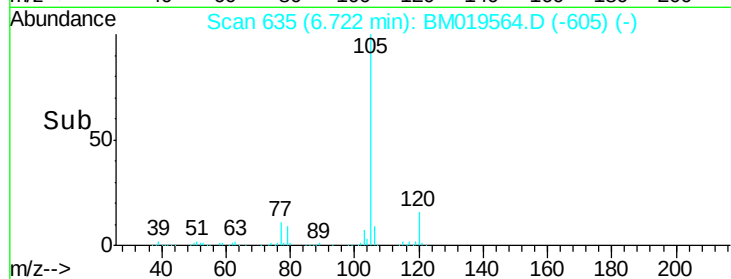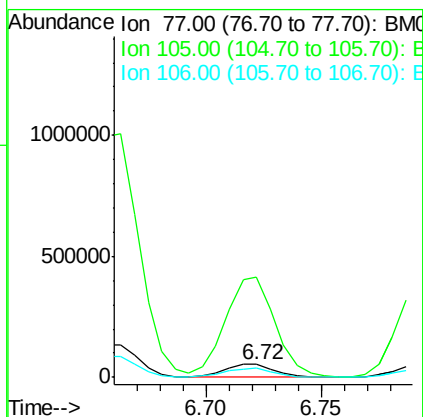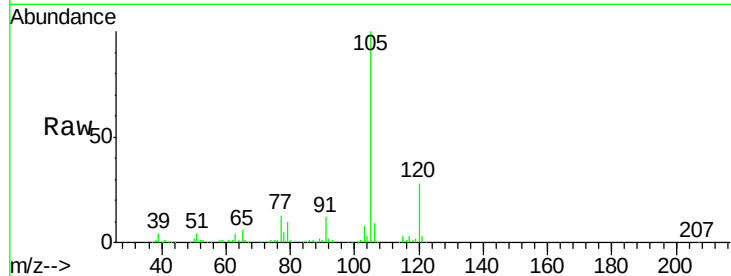

#14

Acetophenone

Concen: 1.116 ng/ul

RT: 8.43 min Scan# 925

Delta R.T. 0.02 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15




Tgt Ion: 105 Resp: 14259


Ion Ratio Lower Upper

105 100

77 81.9 63.2 94.8

51 21.2 19.8 29.8

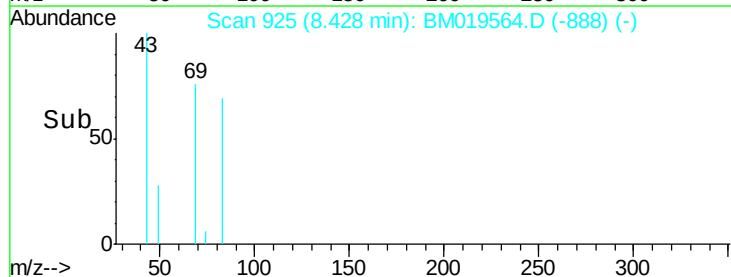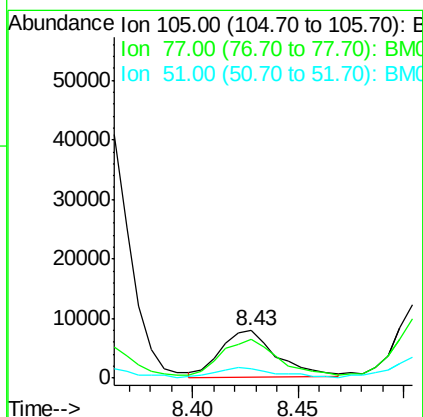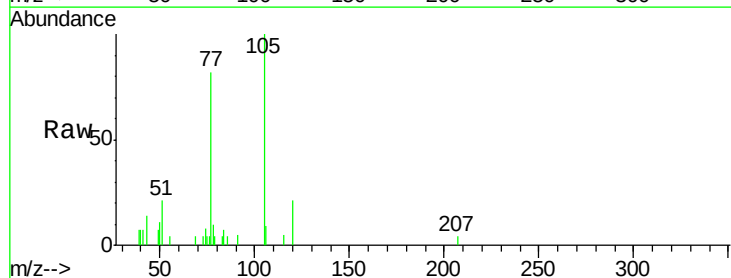

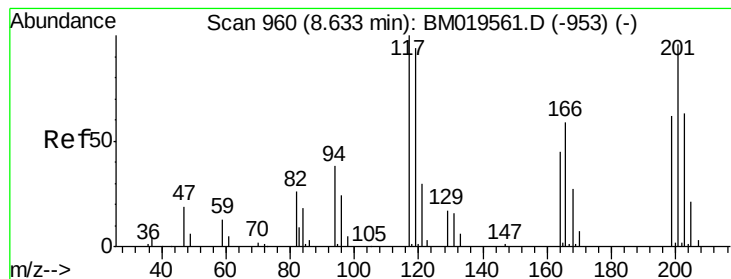

#17

Hexachloroethane

Concen: 17.327 ng/ul

RT: 8.66 min Scan# 965

Delta R.T. 0.03 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15

Instrument :

BNA_M

ClientSampled :

DB6R6DL


Tgt Ion:117 Resp: 58629

Ion Ratio Lower Upper

117 100

201 0.0 96.1 144.1#




199 0.0 59.7 89.5#

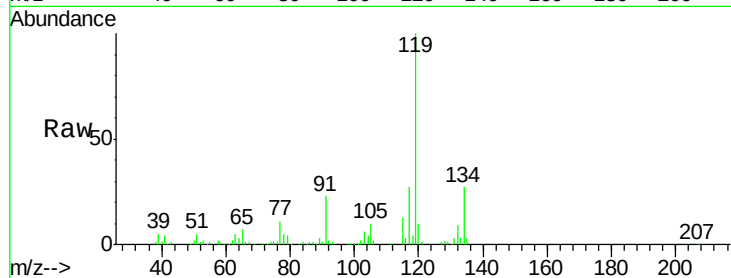

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

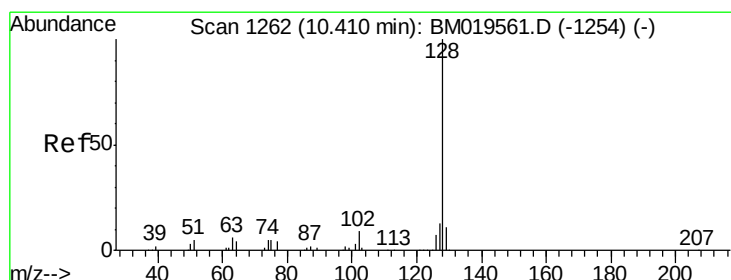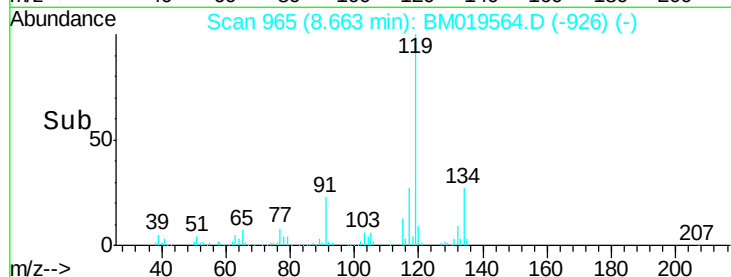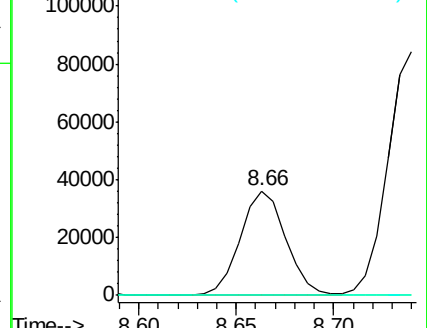

#28

Naphthalene

Concen: 43.116 ng/ul

RT: 10.41 min Scan# 1262

Delta R.T. 0.00 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15


Tgt Ion:128 Resp: 1157343

Ion Ratio Lower Upper

128 100

129 11.0 8.3 12.5



127 13.4 10.8 16.2

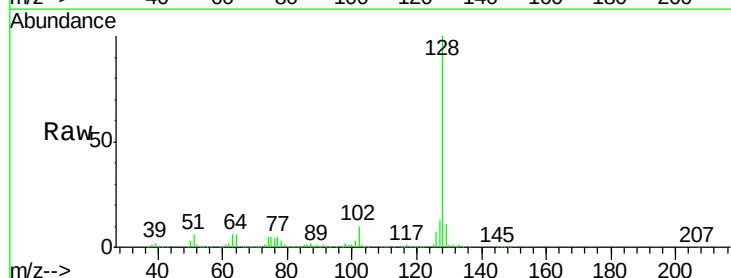


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

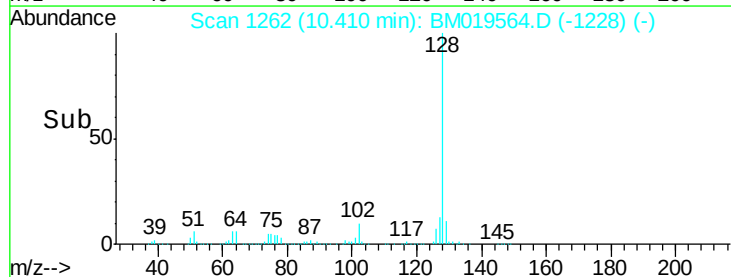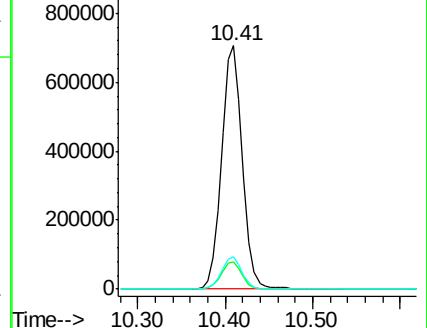

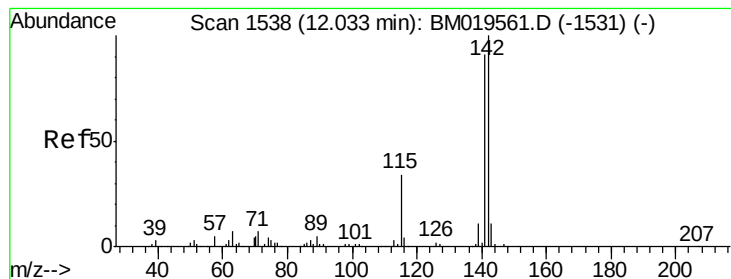

#34

2-Methylnaphthalene

Concen: 10.405 ng/ul

RT: 12.03 min Scan# 1538

Delta R.T. 0.00 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15

Instrument :

BNA_M

ClientSampleId :


DB6R6DL

Tgt Ion:142 Resp: 195697

Ion Ratio Lower Upper

142 100

141 90.9 71.4 107.2

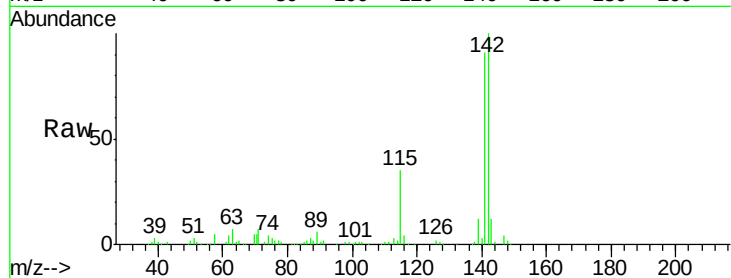

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E



12.03

100000

50000

0

Time--> 11.95 12.00 12.05 12.10

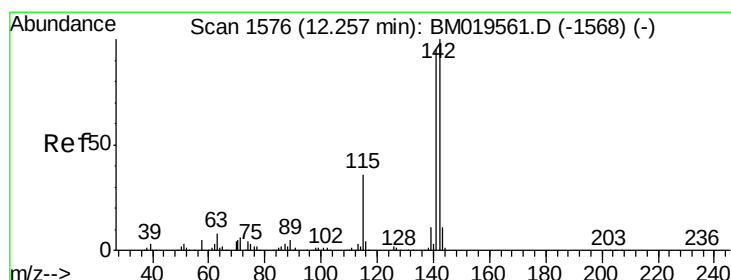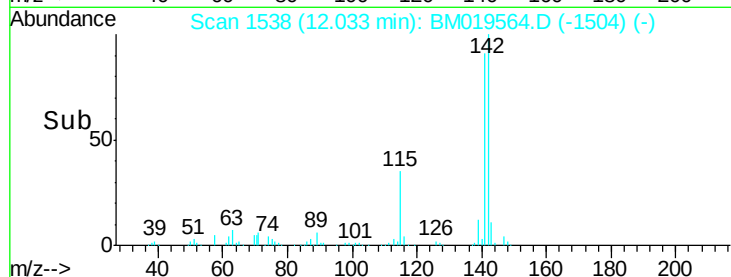

#35

1-Methylnaphthalene

Concen: 5.792 ng/ul

RT: 12.25 min Scan# 1575

Delta R.T. -0.01 min

Lab File: BM019564.D

Acq: 29 Mar 2019 05:15


Tgt Ion:142 Resp: 102871

Ion Ratio Lower Upper

142 100

141 91.5 76.6 115.0

116 3.9 3.6 5.4

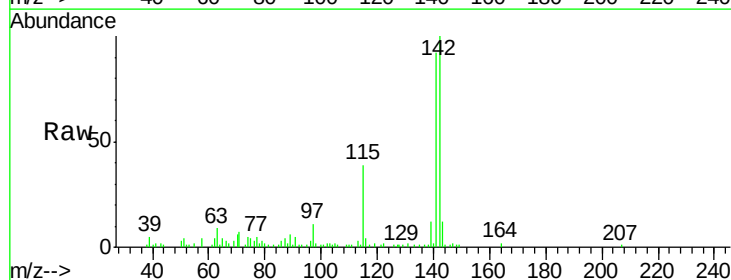

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

12.25

80000

60000

40000

20000

0

Time--> 12.20 12.25 12.30

