

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032819\
 Data File : BM019573.D
 Acq On : 29 Mar 2019 10:41
 Operator : JU/SJ
 Sample : K2052-17RX
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 29 11:26:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 09:53:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	93699	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	409657	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	253583	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	581985	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	698386	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	824949	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8080	3.38	ng/uL	0.00
5) Phenol-d5	6.86	99	671	0.08	ng/ul	0.10
7) Bis-(2-Chloroethyl)ether-d	6.93	67	155308	27.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	65205	10.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	19738	3.15	ng/ul	0.02
19) Nitrobenzene-d5	8.75	128	92792	31.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	81737	25.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	237948	38.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	2976	0.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	677344	33.10	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	4173	0.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	1130	0.35	ng/ul	0.07
58) Fluorene-d10	15.24	176	424216	24.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	59104	15.36	ng/ul	0.00
71) Anthracene-d10	17.10	188	13559	0.49	ng/ul	0.00
79) Pyrene-d10	19.42	212	548	0.02	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.27	264	1054	0.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Bis(2-Chloroethyl)ether	6.99	93	790241	118.636	ng/ul#	44




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032819\
Data File : BM019573.D
Acq On : 29 Mar 2019 10:41
Operator : JU/SJ
Sample : K2052-17RX
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 29 11:26:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 09:53:26 2019
Response via : Initial Calibration

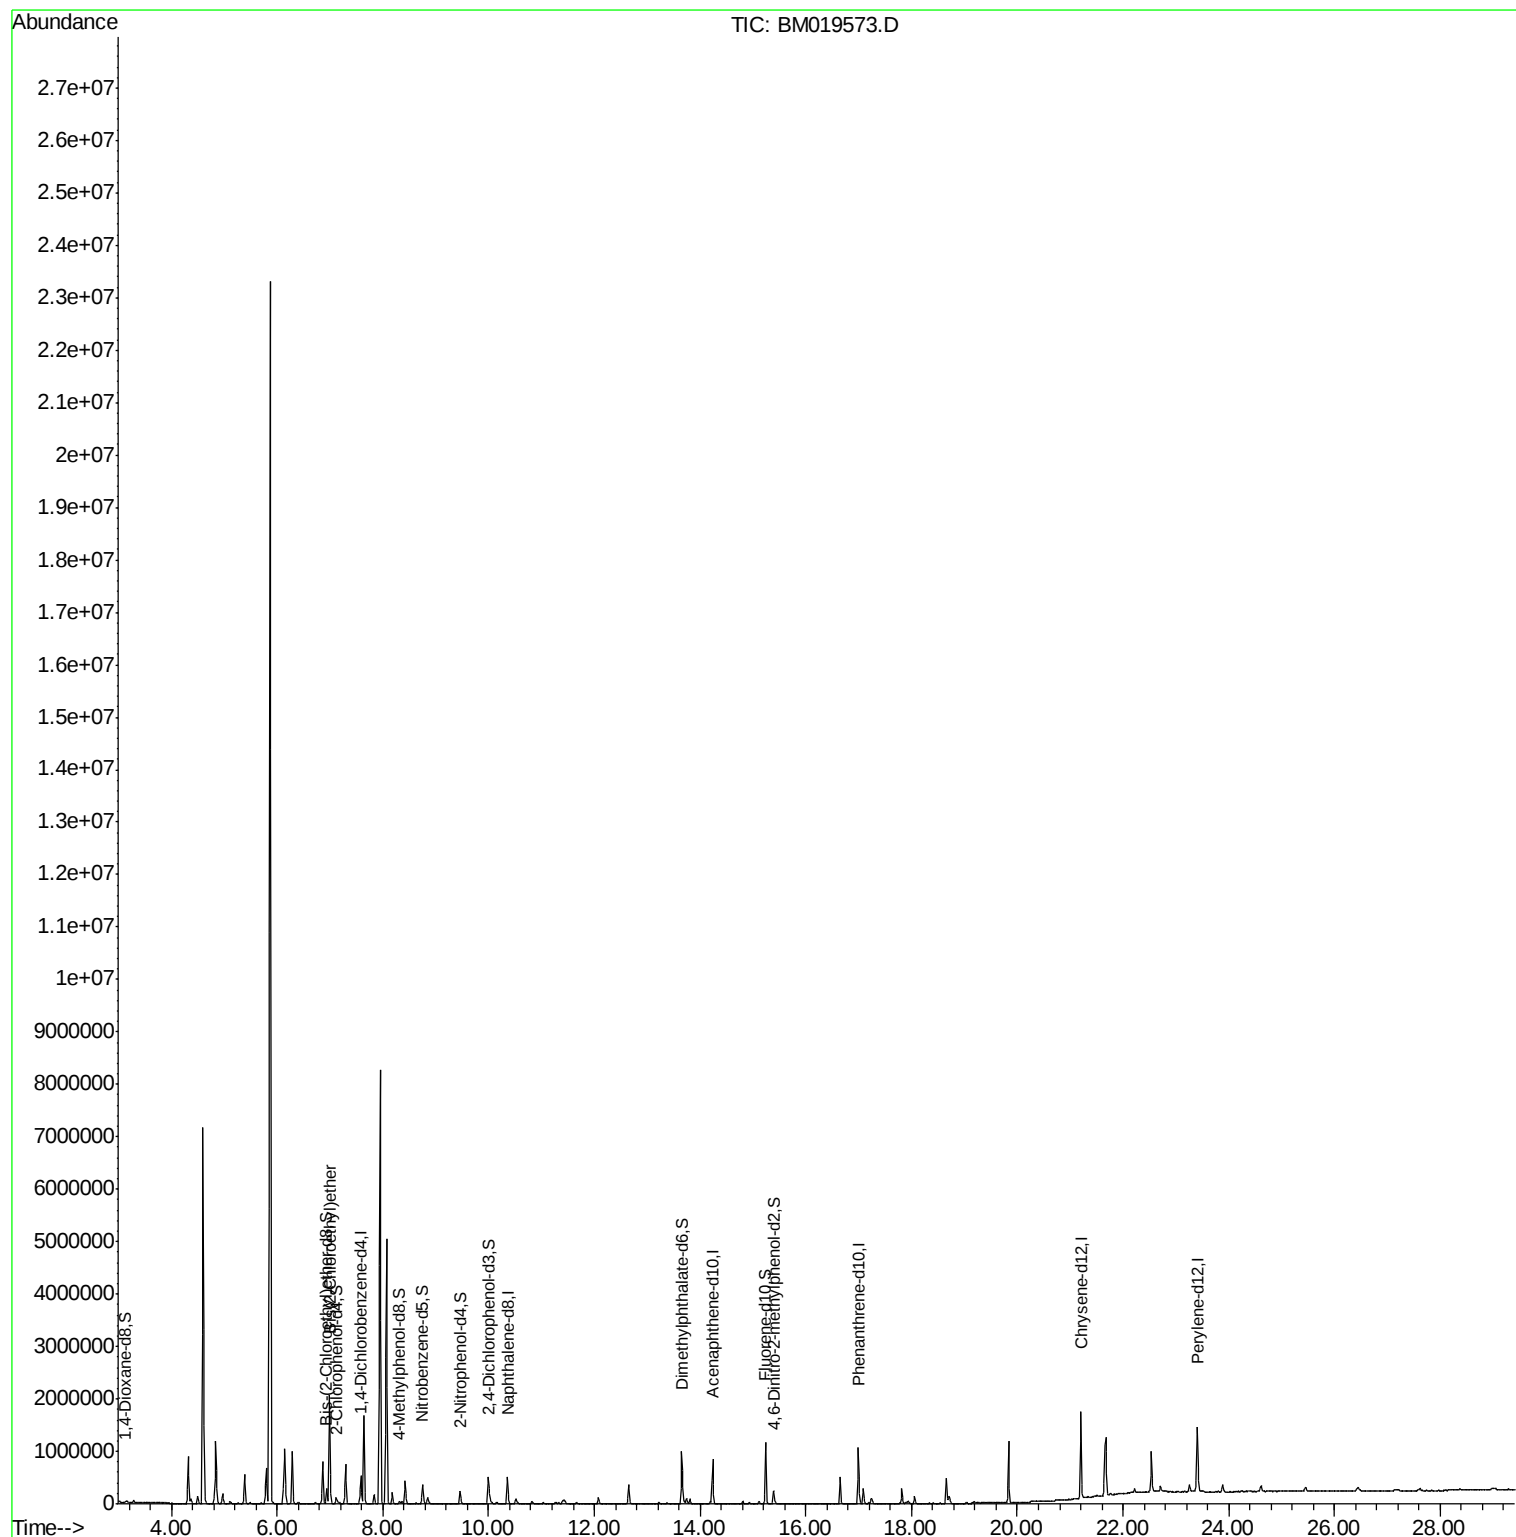

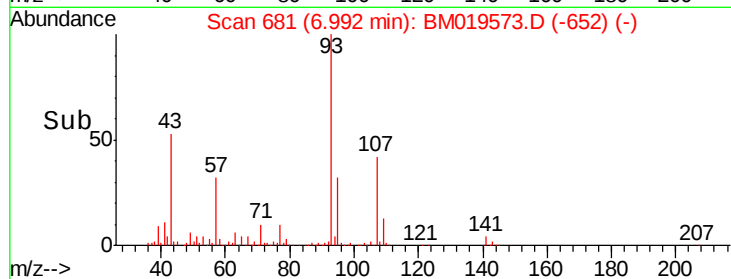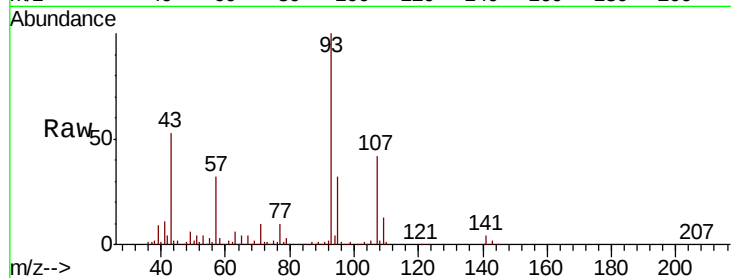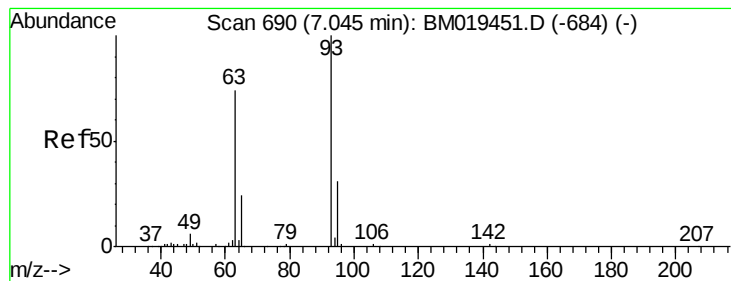

#8

Bis(2-Chloroethyl)ether

Concen: 118.636 ng/ul

RT: 6.99 min Scan# 681

Delta R.T. -0.03 min

Lab File: BM019573.D

Acq: 29 Mar 2019 10:41

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 93 Resp: 790241

Ion Ratio Lower Upper

93 100

63 6.2 59.4 89.2#

95 31.5 26.4 39.6

