

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032819\
 Data File : BM019562.D
 Acq On : 29 Mar 2019 04:03
 Operator : JU/SJ
 Sample : K2065-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5L8

Manual Integrations
 APPROVED

Sohil
 3/29/2019 4:49:14 PM

Quant Time: Mar 29 06:56:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 06:50:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	127509	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	578214	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	329450	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	714344	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	914328	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1122257	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	18337	5.63	ng/uL	0.00
5) Phenol-d5	6.76	99	147543	12.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	105879	13.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	128061	14.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	122896	14.42	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	56509	13.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	62656	13.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	107109	12.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	152993	14.71	ng/ul	0.01
44) Dimethylphthalate-d6	13.66	166	425943	16.02	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	483800	14.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	37372m	8.97	ng/ul	0.03
58) Fluorene-d10	15.24	176	361832	15.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	43438	9.20	ng/ul	0.00
71) Anthracene-d10	17.10	188	536525	15.65	ng/ul	0.00
79) Pyrene-d10	19.40	212	622179	14.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	863525	14.51	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.71	163	62600	2.347	ng/ul# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032819\
Data File : BM019562.D
Acq On : 29 Mar 2019 04:03
Operator : JU/SJ
Sample : K2065-19
Misc :
ALS Vial : 24 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BF5L8

Quant Time: Mar 29 06:56:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 06:50:20 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/29/2019 4:49:14 PM

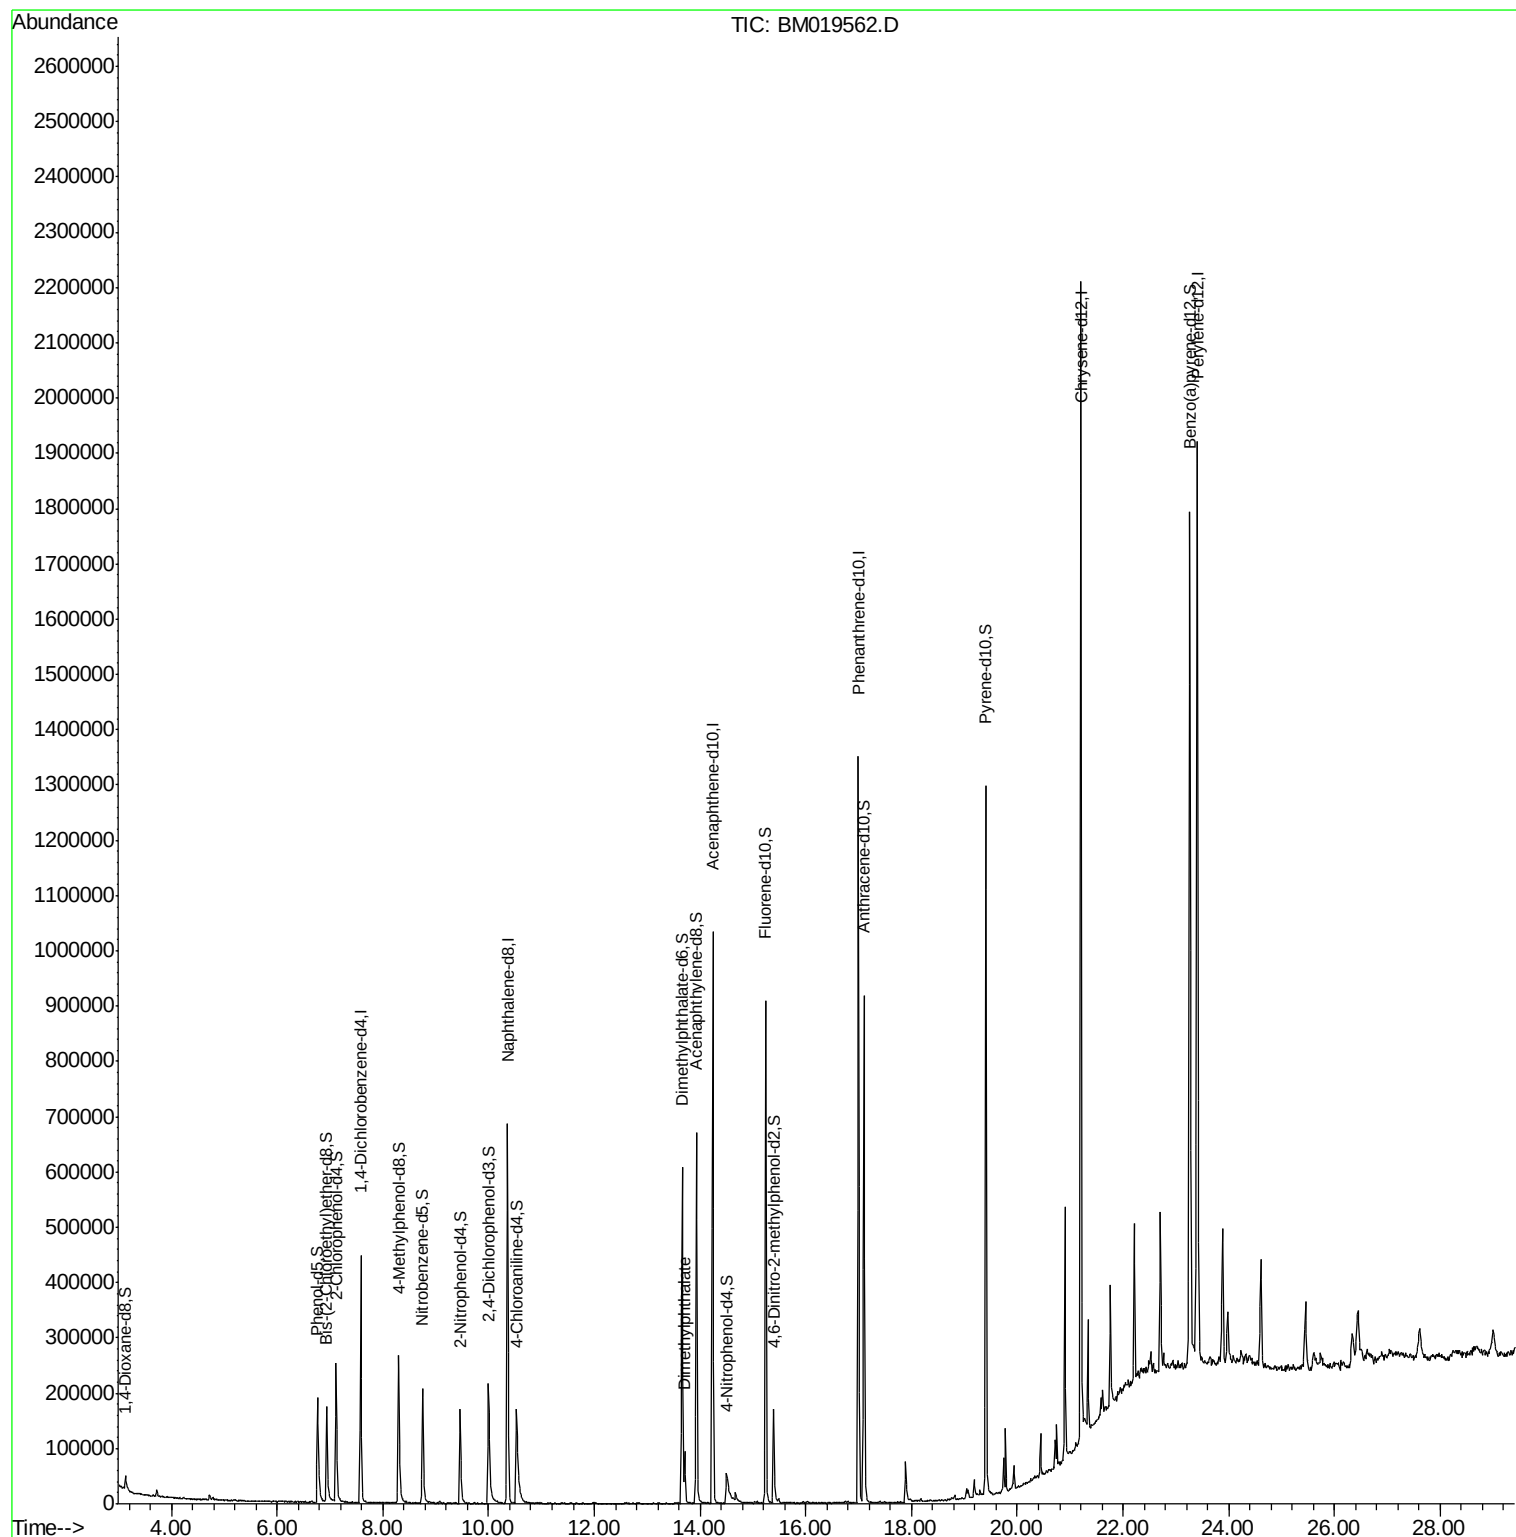

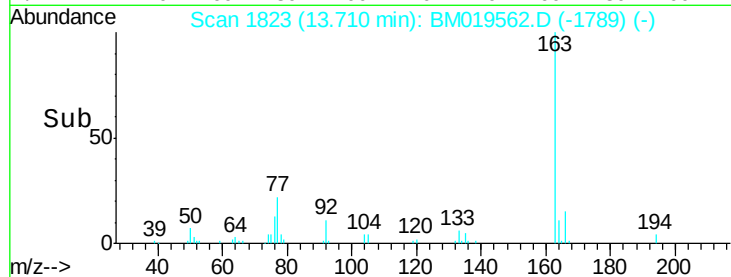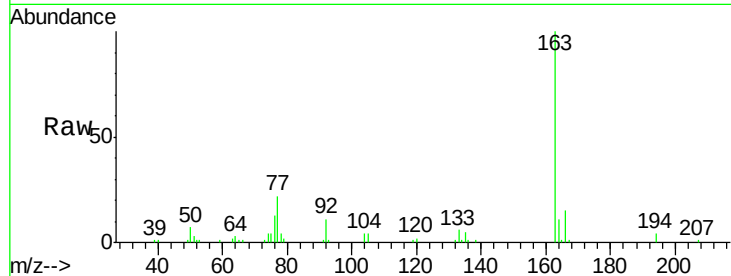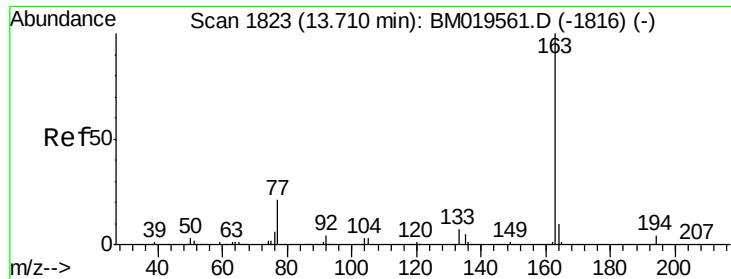

#45

Dimethylphthalate

Concen: 2.347 ng/ul

RT: 13.71 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BM019562.D

Acq: 29 Mar 2019 04:03

Instrument :

BNA_M

ClientSampleId :

BF5L8

Tgt Ion:163 Resp: 62600
Ion Ratio Lower Upper

163 100

194 3.7 4.0 6.0#

164 10.8 8.4 12.6

Manual Integrations
APPROVED

Sohil
3/29/2019 4:49:14 PM

