
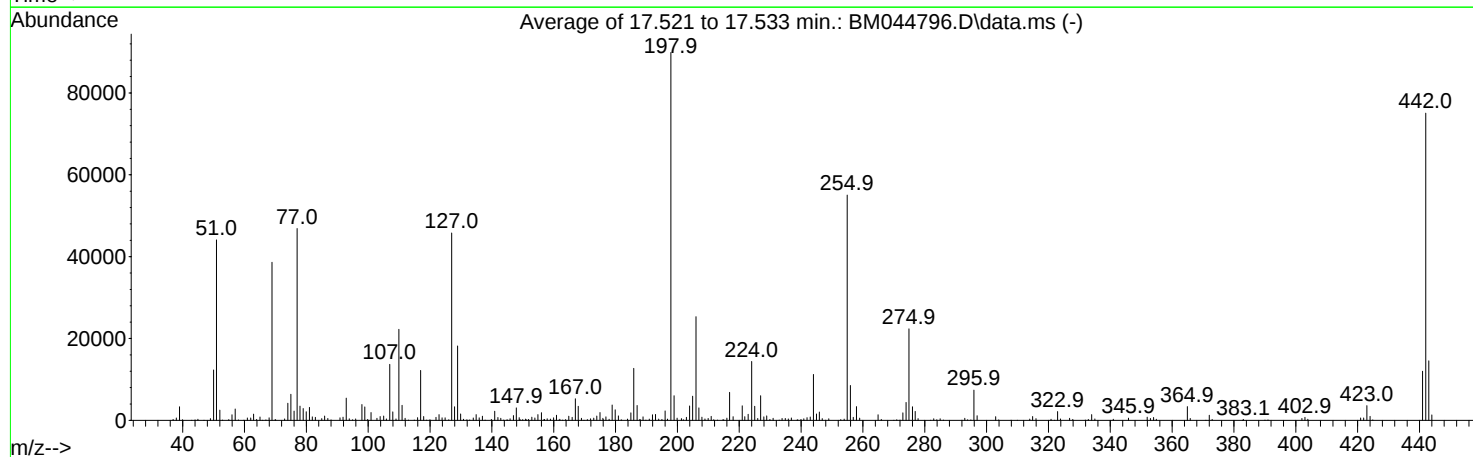


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032824\
Data File : BM044796.D
Acq On : 28 Mar 2024 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 29 01:24:21 2024

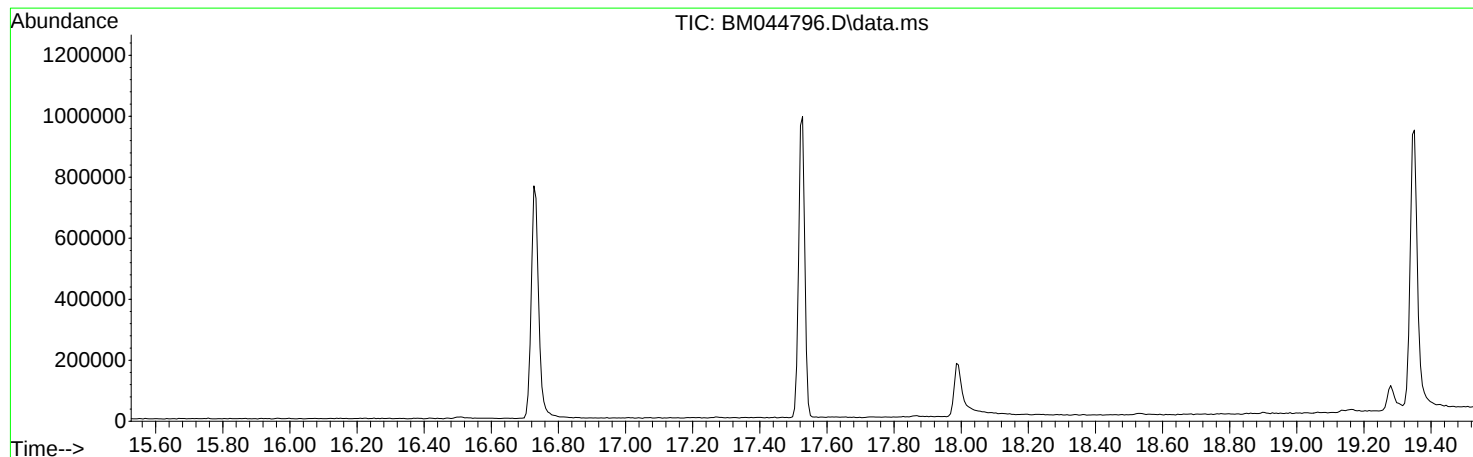




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	44096	PASS
68	69	0.00	2	1.6	626	PASS
69	198	0.00	100	43.0	38612	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	50.9	45779	PASS
197	198	0.00	2	0.3	308	PASS
198	198	100	100	100.0	89883	PASS
199	198	5	9	6.7	6026	PASS
275	198	10	60	24.9	22373	PASS
365	198	1	100	3.7	3346	PASS
441	198	0.01	100	13.3	11984	PASS
442	442	50	100	100.0	75080	PASS
443	442	15	24	19.4	14561	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032824\
Data File : BM044796.D
Acq On : 28 Mar 2024 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 29 01:33:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 29 01:24:21 2024
Response via : Initial Calibration

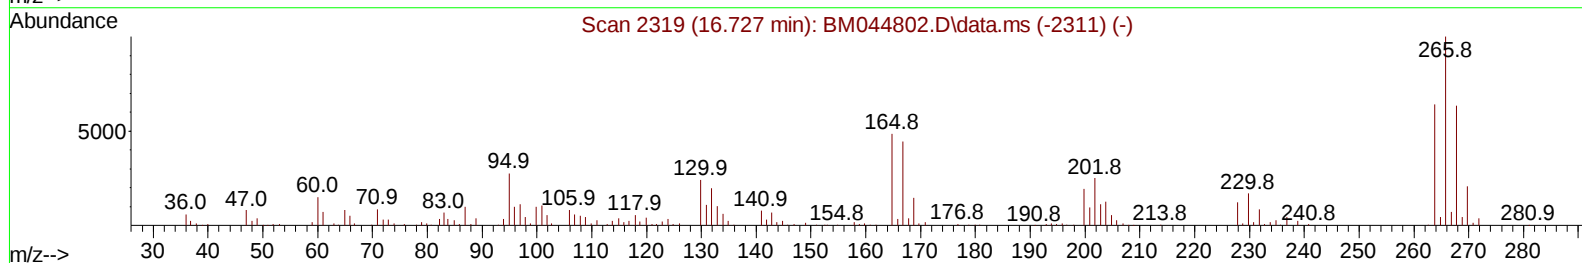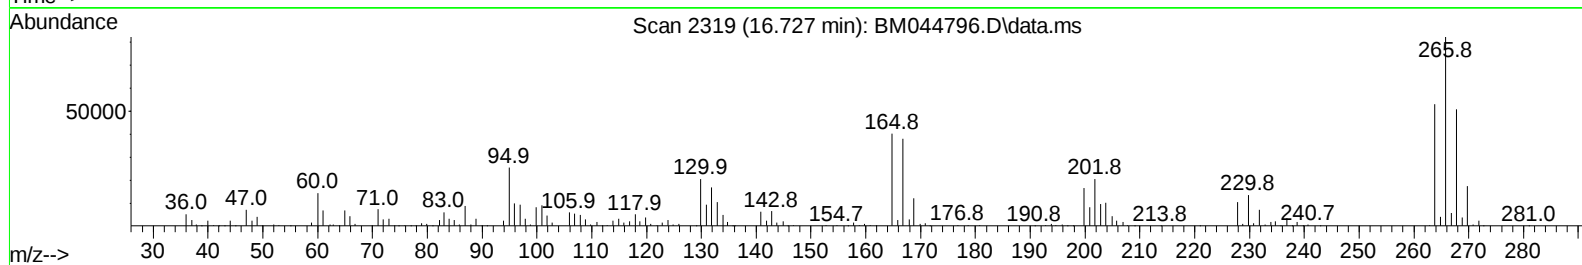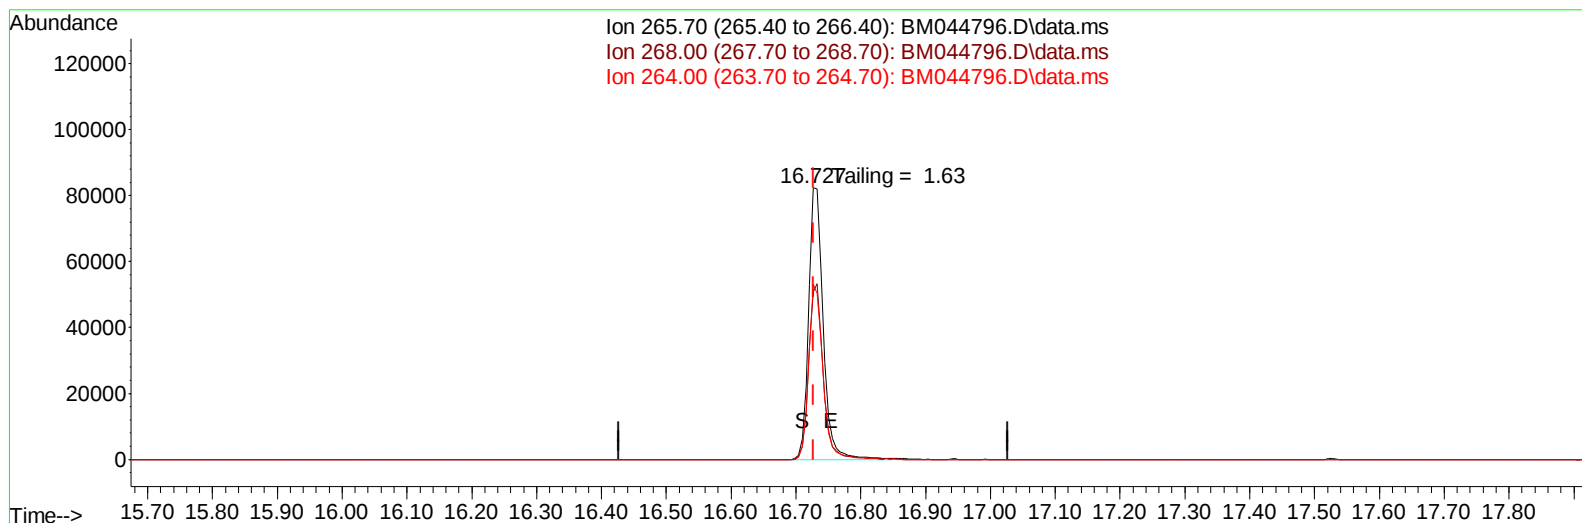

TIC: BM044796.D\data.ms

(70) Pentachlorophenol (C)

16.727min (+ 0.000) 0.00 ng

response 131000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.76
264.00	64.10	64.41
0.00	0.00	0.00

Instrument :
BNA_M
ClientSampleId :
DFTPP

Abundance



Ion 184.00 (183.70 to 184.70): BM044796.D\data.ms
Ion 185.00 (184.70 to 185.70): BM044796.D\data.ms
Ion 183.00 (182.70 to 183.70): BM044796.D\data.ms

19.350
Tailing = 0.99

S E

m/z--> 18.30 18.40 18.50 18.60 18.70 18.80 18.90 19.00 19.10 19.20 19.30 19.40 19.50 19.60 19.70 19.80 19.90 20.00 20.10 20.20 20.30 20.40

m/z	Abundance
19.350	~350,000

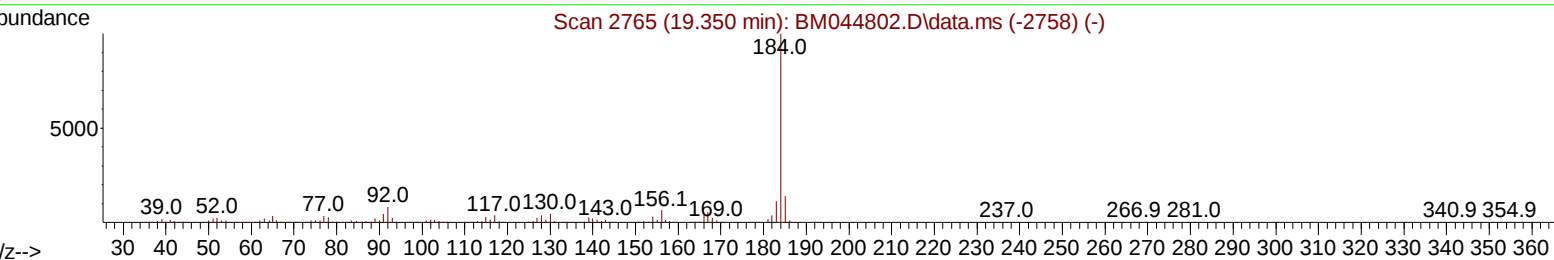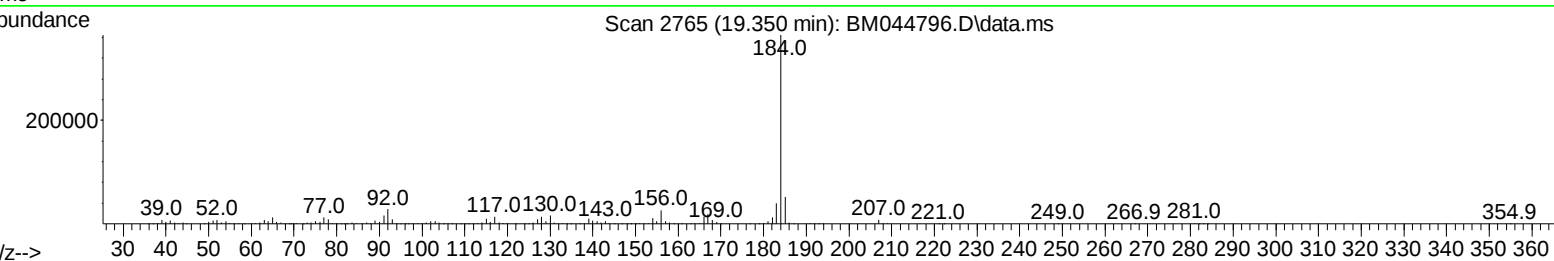

TIC: BM044796.D\data.ms

(77) **Benzidine**

19.350min (+ 0.000) 74662.43 ng

response **563439**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.20
183.00	11.30	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2024	BNA_M	<u>BM044796.D</u>
Compound Name	Response	Retention Time
DDT	258613	20.58
DDD	7382	20.139
DDE	0	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7382	265995	2.78

Instrument :
BNA_M
ClientSampleId :
DFTPP