

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
 Data File : BM019589.D
 Acq On : 29 Mar 2019 20:49
 Operator : JU/SJ
 Sample : K2085-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 29 22:57:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	124728	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	566154	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	322420	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	690608	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	872405	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1088245	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	21304	6.69	ng/uL	0.00
5) Phenol-d5	6.76	99	243841	21.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	161804	21.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	196771	23.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	206382	24.75	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	88415	21.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	106881	23.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	190707	22.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	281202	27.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	667027	25.64	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	801678	24.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	86655	21.25	ng/ul	0.00
58) Fluorene-d10	15.24	176	568689	25.37	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	80349	17.59	ng/ul	0.00
71) Anthracene-d10	17.10	188	880960	26.58	ng/ul	0.00
79) Pyrene-d10	19.40	212	1025861	25.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	1404754	24.35	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.79	94	29268	2.525	ng/ul#	82
45) Dimethylphthalate	13.70	163	118421	4.537	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
Data File : BM019589.D
Acq On : 29 Mar 2019 20:49
Operator : JU/SJ
Sample : K2085-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 29 22:57:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

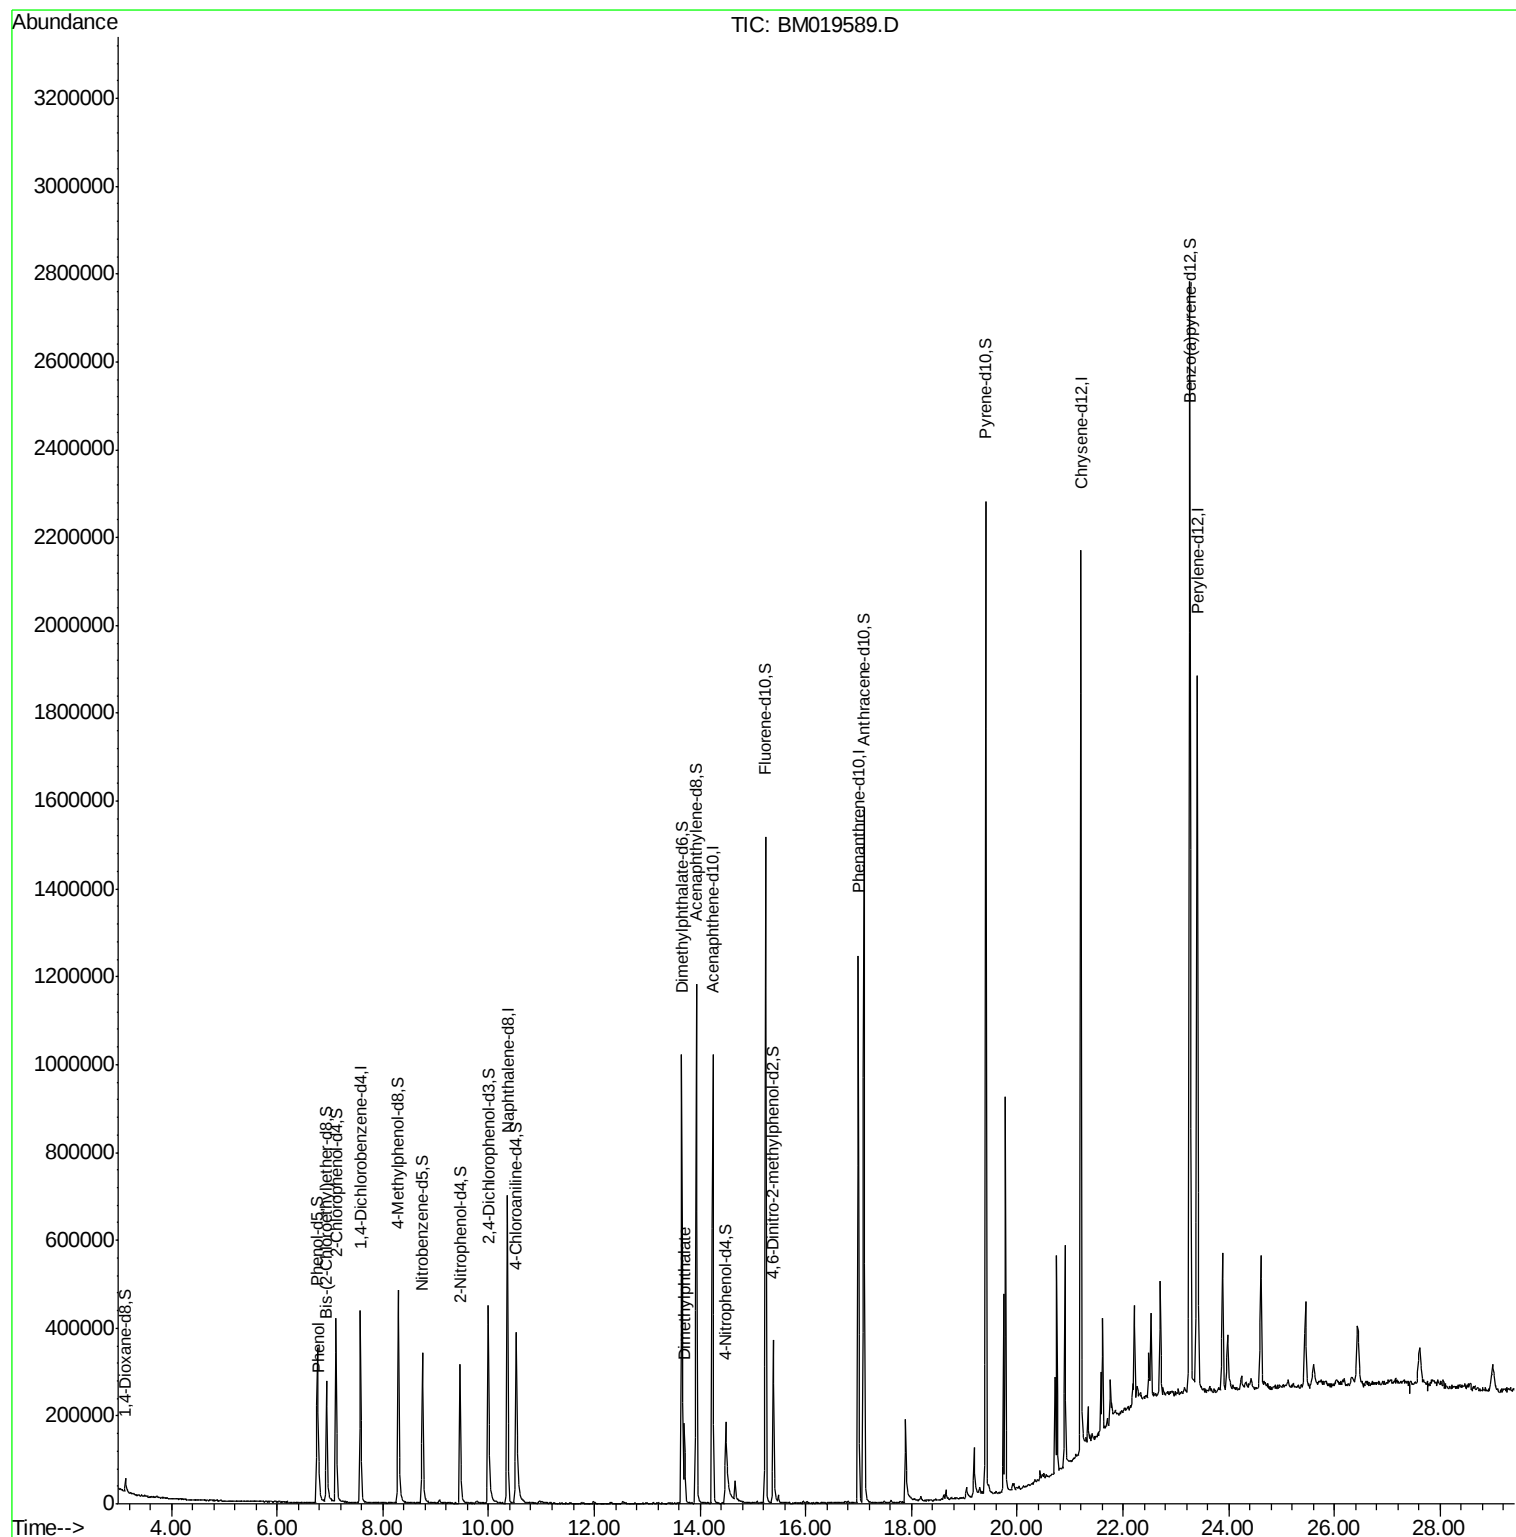

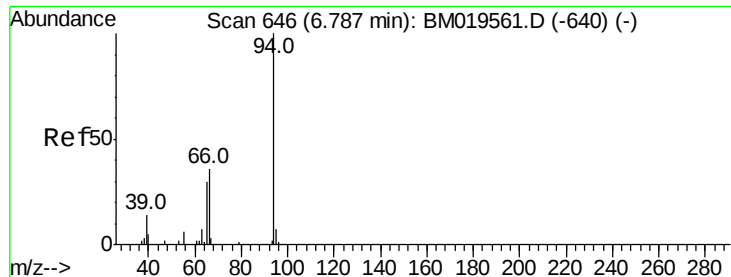

#6

Phenol

Concen: 2.525 ng/ul

RT: 6.79 min Scan# 646

Delta R.T. -0.00 min

Lab File: BM019589.D

Acq: 29 Mar 2019 20:49

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 29268

Ion Ratio Lower Upper

94 100

65 35.0 23.0 34.6#




66 52.2 30.4 45.6#

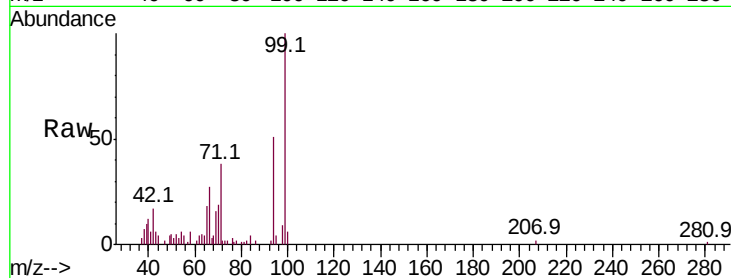

Abundance Ion 94.00 (93.70 to 94.70): BM019561.D (-640) (-)

Ion 65.00 (64.70 to 65.70): BM019561.D (-640) (-)

Ion 66.00 (65.70 to 66.70): BM019561.D (-640) (-)

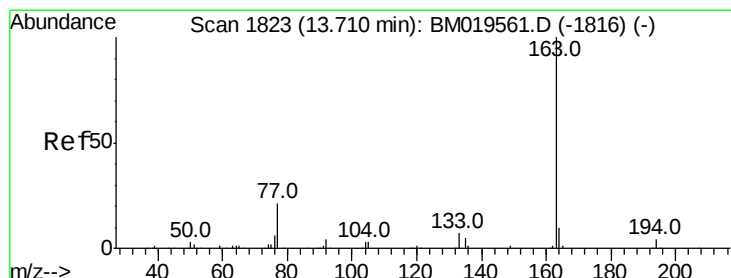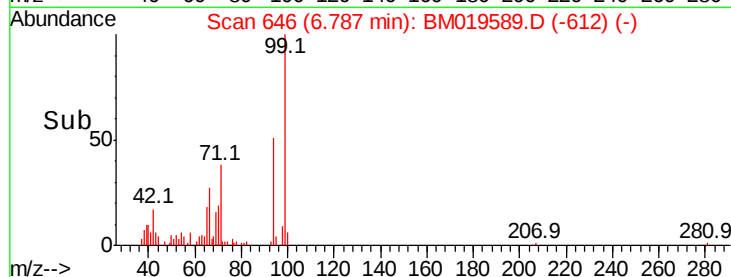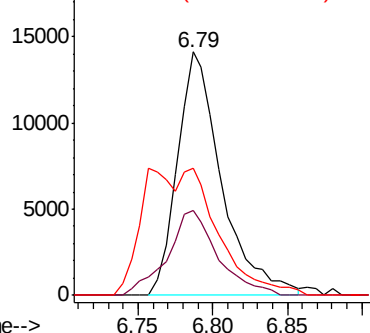

#45

Dimethylphthalate

Concen: 4.537 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM019589.D

Acq: 29 Mar 2019 20:49


Tgt Ion: 163 Resp: 118421

Ion Ratio Lower Upper

163 100

194 3.6 4.0 6.0#

164 9.6 8.4 12.6

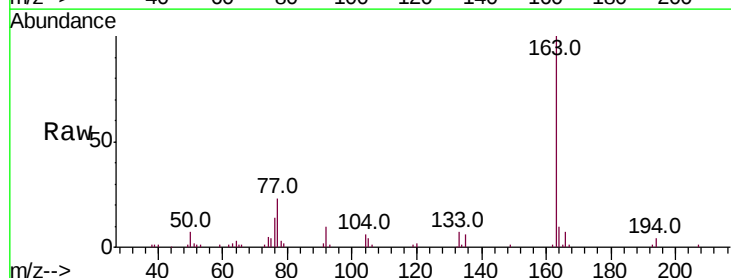

Abundance Ion 163.00 (162.70 to 163.70): BM019561.D (-1816) (-)

Ion 194.00 (193.70 to 194.70): BM019561.D (-1816) (-)

Ion 164.00 (163.70 to 164.70): BM019561.D (-1816) (-)

