

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019599.D
 Acq On : 30 Mar 2019 02:53
 Operator : JU/SJ
 Sample : K2084-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF7X5

Quant Time: Mar 30 03:49:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	114436	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	509369	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	289170	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	655292	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	821817	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1045395	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	14380	4.92	ng/uL	0.00
5) Phenol-d5	6.76	99	113498	11.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	91155	13.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	98039	12.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	69014	9.02	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	44502	12.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	49603	12.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	81213	10.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	94110m	10.27	ng/ul	0.02
44) Dimethylphthalate-d6	13.66	166	328132	14.06	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	362009	12.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	29035m	7.94	ng/ul	0.03
58) Fluorene-d10	15.24	176	269591	13.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	32707	7.55	ng/ul	0.00
71) Anthracene-d10	17.09	188	406452	12.93	ng/ul	0.00
79) Pyrene-d10	19.40	212	454617	11.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	611908	11.04	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.79	94	24614	2.315 ng/ul#	86
45) Dimethylphthalate	13.71	163	53199	2.272 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019599.D
Acq On : 30 Mar 2019 02:53
Operator : JU/SJ
Sample : K2084-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF7X5

Quant Time: Mar 30 03:49:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

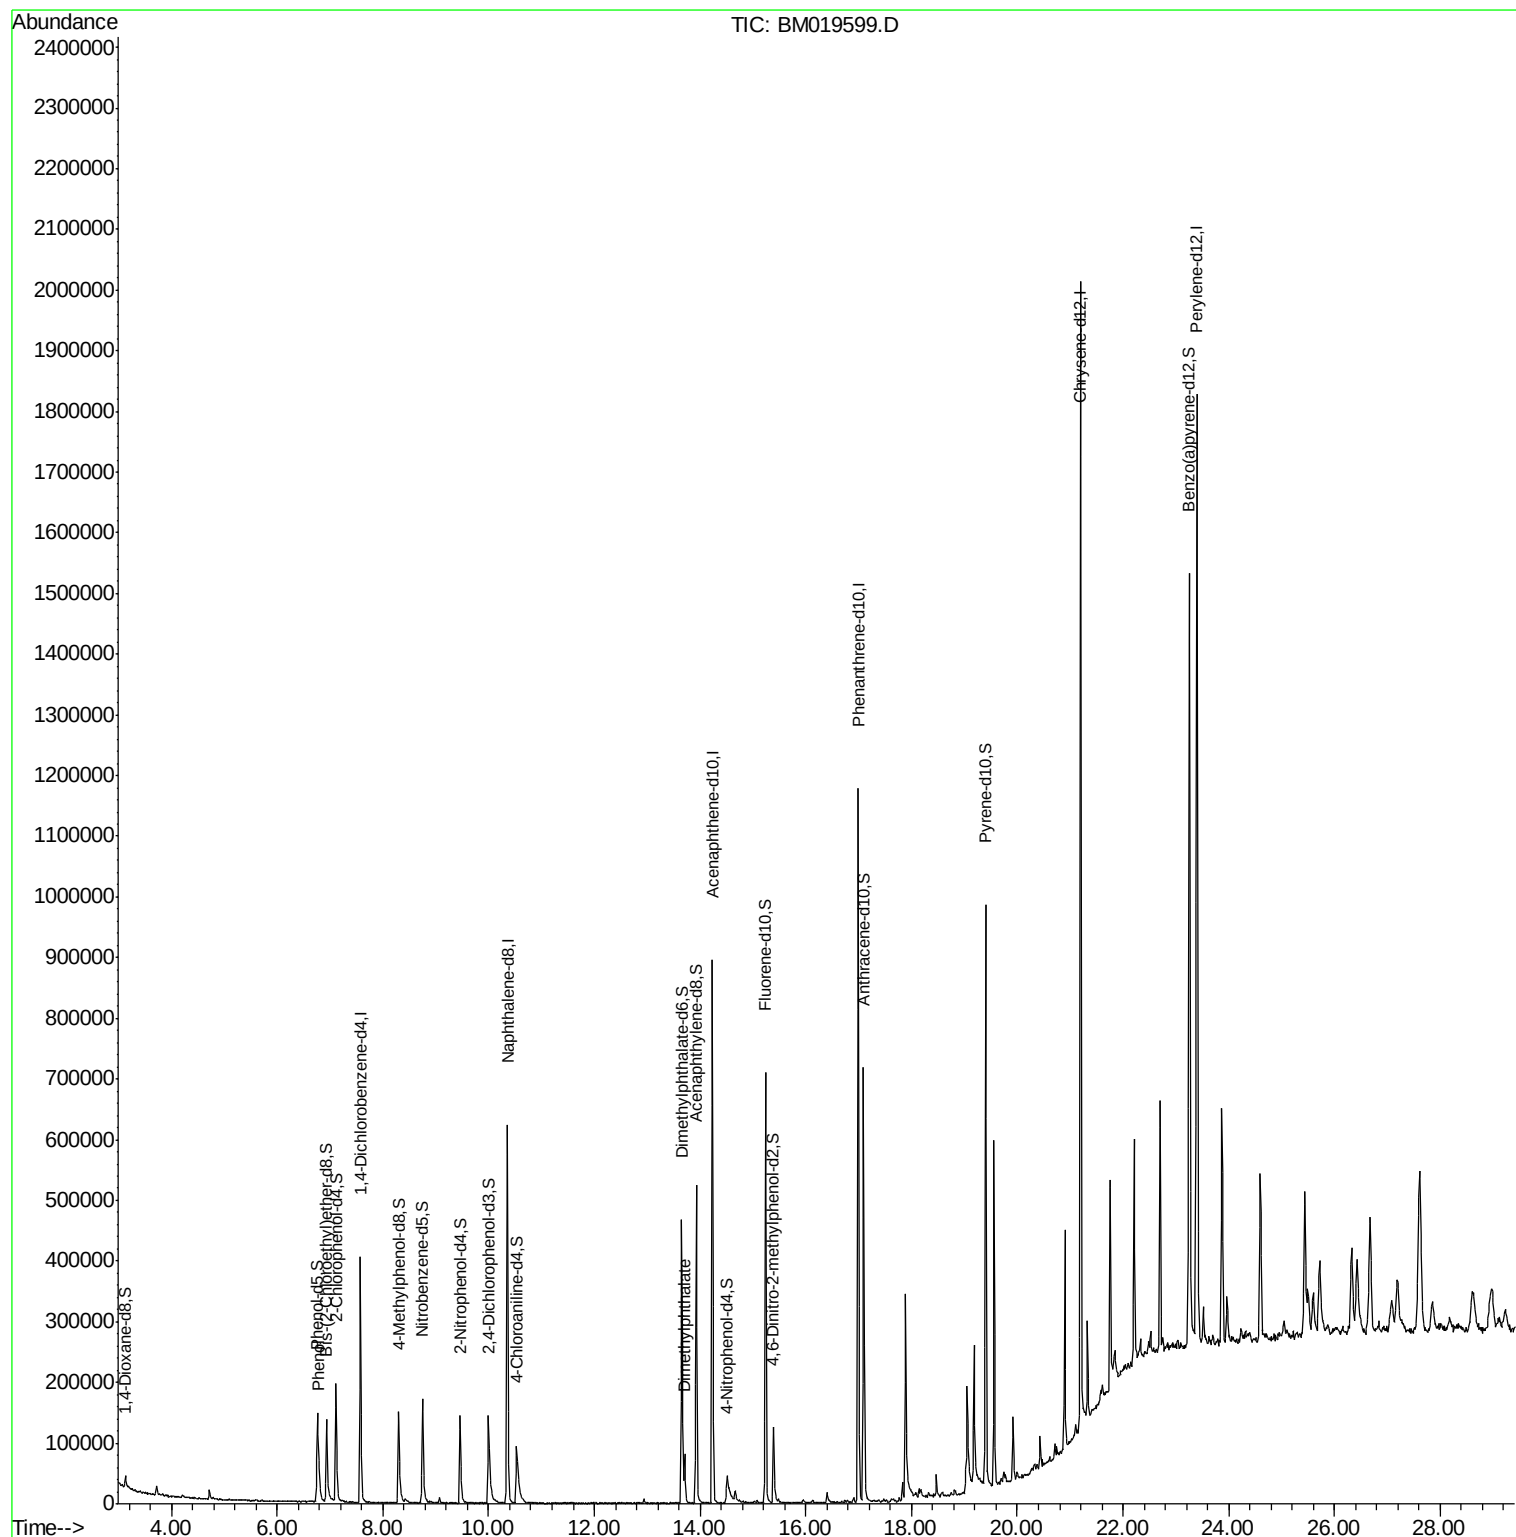

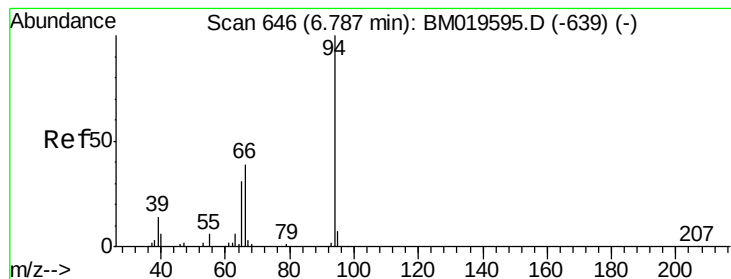





#6

Phenol

Concen: 2.315 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. 0.01 min
 Lab File: BM019599.D
 Acq: 30 Mar 2019 02:53

Instrument :
 BNA_M
 ClientSampled :
 BF7X5

Tgt Ion: 94 Resp: 24614
 Ion Ratio Lower Upper
 94 100
 65 33.6 23.0 34.6
 66 49.0 30.4 45.6#

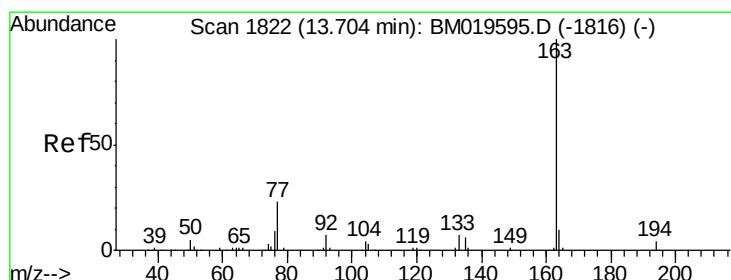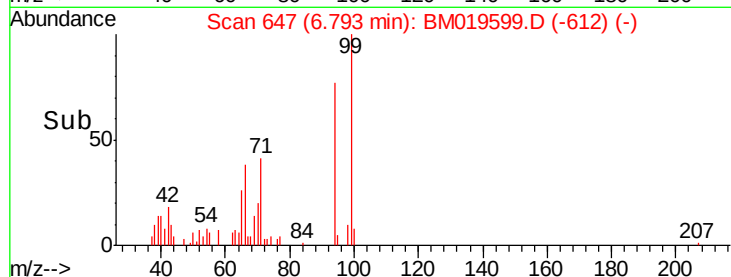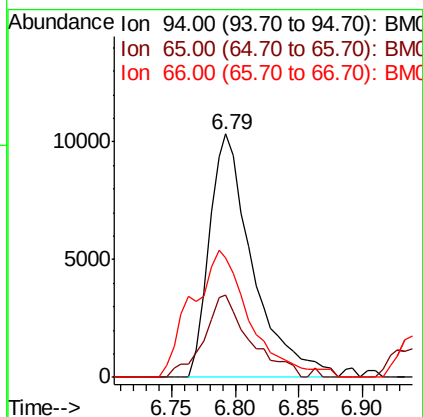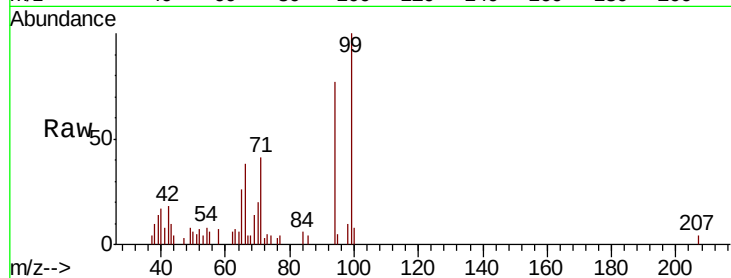

#45

Dimethylphthalate

Concen: 2.272 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.00 min
 Lab File: BM019599.D
 Acq: 30 Mar 2019 02:53

Tgt Ion: 163 Resp: 53199
 Ion Ratio Lower Upper
 163 100
 194 3.3 4.0 6.0#
 164 10.3 8.4 12.6

