

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
 Data File : BM019603.D
 Acq On : 30 Mar 2019 05:18
 Operator : JU/SJ
 Sample : PB118367BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 30 05:59:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	108280	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	498157	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	276850	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	627050	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	757778	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	987352	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	17504	6.33	ng/uL	0.00
5) Phenol-d5	6.76	99	319025	33.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	207504	32.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	251129	34.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	258339	35.69	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	117803	33.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	134268	33.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	220278	29.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	331603	37.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	827519	37.04	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	993933	35.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	101609	29.02	ng/ul	0.00
58) Fluorene-d10	15.24	176	700134	36.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	101032	24.36	ng/ul	0.00
71) Anthracene-d10	17.09	188	1113818	37.02	ng/ul	0.00
79) Pyrene-d10	19.40	212	1270935	36.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1817715	34.73	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.29	70	7456	1.129 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
Data File : BM019603.D
Acq On : 30 Mar 2019 05:18
Operator : JU/SJ
Sample : PB118367BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 30 05:59:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

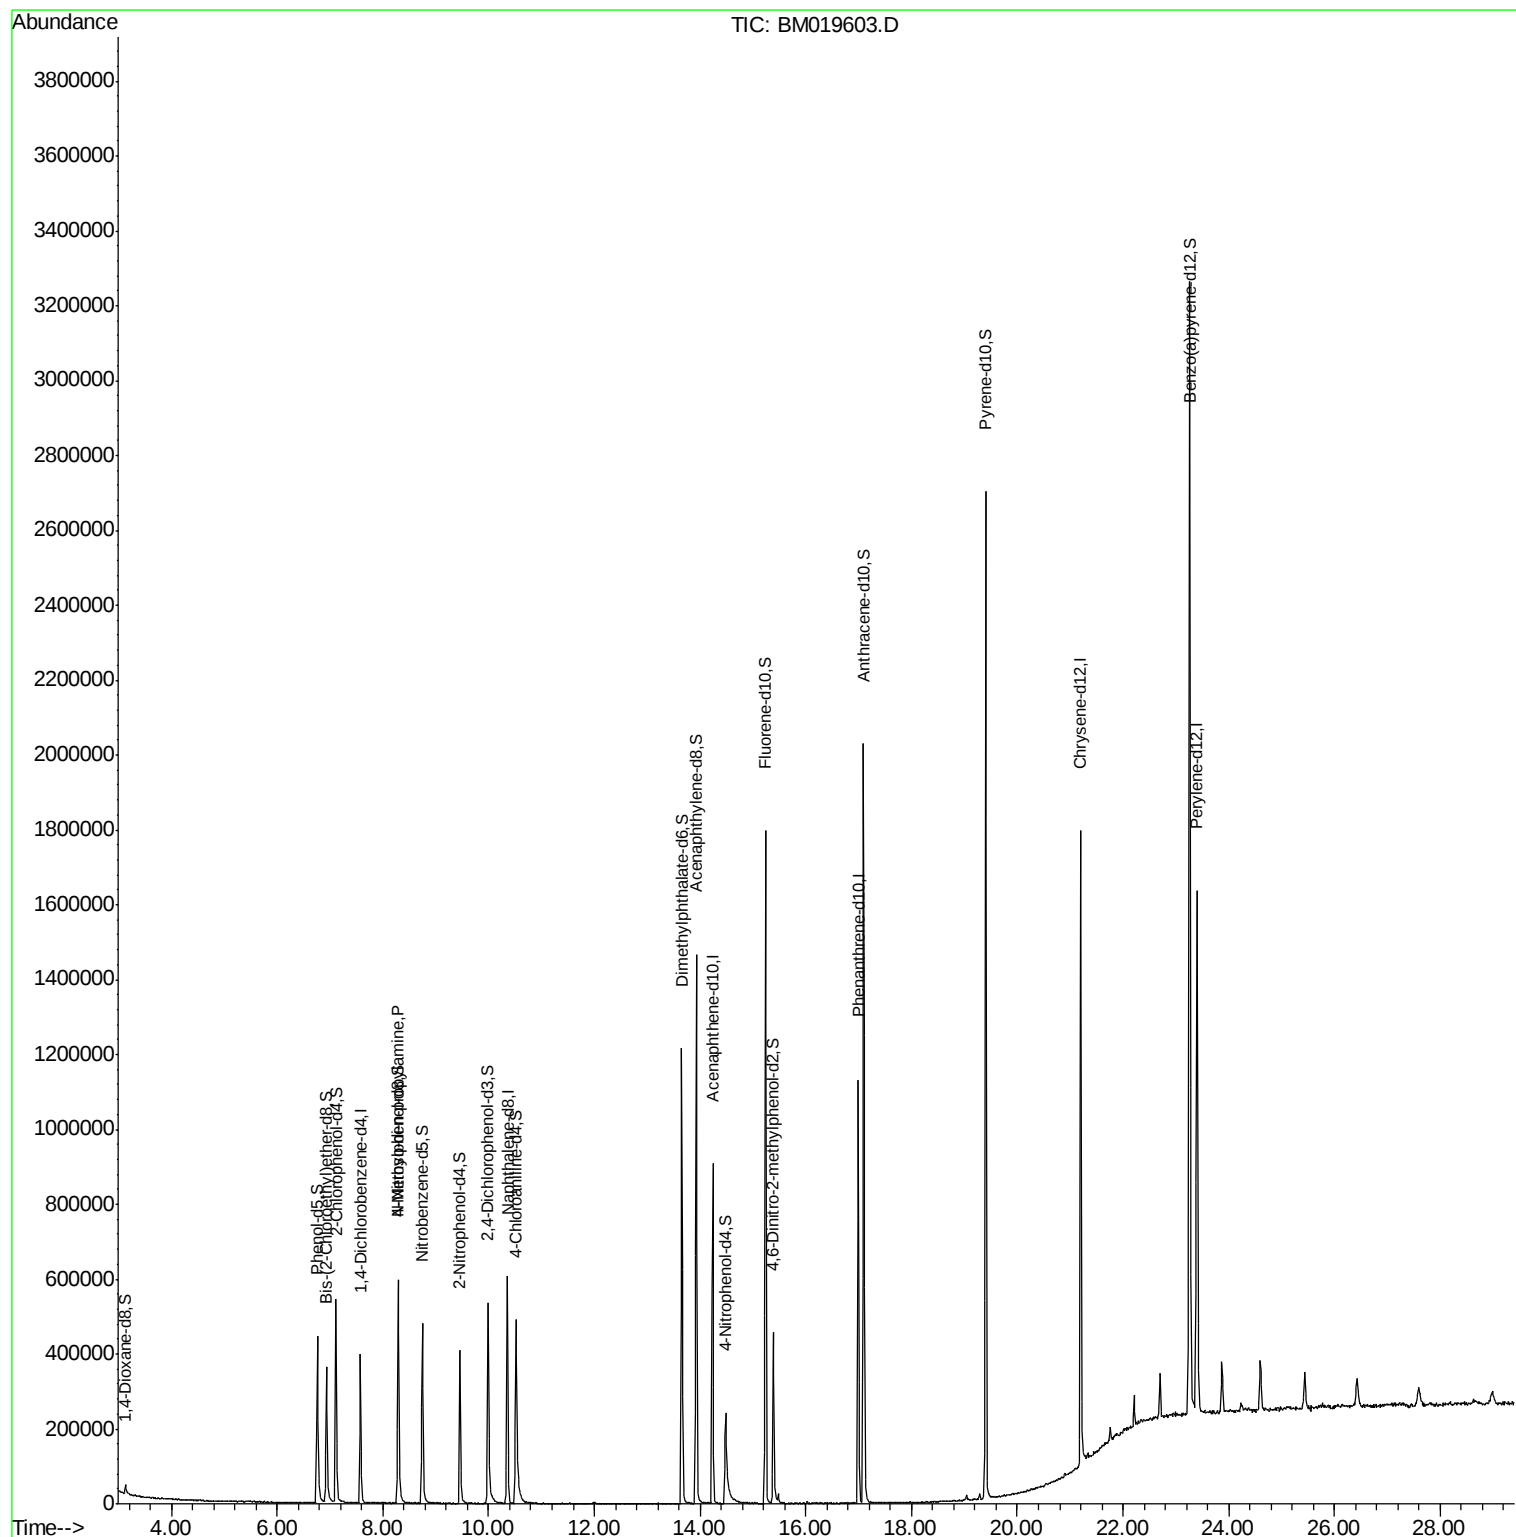

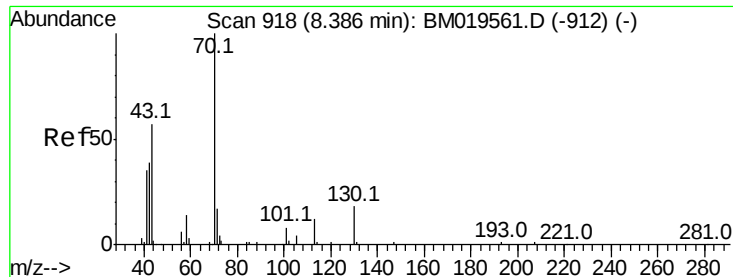

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.129 ng/ul
 RT: 8.29 min Scan# 901
 Delta R.T. -0.10 min
 Lab File: BM019603.D
 Acq: 30 Mar 2019 05:18

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 7456
 Ion Ratio Lower Upper
 70 100
 42 266.8 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

