

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
 Data File : BM019606.D
 Acq On : 30 Mar 2019 07:07
 Operator : JU/SJ
 Sample : K2122-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 30 20:56:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	132346	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	602718	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	337820	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	771848	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	955453	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1189051	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	11638	3.44	ng/uL	0.00
5) Phenol-d5	6.76	99	104979	8.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	78287	9.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	90475	10.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	89101	10.07	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	39774	9.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	42871	8.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	72971	8.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	112121	10.34	ng/ul	0.01
44) Dimethylphthalate-d6	13.66	166	303134	11.12	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	324723	9.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	6218	1.46	ng/ul	0.04
58) Fluorene-d10	15.24	176	249691	10.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	22385	4.39	ng/ul	0.00
71) Anthracene-d10	17.09	188	377872	10.20	ng/ul	0.00
79) Pyrene-d10	19.40	212	425032	9.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	566154	8.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.71	163	43839	1.603	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032919\
Data File : BM019606.D
Acq On : 30 Mar 2019 07:07
Operator : JU/SJ
Sample : K2122-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 30 20:56:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

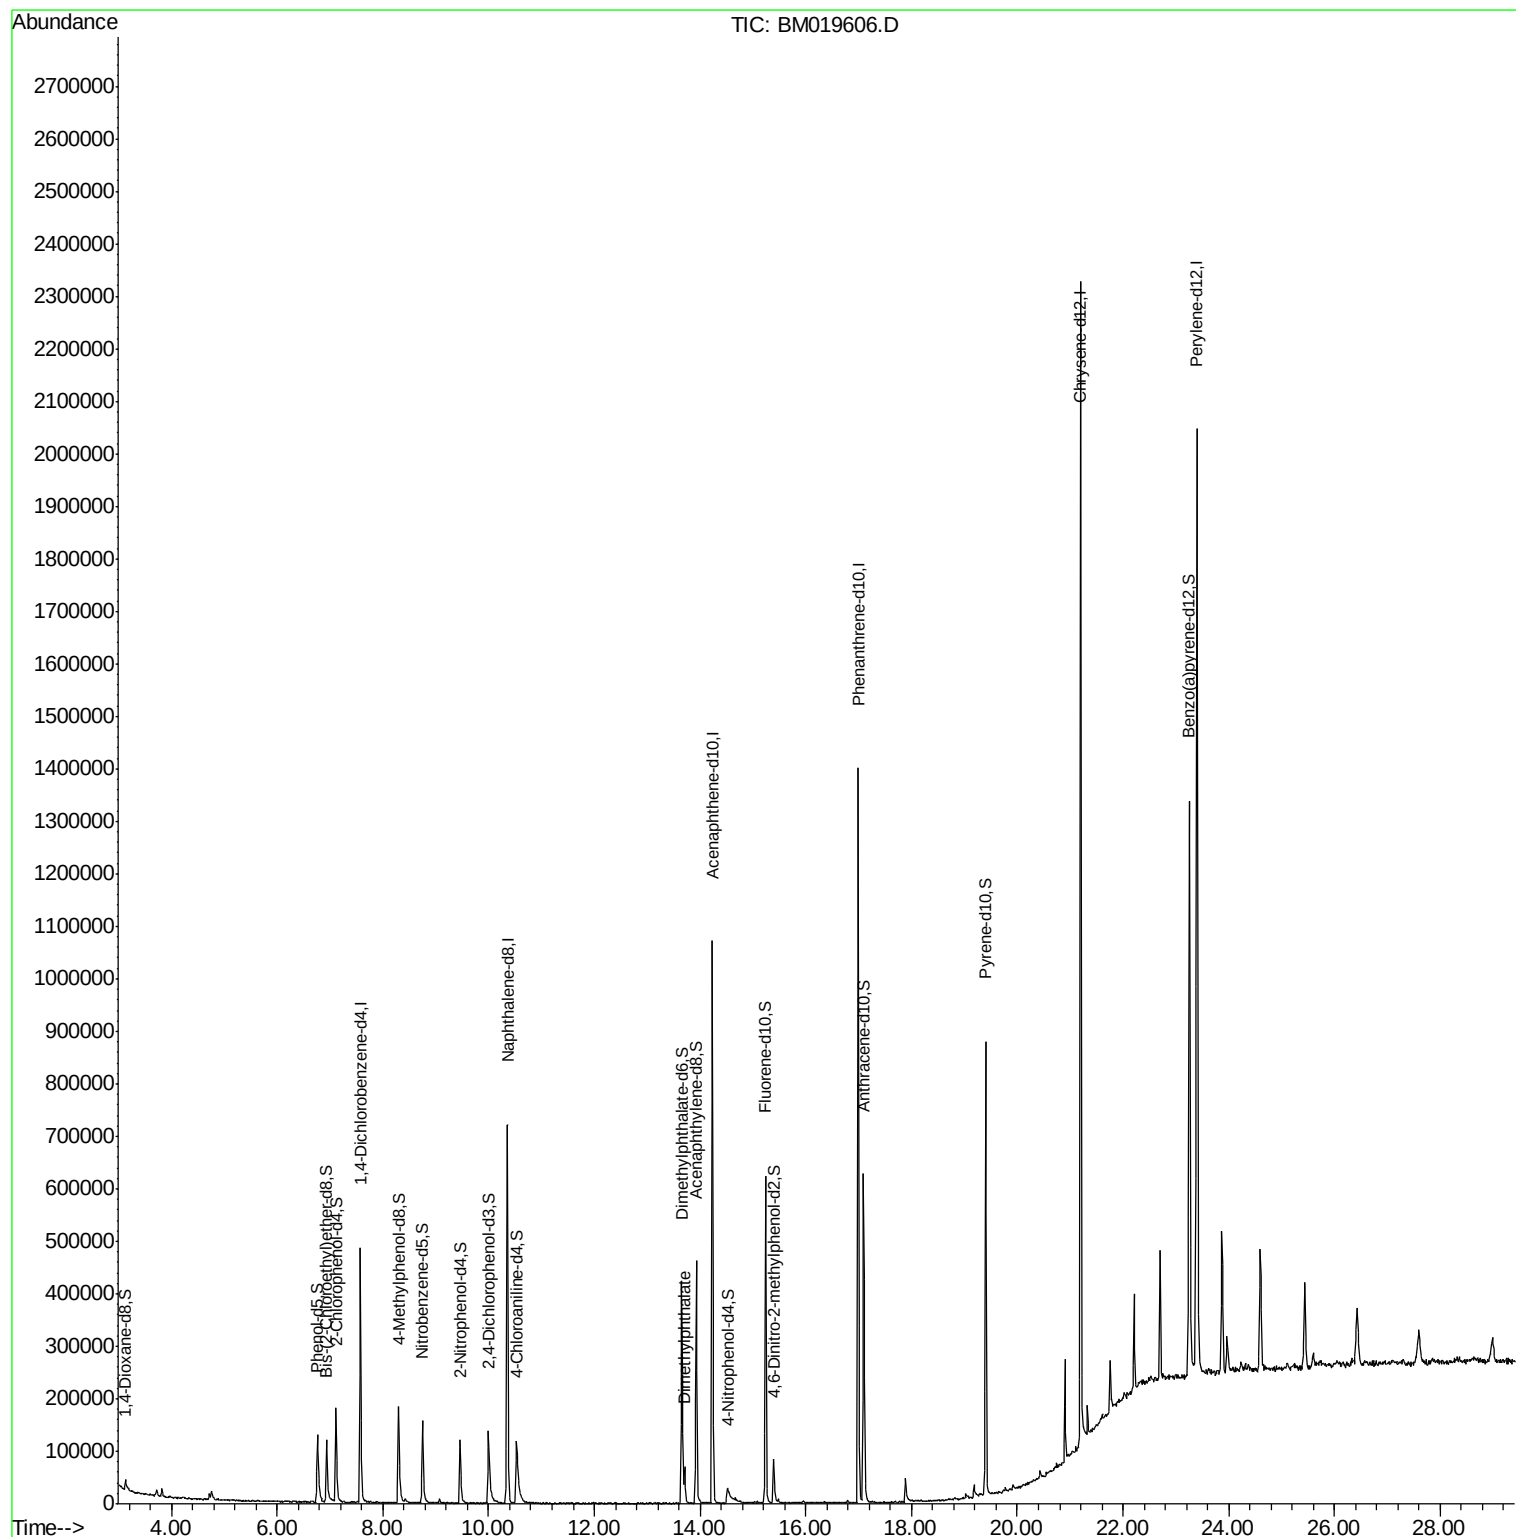

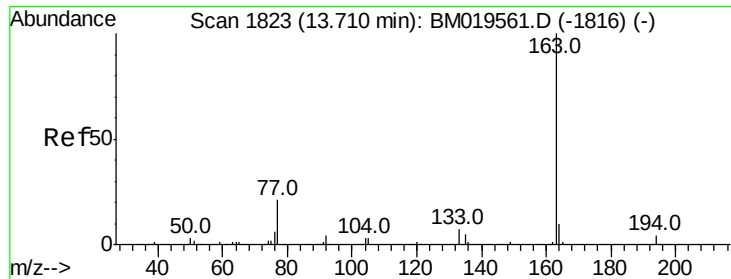

#45

Dimethylphthalate

Concen: 1.603 ng/ul

RT: 13.71 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BM019606.D

Acq: 30 Mar 2019 07:07

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 43839

Ion Ratio Lower Upper

163 100

194 4.4 4.0 6.0

164 9.4 8.4 12.6

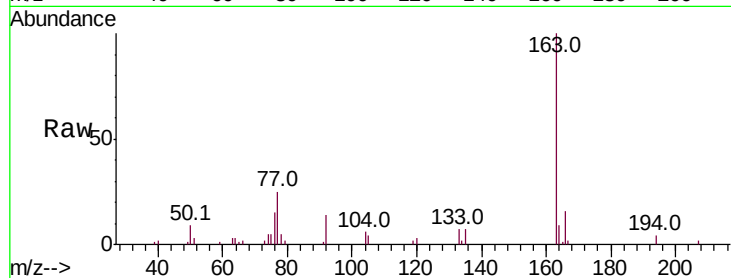

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

