

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019606.D
 Acq On : 30 Mar 2019 07:07
 Operator : JU/SJ
 Sample : K2122-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5B2

Quant Time: Mar 30 21:07:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	132346	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	602718	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	337820	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	771848	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	955453	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1189051	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	13933m	4.12	ng/uL	0.00
5) Phenol-d5	6.76	99	104979	8.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	78287	9.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	90475	10.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	89101	10.07	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	39774	9.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	42871	8.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	72971	8.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	112121	10.34	ng/ul	0.01
44) Dimethylphthalate-d6	13.66	166	303134	11.12	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	324723	9.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	21747m	5.09	ng/ul	0.05
58) Fluorene-d10	15.24	176	249691	10.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	22385	4.39	ng/ul	0.00
71) Anthracene-d10	17.09	188	377872	10.20	ng/ul	0.00
79) Pyrene-d10	19.40	212	425032	9.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	566154	8.98	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.71	163	43839	1.603	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019606.D
Acq On : 30 Mar 2019 07:07
Operator : JU/SJ
Sample : K2122-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5B2

Quant Time: Mar 30 21:07:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

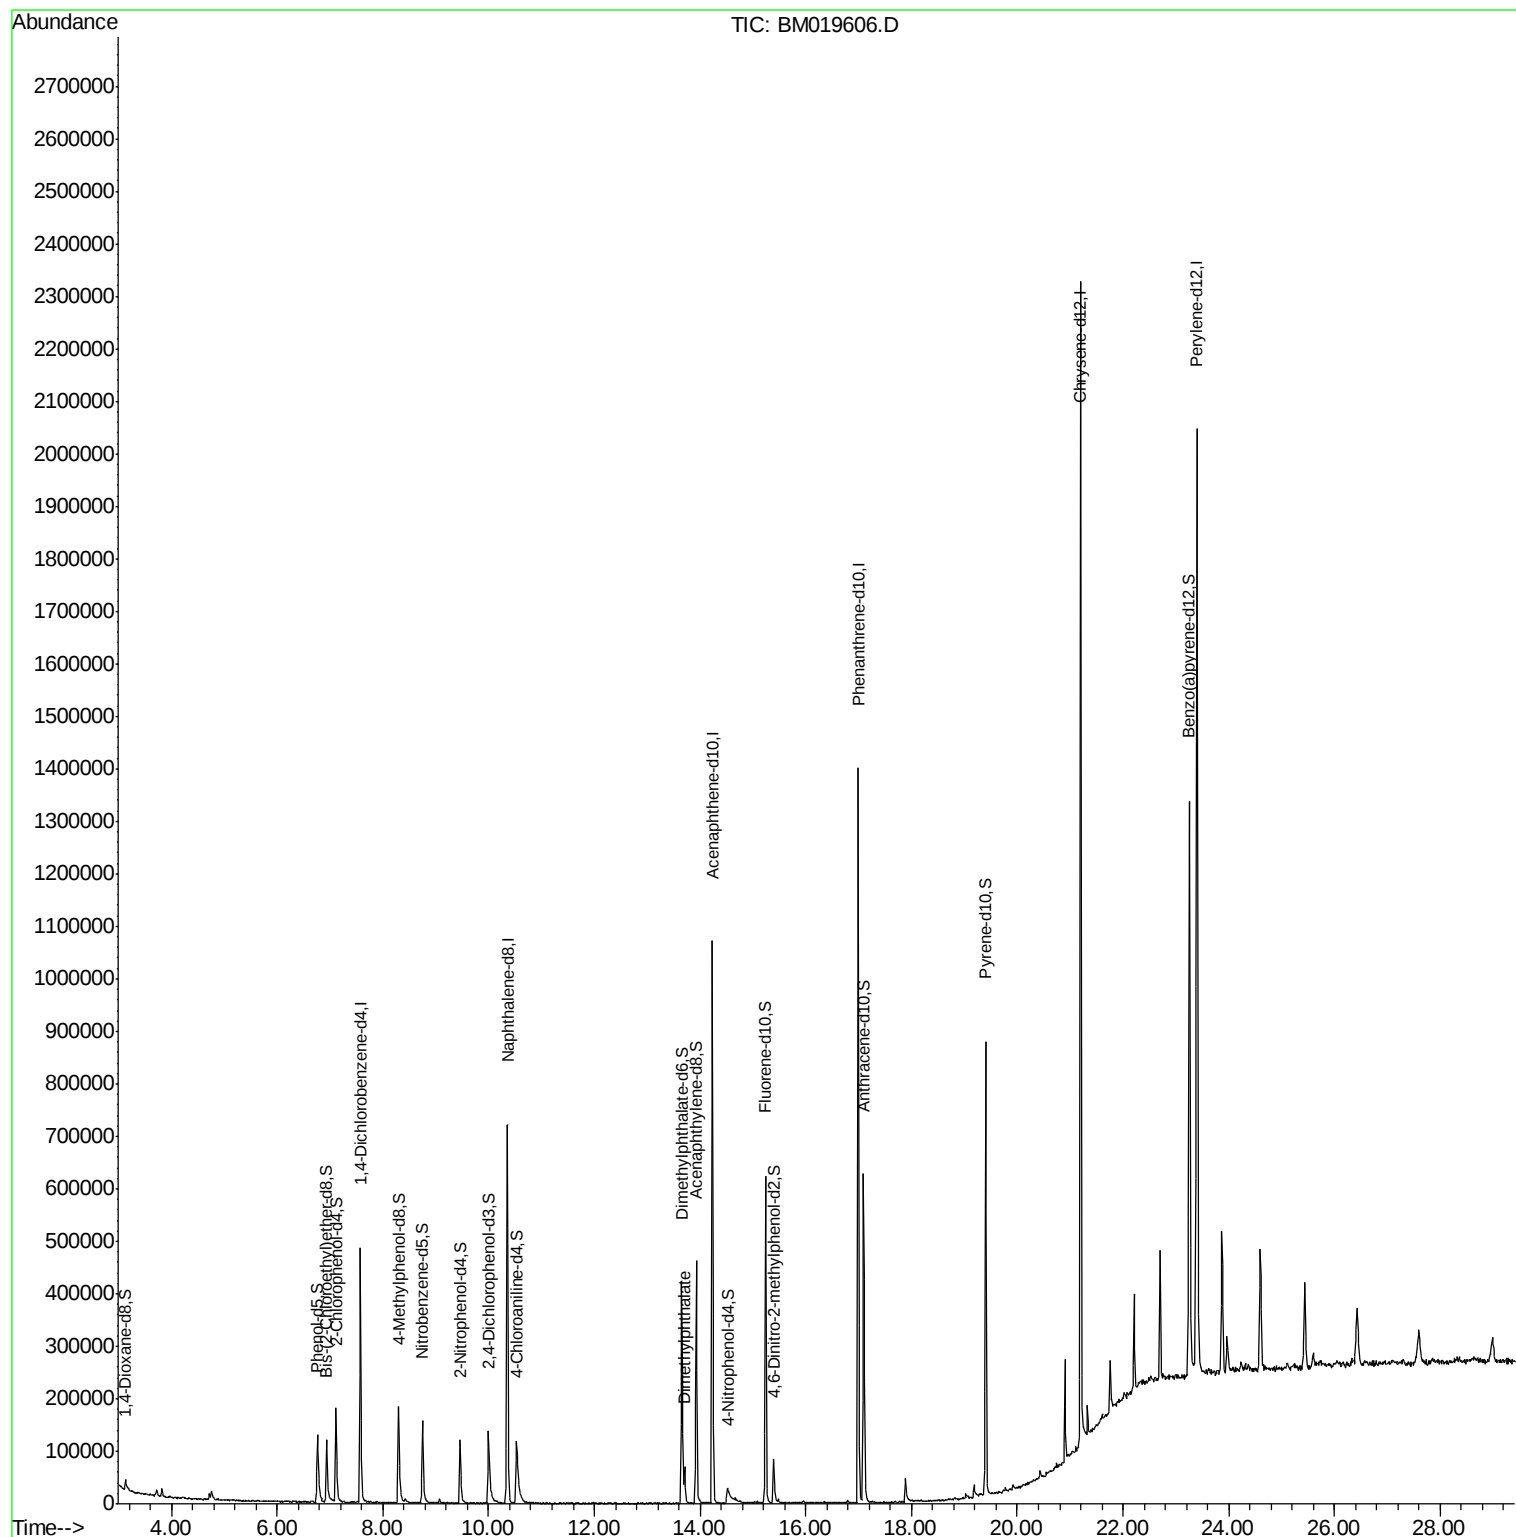


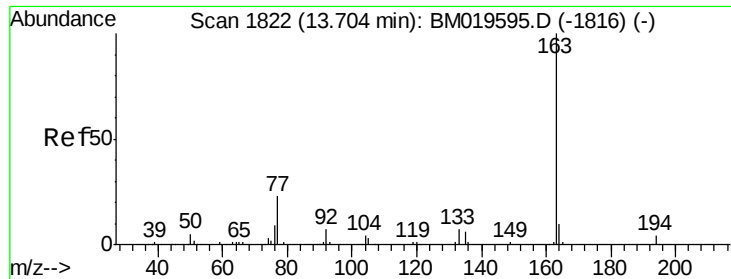

#45
 Dimethylphthalate
 Concen: 1.603 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.00 min
 Lab File: BM019606.D
 Acq: 30 Mar 2019 07:07

Instrument :
 BNA_M
 ClientSampleId :
 BF5B2

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.4	4.0	6.0
164	9.4	8.4	12.6

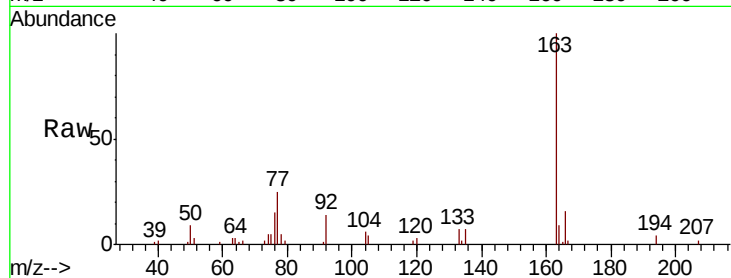

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

