

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019609.D
 Acq On : 30 Mar 2019 08:56
 Operator : JU/SJ
 Sample : K2122-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5C1

Quant Time: Mar 30 20:56:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	134975	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	615743	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	351553	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	805768	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	985430	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1232390	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	25490	7.39	ng/uL	0.00
5) Phenol-d5	6.76	99	285439	23.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	197845	24.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	230883	25.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	210408	23.32	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	107231	24.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	124716	25.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	205650	22.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	290869	26.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	760757	26.82	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	934038	26.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	101117	22.74	ng/ul	0.00
58) Fluorene-d10	15.24	176	658174	26.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	99440	18.66	ng/ul	0.00
71) Anthracene-d10	17.09	188	1047934	27.10	ng/ul	0.00
79) Pyrene-d10	19.40	212	1193495	26.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1600128	24.49	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.70	163	109323	3.841 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019609.D
Acq On : 30 Mar 2019 08:56
Operator : JU/SJ
Sample : K2122-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5C1

Quant Time: Mar 30 20:56:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

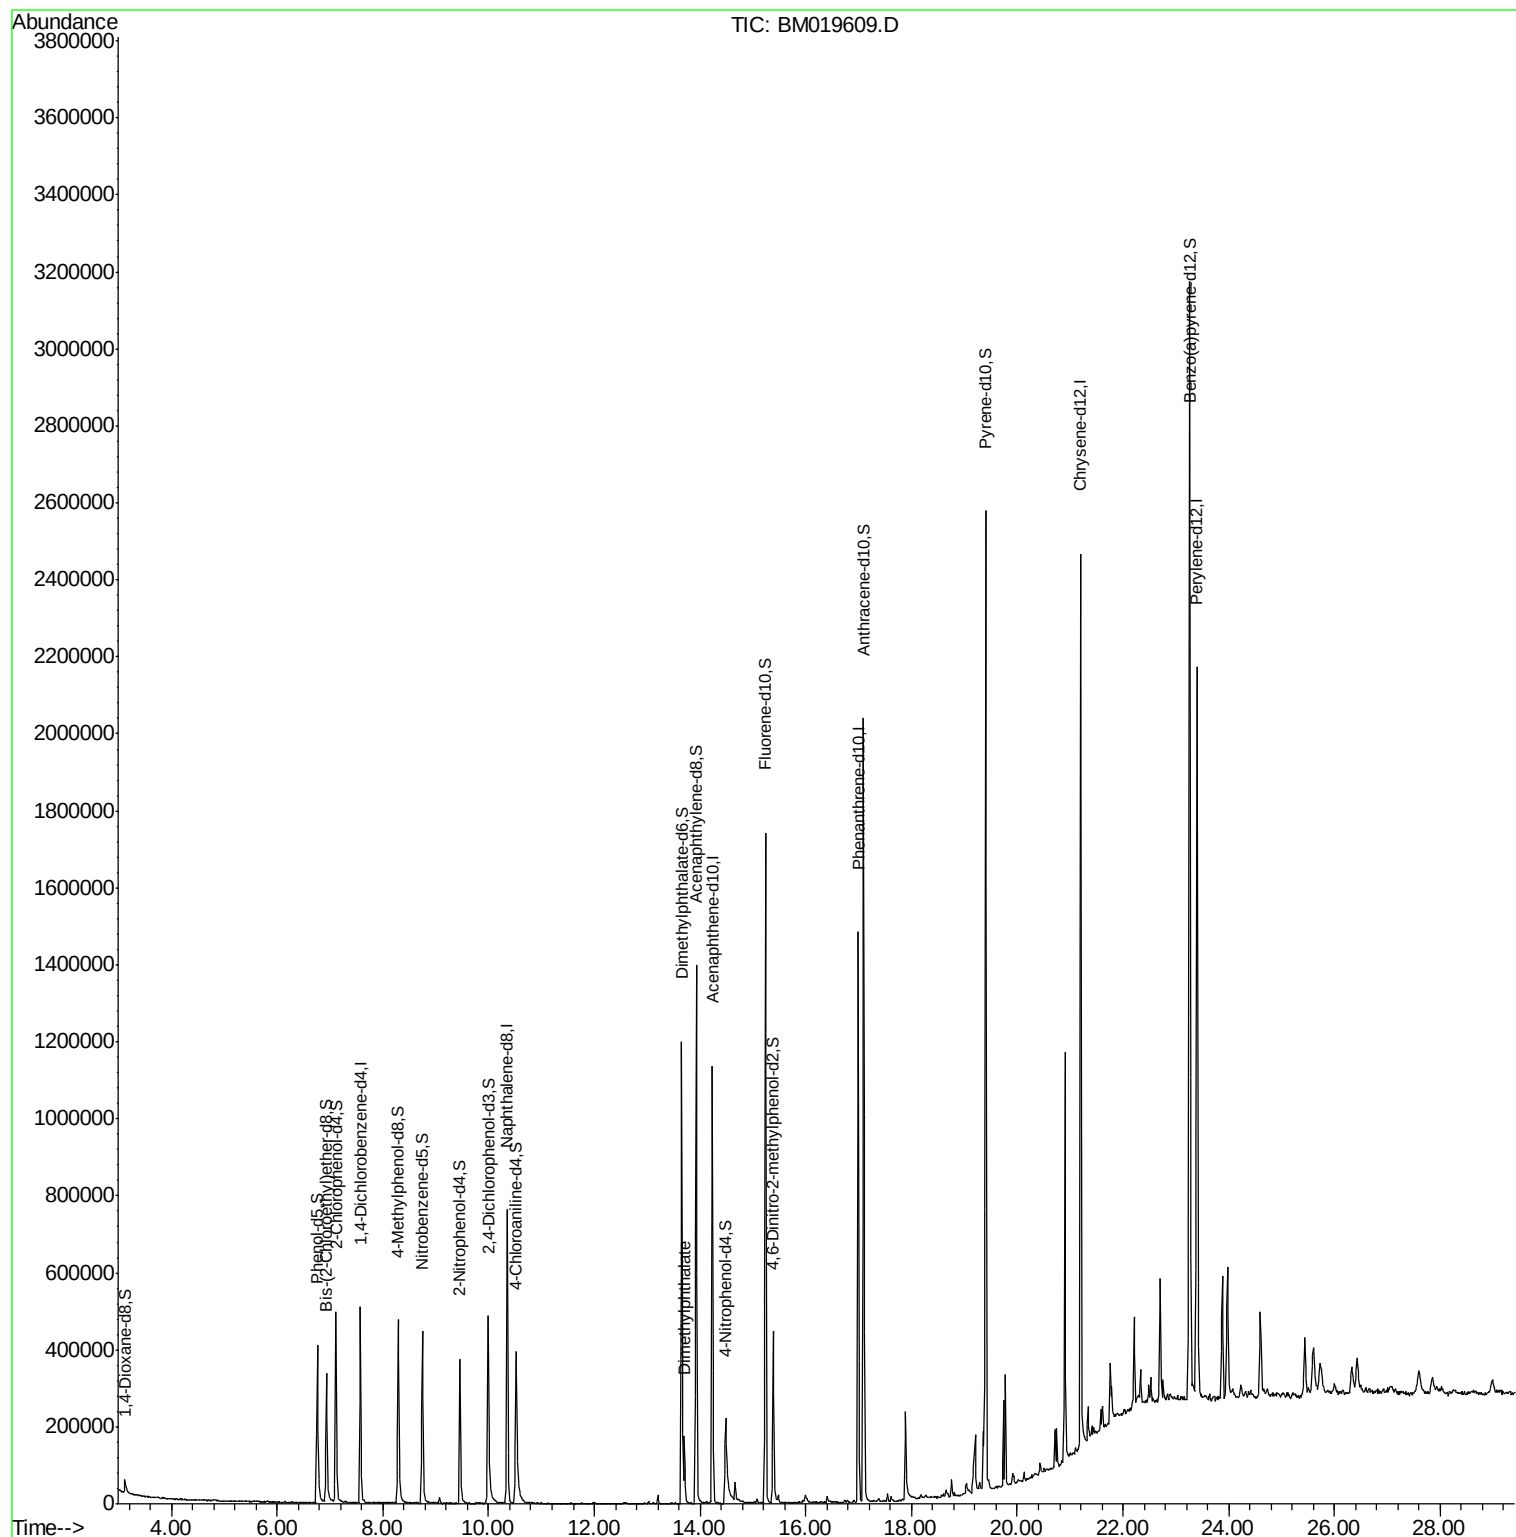

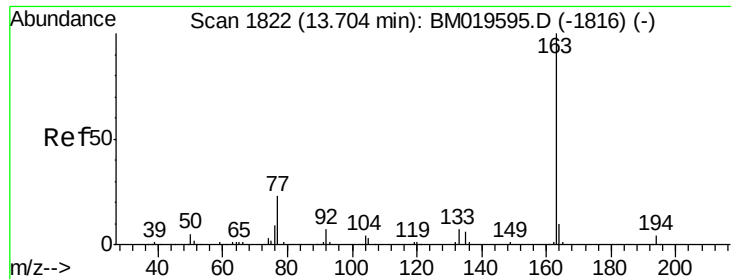

#45
 Dimethylphthalate
 Concen: 3.841 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019609.D
 Acq: 30 Mar 2019 08:56

Instrument :
 BNA_M
 ClientSampleId :
 BF5C1

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	4.0	6.0
164	11.1	8.4	12.6

