

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019585.D
 Acq On : 29 Mar 2019 18:24
 Operator : JU/SJ
 Sample : K2085-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF7T5

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:37 PM

Quant Time: Mar 29 23:26:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	110639	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	498491	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	277054	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	662260	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	825225	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1025093	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	12015	4.25	ng/uL	0.00
5) Phenol-d5	6.77	99	96646	9.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	72252	10.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	81082	10.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	77182	10.44	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	37260	10.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	38946	9.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	66897	8.96	ng/ul	0.01
29) 4-Chloroaniline-d4	10.56	131	37090m	4.14	ng/ul	0.04
44) Dimethylphthalate-d6	13.66	166	284893	12.74	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	307604	11.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	24005m	6.85	ng/ul	0.04
58) Fluorene-d10	15.24	176	233883	12.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	25408	5.80	ng/ul	0.00
71) Anthracene-d10	17.10	188	386421	12.16	ng/ul	0.00
79) Pyrene-d10	19.40	212	447460	11.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	594373	10.94	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.71	163	53941	2.405	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019585.D
Acq On : 29 Mar 2019 18:24
Operator : JU/SJ
Sample : K2085-10
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF7T5

Manual Integrations
APPROVED

Sohil
4/1/2019 5:48:37 PM

Quant Time: Mar 29 23:26:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

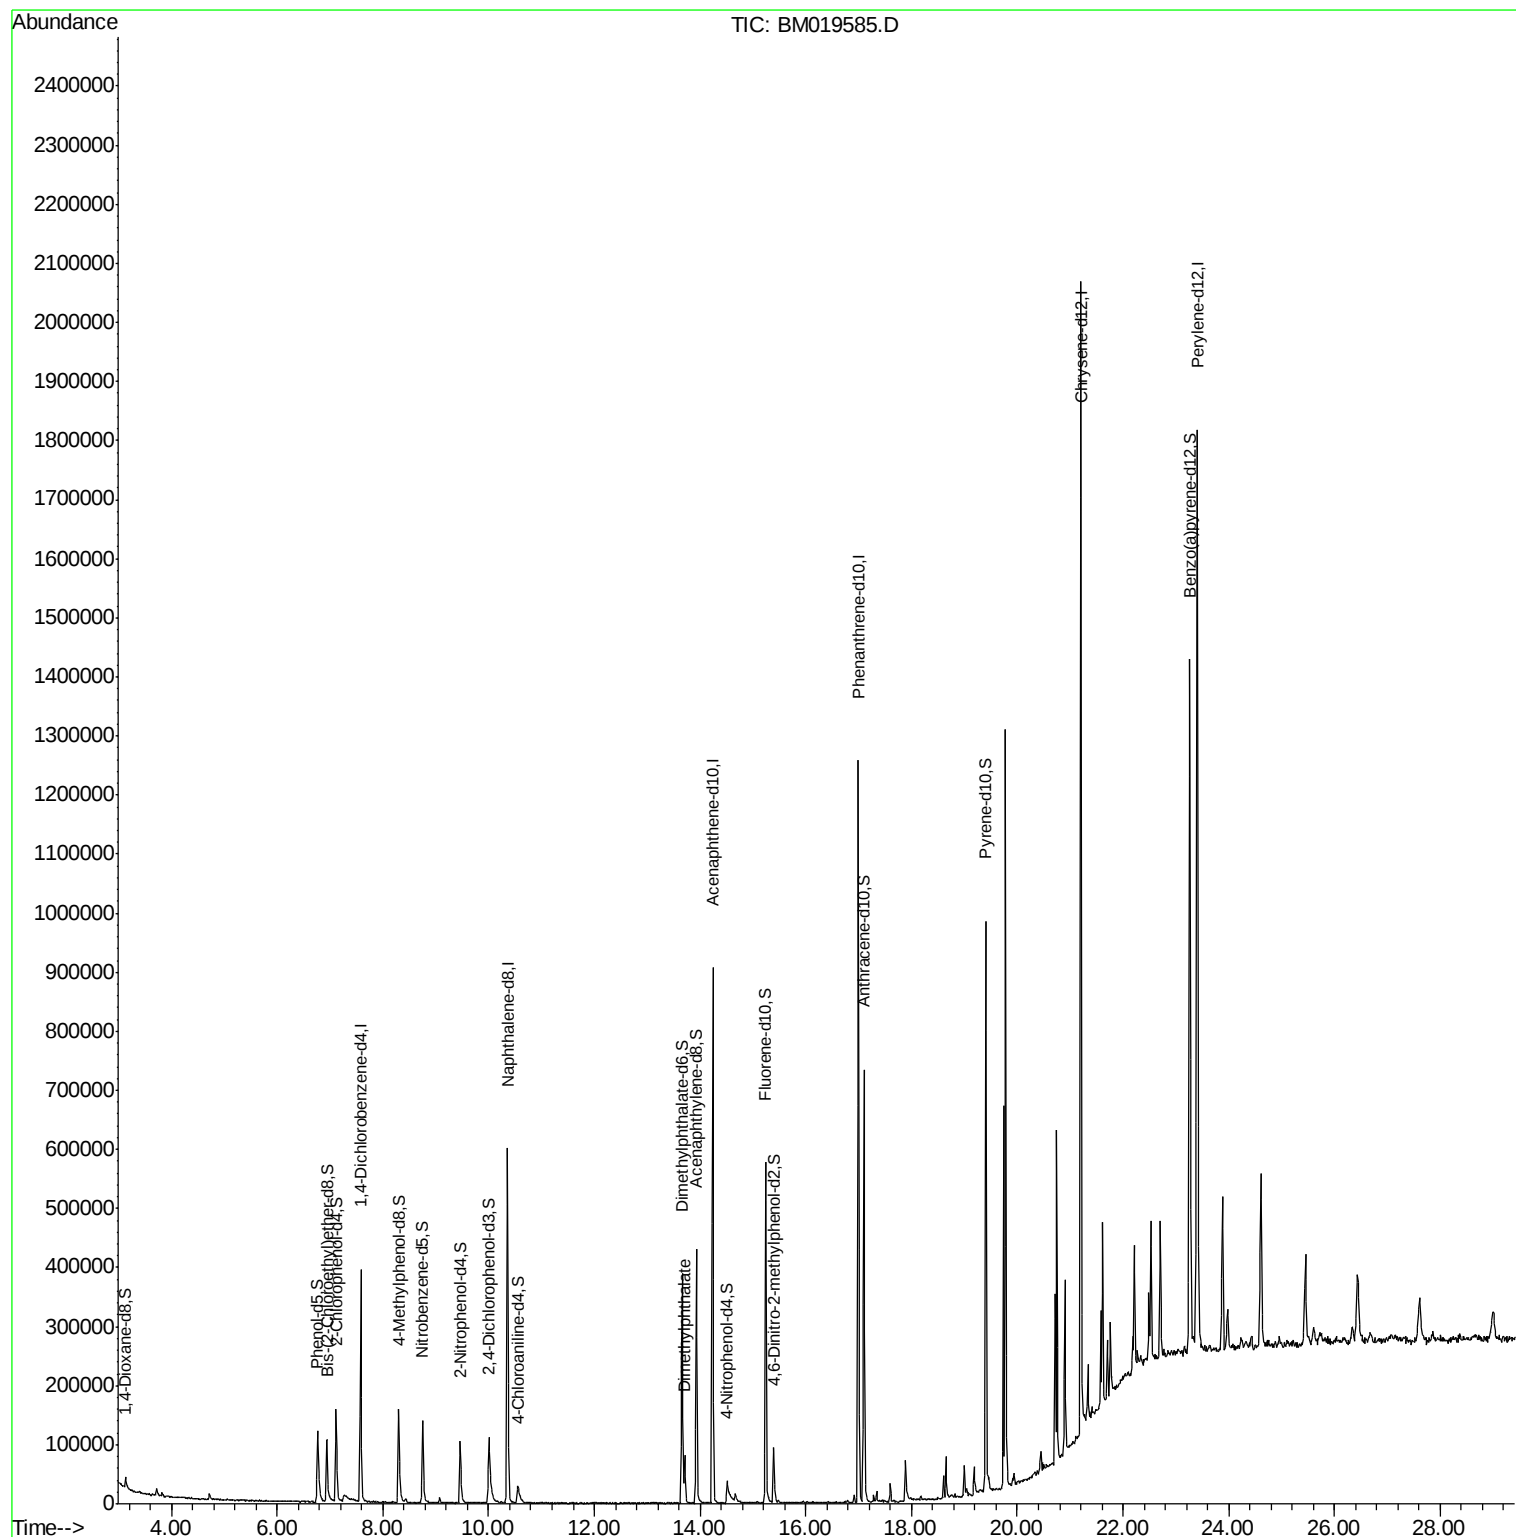

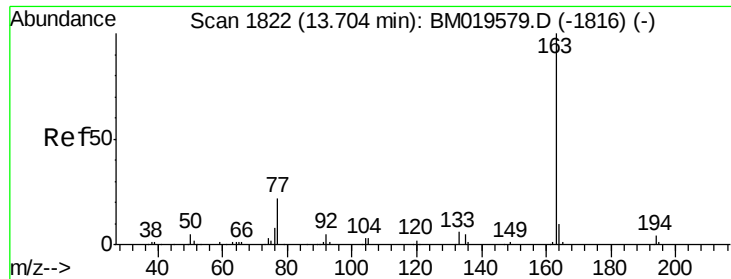

#45
 Dimethylphthalate
 Concen: 2.405 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.00 min
 Lab File: BM019585.D
 Acq: 29 Mar 2019 18:24

Instrument :
 BNA_M
 ClientSampleId :
 BF7T5

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	53941		
194	4.1		4.0	6.0
164	10.7		8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:37 PM

