

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019600.D
 Acq On : 30 Mar 2019 03:30
 Operator : JU/SJ
 Sample : K2084-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF7X6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:45 PM

Quant Time: Mar 30 06:01:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	131067	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	595363	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	333899	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	759059	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	930587	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1168743	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	18915	5.65	ng/uL	0.00
5) Phenol-d5	6.76	99	242713	20.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	159364	20.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	193815	21.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	193174	22.05	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	87229	20.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	99243	21.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	181027	20.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	252351	23.56	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	622522	23.11	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	754829	22.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	80312m	19.02	ng/ul	0.00
58) Fluorene-d10	15.24	176	538449	23.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	76593	15.26	ng/ul	0.00
71) Anthracene-d10	17.09	188	856174	23.50	ng/ul	0.00
79) Pyrene-d10	19.40	212	976604	22.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1383960	22.34	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	99627	3.686	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019600.D
Acq On : 30 Mar 2019 03:30
Operator : JU/SJ
Sample : K2084-08
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF7X6

Manual Integrations
APPROVED

Sohil
4/1/2019 5:48:45 PM

Quant Time: Mar 30 06:01:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

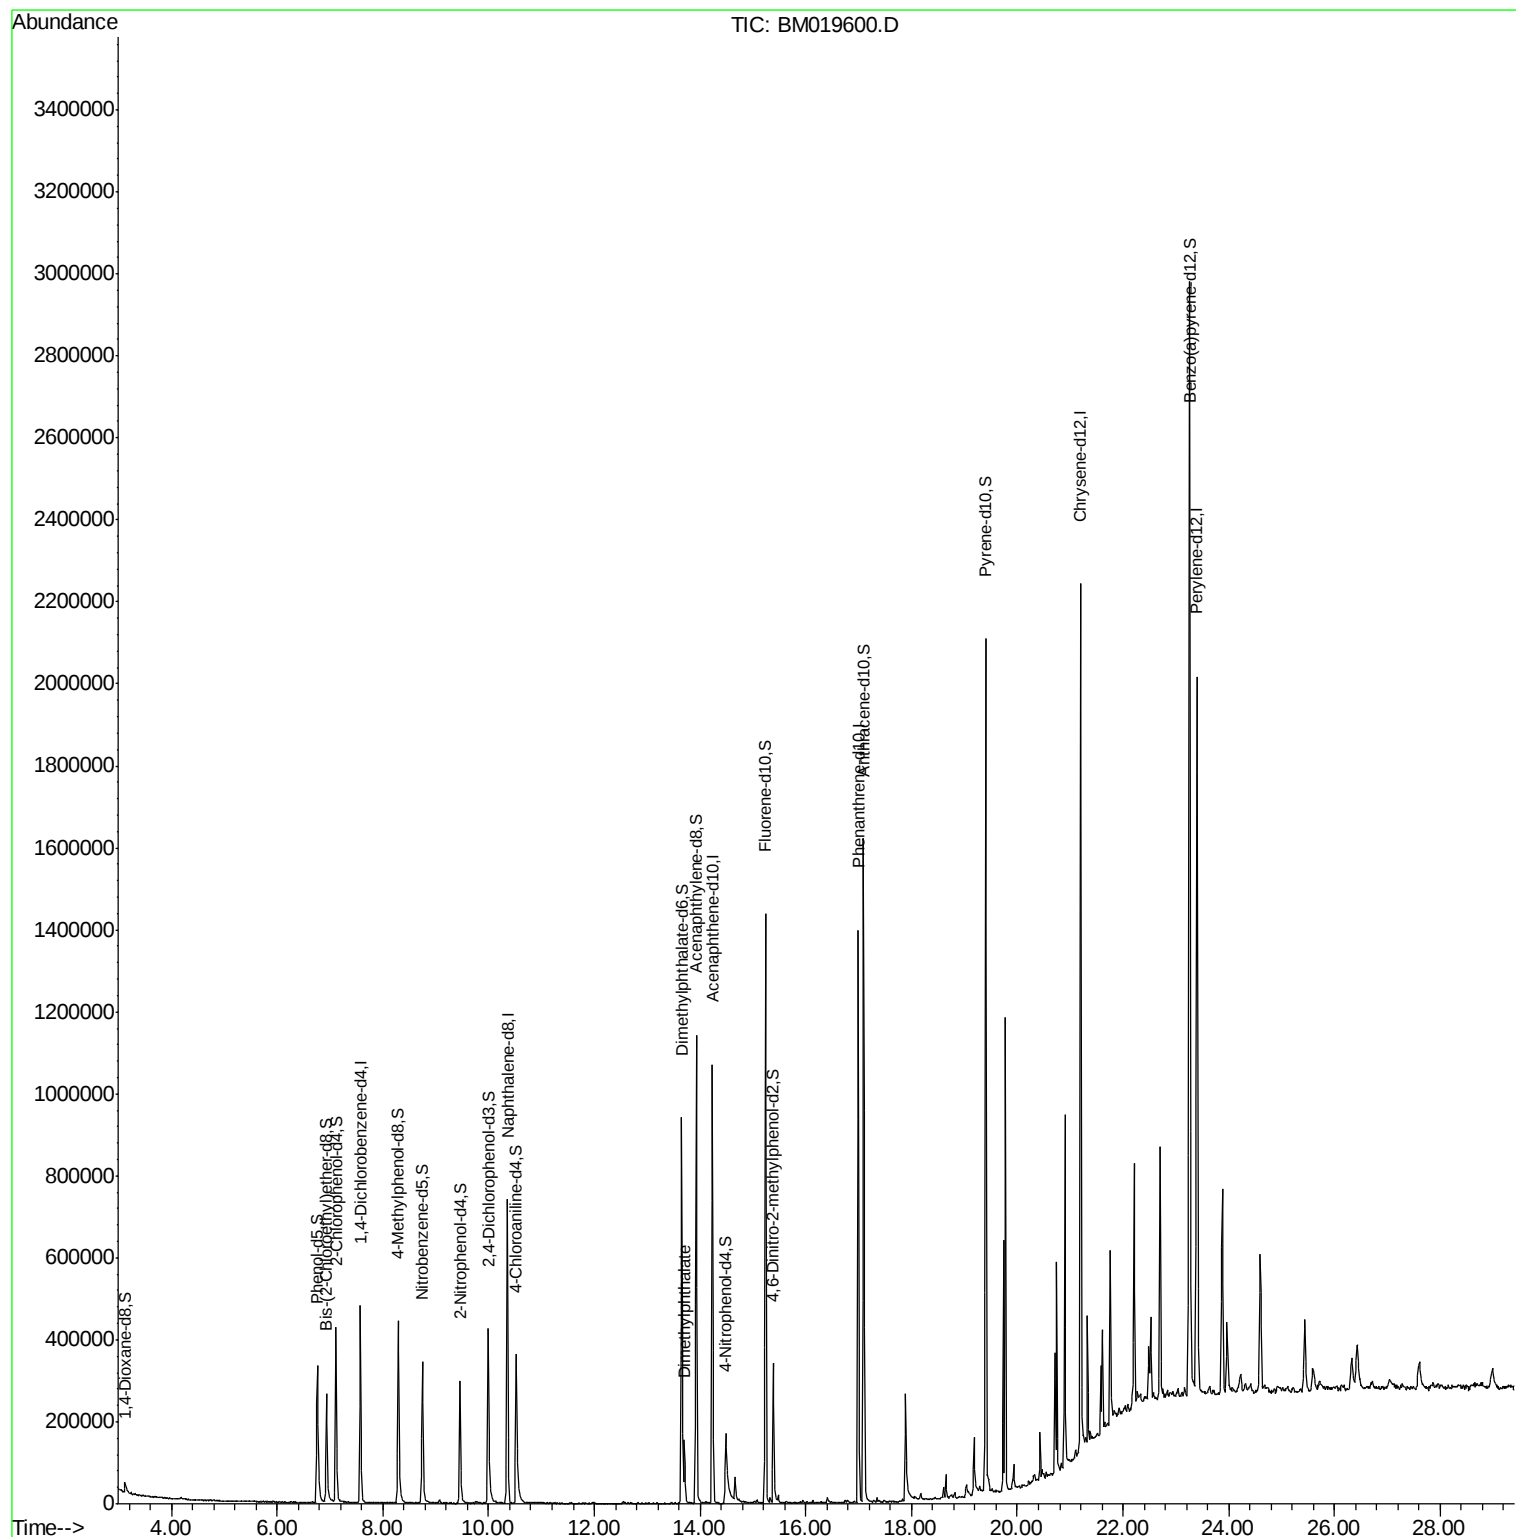

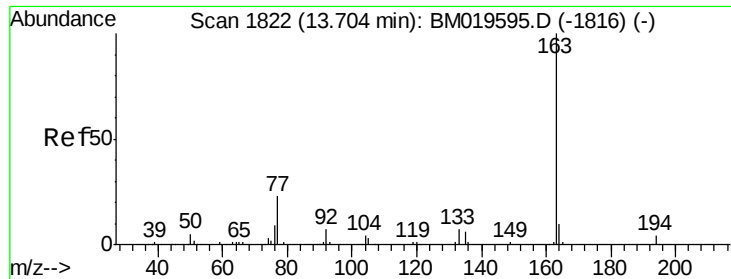

#45
 Dimethylphthalate
 Concen: 3.686 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019600.D
 Acq: 30 Mar 2019 03:30

Instrument :
 BNA_M
 ClientSampleId :
 BF7X6

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	99627		
194	3.6	4.0	6.0#	
164	10.5	8.4	12.6	

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:45 PM

