

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
 Data File : BM019605.D
 Acq On : 30 Mar 2019 06:31
 Operator : JU/SJ
 Sample : K2122-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5B1

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:50 PM

Quant Time: Mar 30 21:03:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	77923	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	343279	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	191030	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	449298	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	645829	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	912253	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	11021m	5.54	ng/uL	0.00
5) Phenol-d5	6.76	99	98222	14.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	69964	15.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	78249	14.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	75593	14.51	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	33524m	13.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	37628	13.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	59421	11.56	ng/ul	0.01
29) 4-Chloroaniline-d4	10.53	131	96293	15.59	ng/ul	0.01
44) Dimethylphthalate-d6	13.66	166	257544	16.71	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	276026	14.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	21963m	9.09	ng/ul	0.04
58) Fluorene-d10	15.24	176	216239	16.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	23875	8.04	ng/ul	0.00
71) Anthracene-d10	17.10	188	337551	15.66	ng/ul	0.00
79) Pyrene-d10	19.40	212	407054	13.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	687154	14.21	ng/ul	0.00

Target Compounds					Qvalue	
45) Dimethylphthalate	13.71	163	48400	3.130	ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032919\
Data File : BM019605.D
Acq On : 30 Mar 2019 06:31
Operator : JU/SJ
Sample : K2122-02
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BF5B1

Quant Time: Mar 30 21:03:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/1/2019 5:48:50 PM

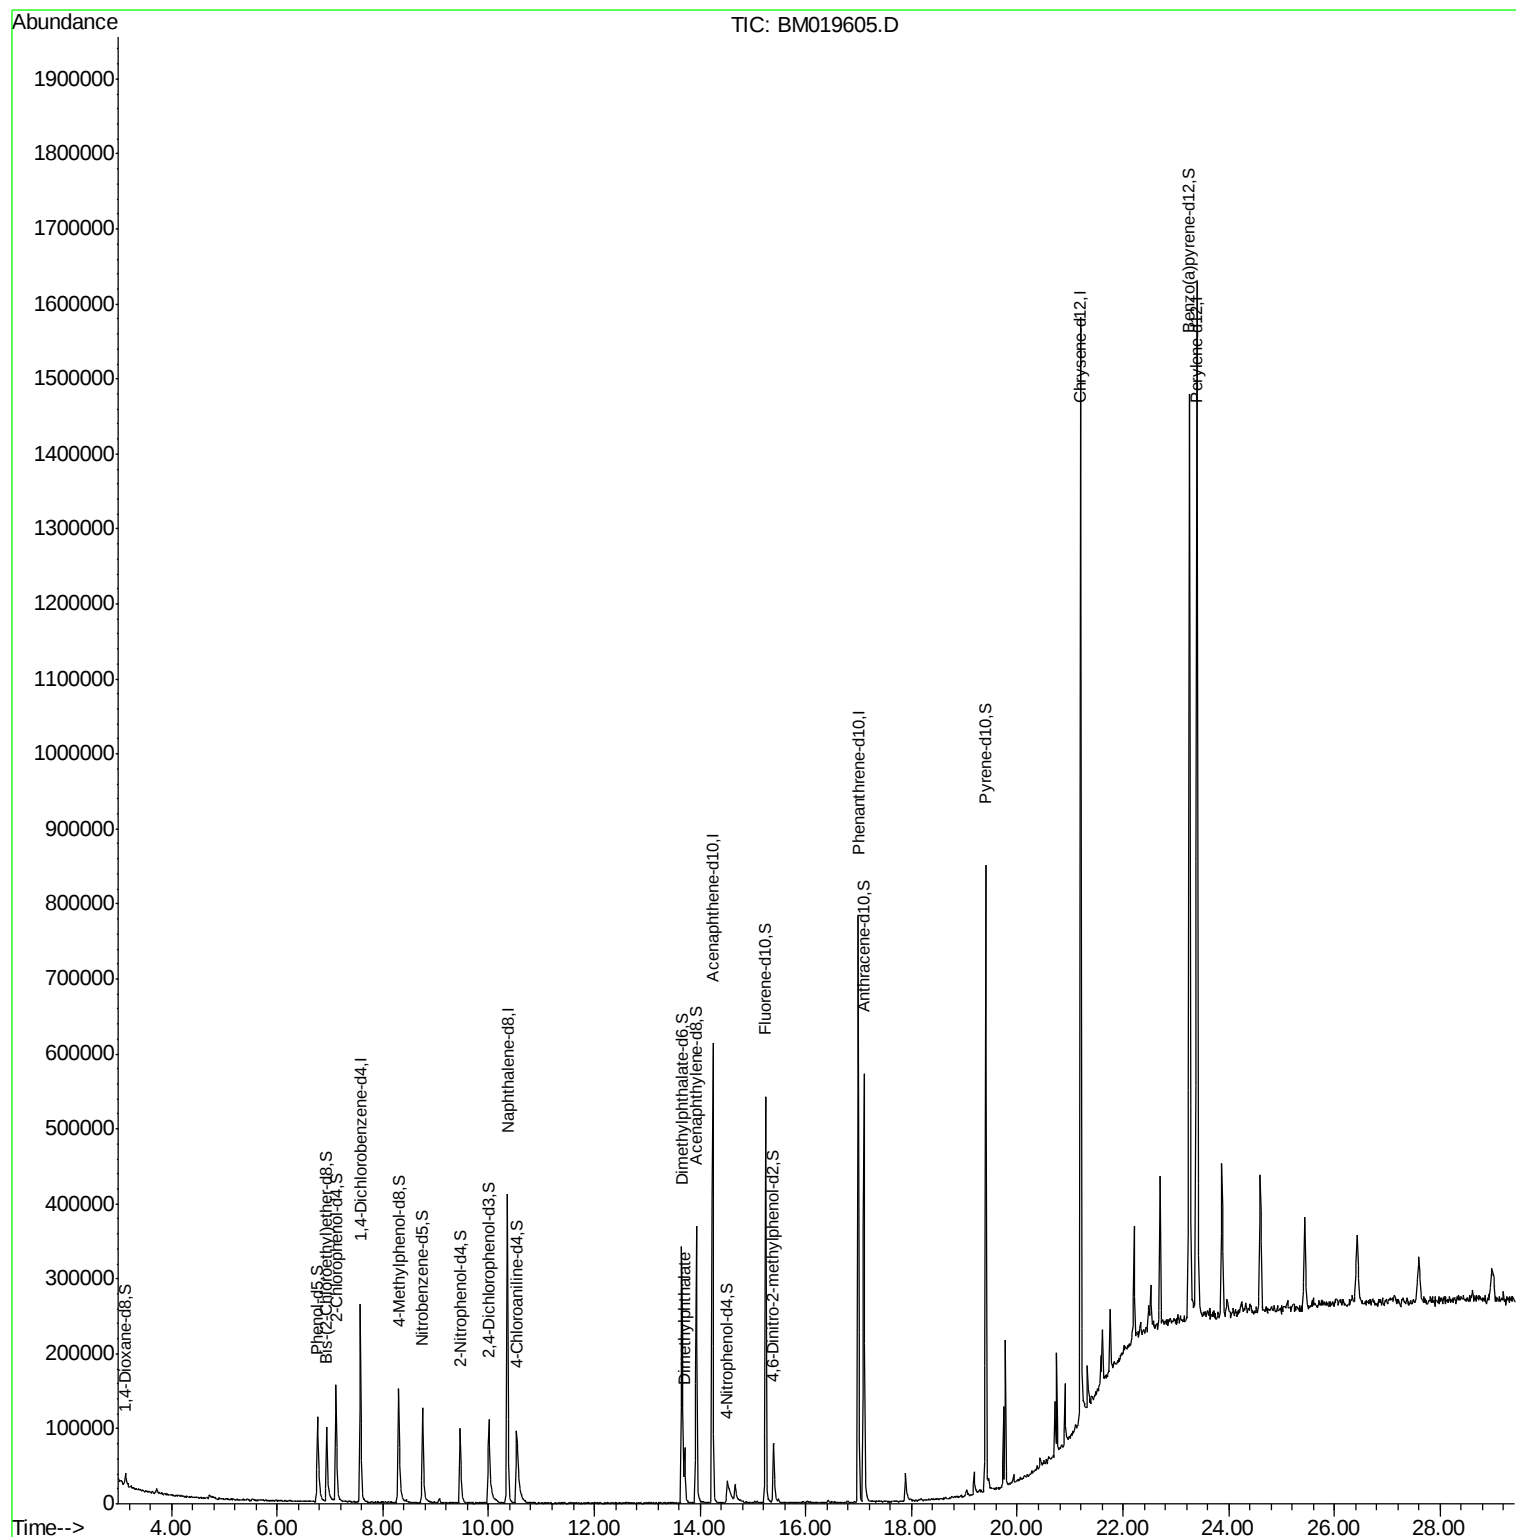

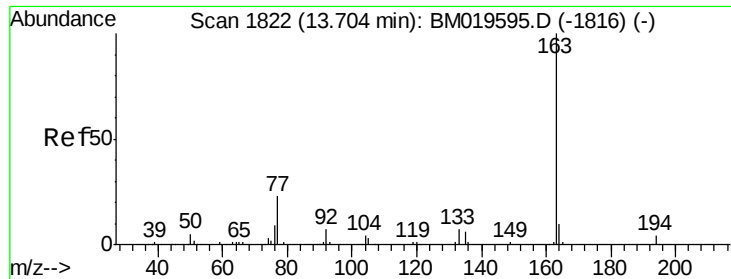

#45
 Dimethylphthalate
 Concen: 3.130 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.00 min
 Lab File: BM019605.D
 Acq: 30 Mar 2019 06:31

Instrument :
 BNA_M
 ClientSampleId :
 BF5B1

Tgt Ion	Ratio	Resp Lower	Upper
163	100		
194	2.9	4.0	6.0#
164	9.2	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:48:50 PM

