
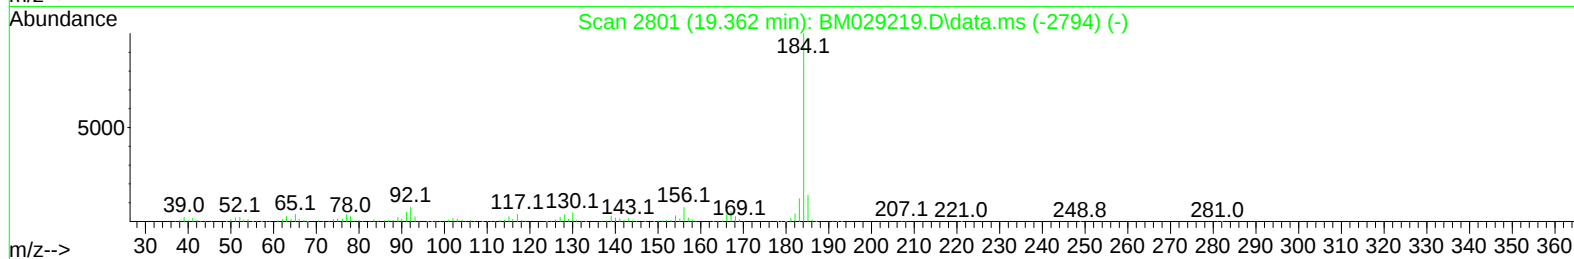
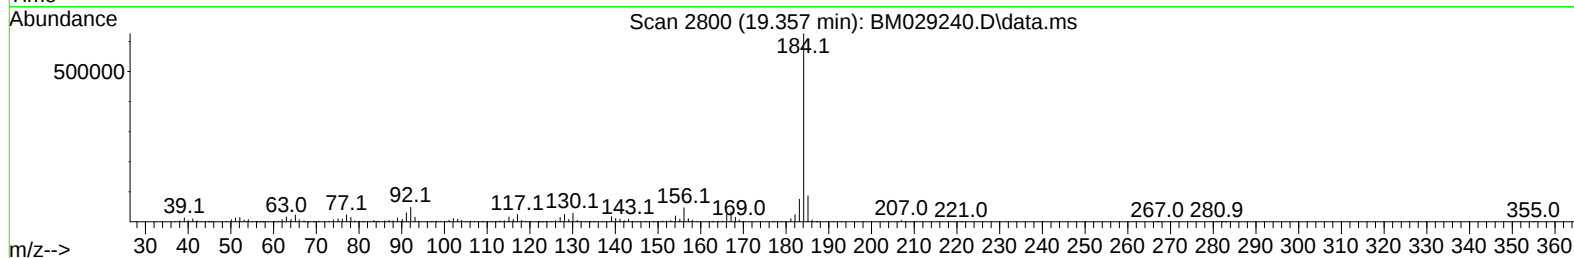


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
Data File : BM029240.D
Acq On : 29 Mar 2021 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 10:47:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 16:05:40 2021
Response via : Initial Calibration

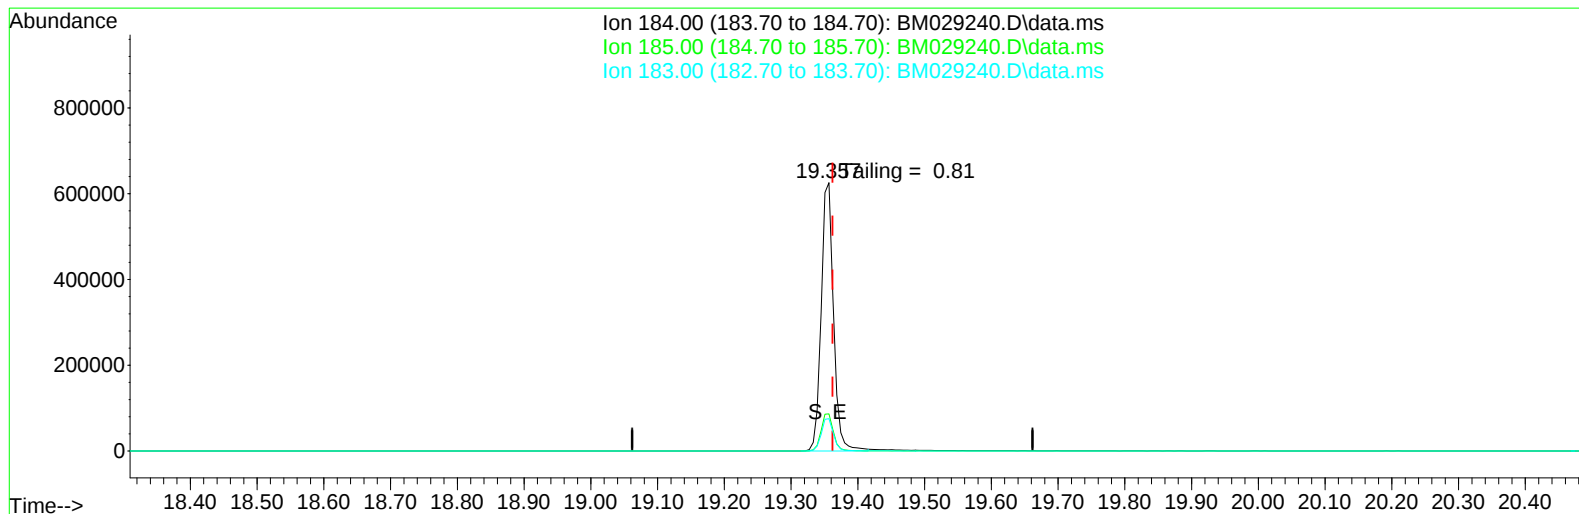

TIC: BM029240.D\data.ms




(77) Benzidine

19.357min (-0.005) 0.00 ng

response 808195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.85
183.00	12.20	12.05
0.00	0.00	0.00

Quant Time: Mar 29 10:47:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 16:05:40 2021
Response via : Initial Calibration

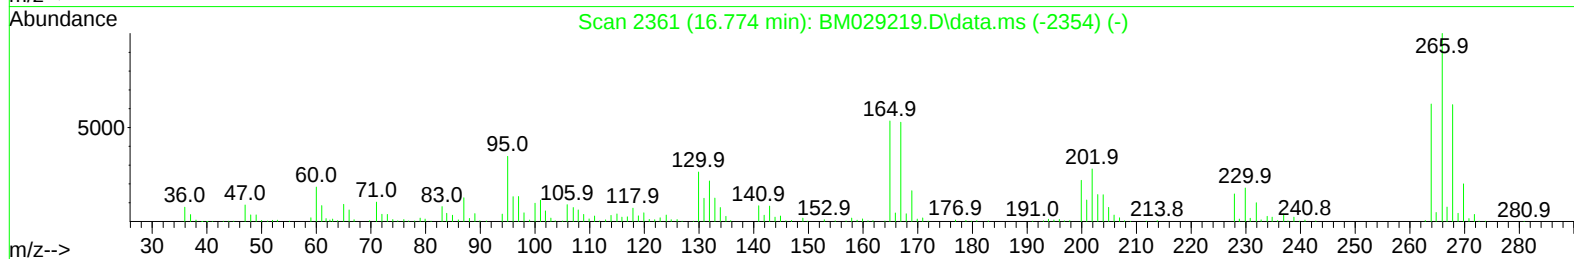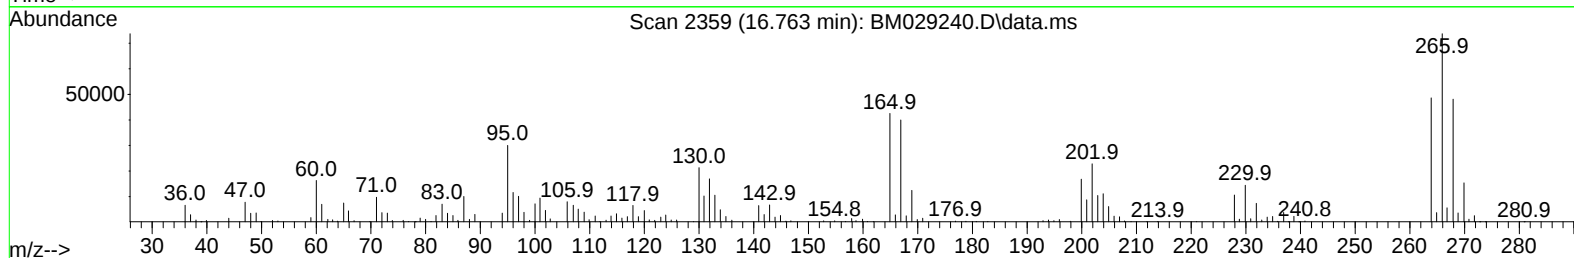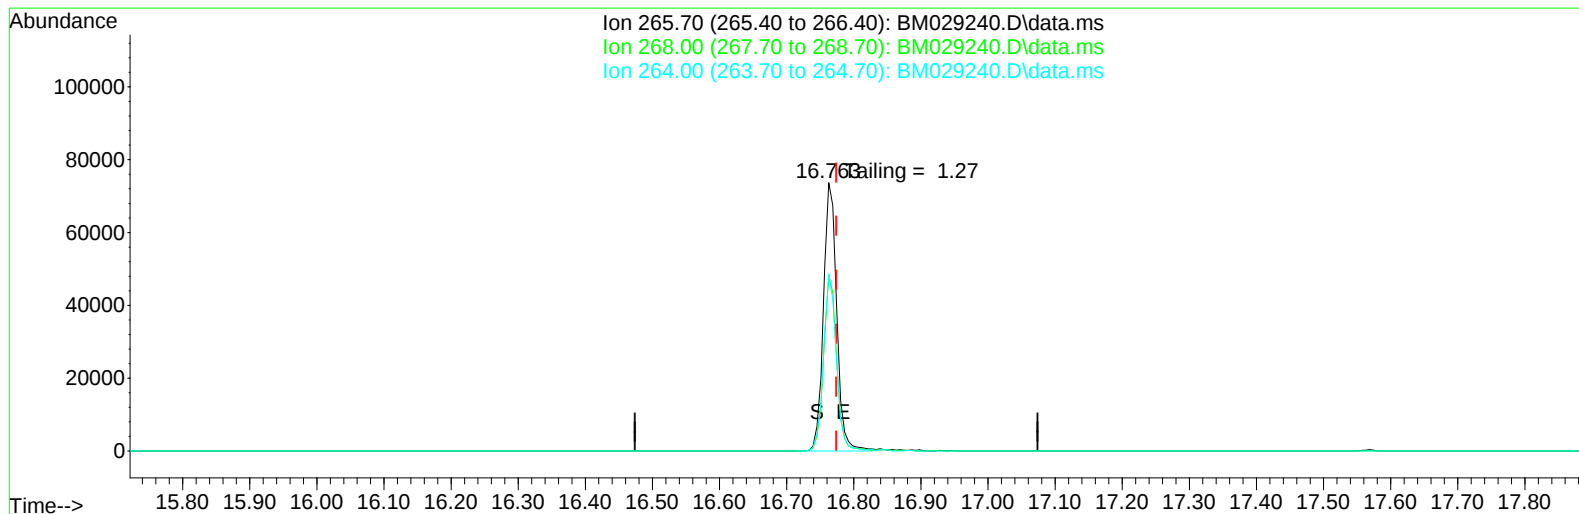

TIC: BM029240.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.011) 0.00 ng

response **102145**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	65.30
264.00	63.60	65.93
0.00	0.00	0.00