
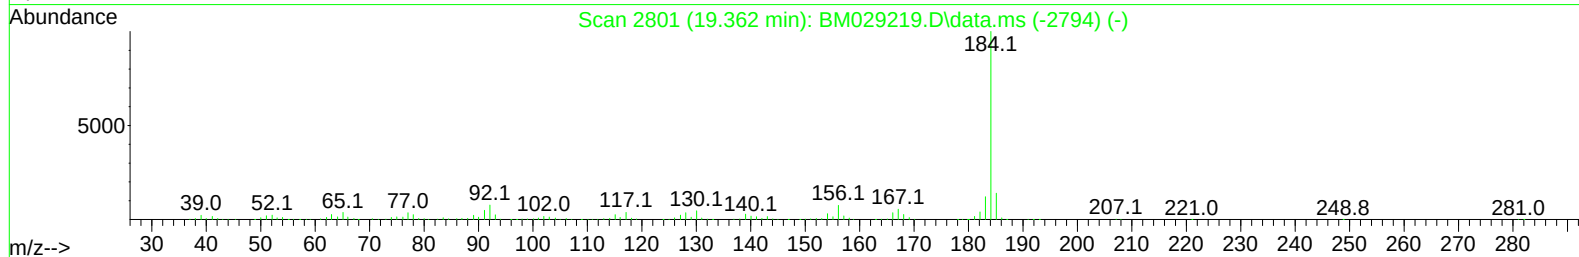
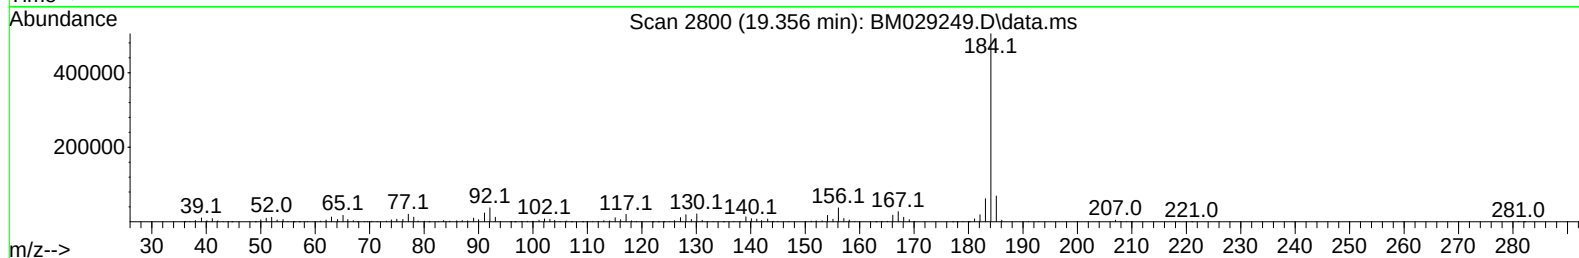


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
Data File : BM029249.D
Acq On : 29 Mar 2021 17:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 18:54:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

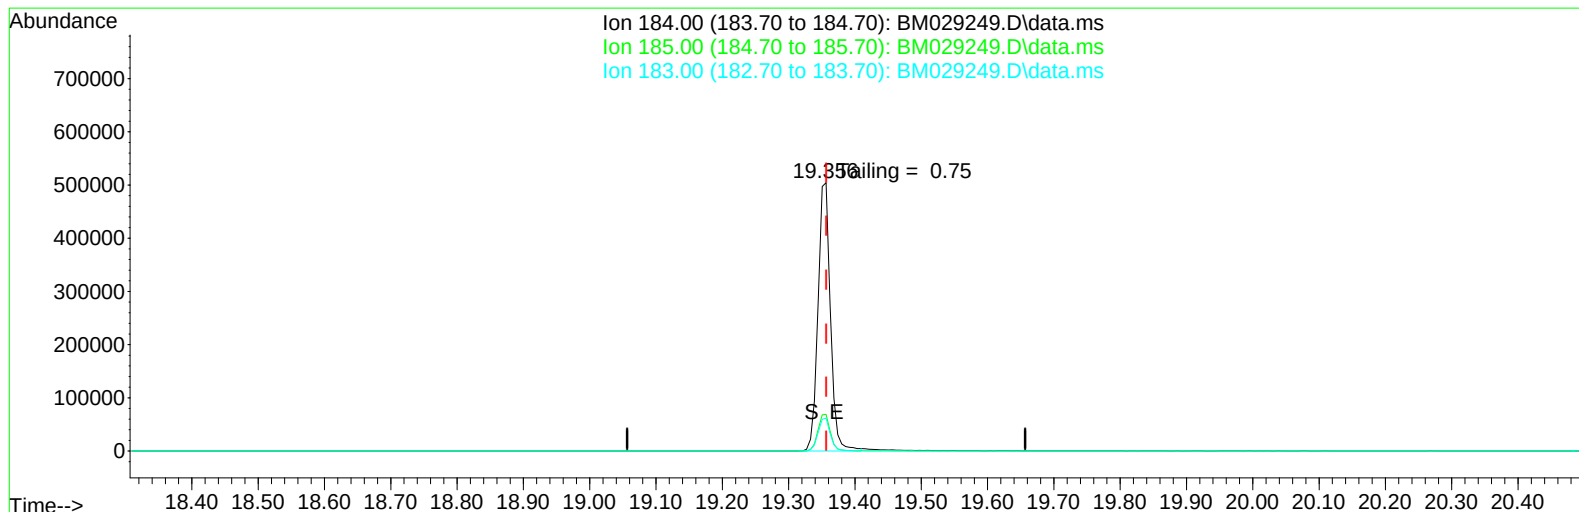

TIC: BM029249.D\data.ms

(77) Benzidine




19.356min (-0.000) 0.00 ng

response 664830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.70
183.00	12.20	12.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
Data File : BM029249.D
Acq On : 29 Mar 2021 17:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 18:54:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

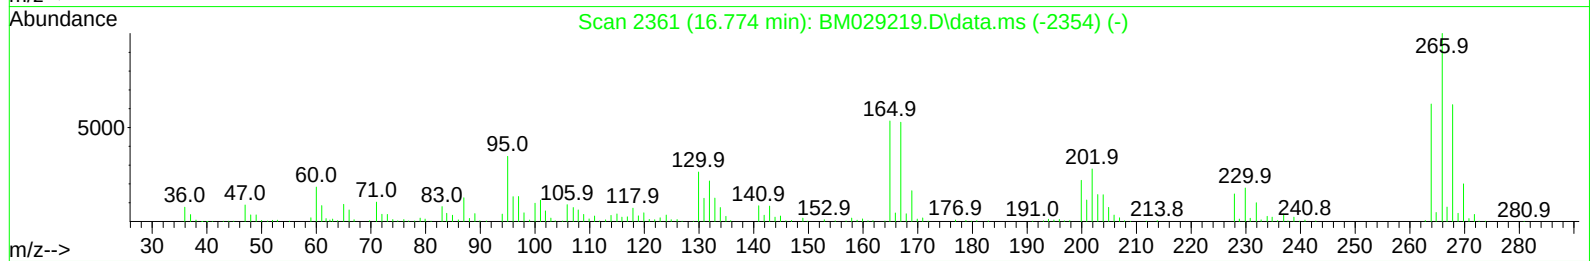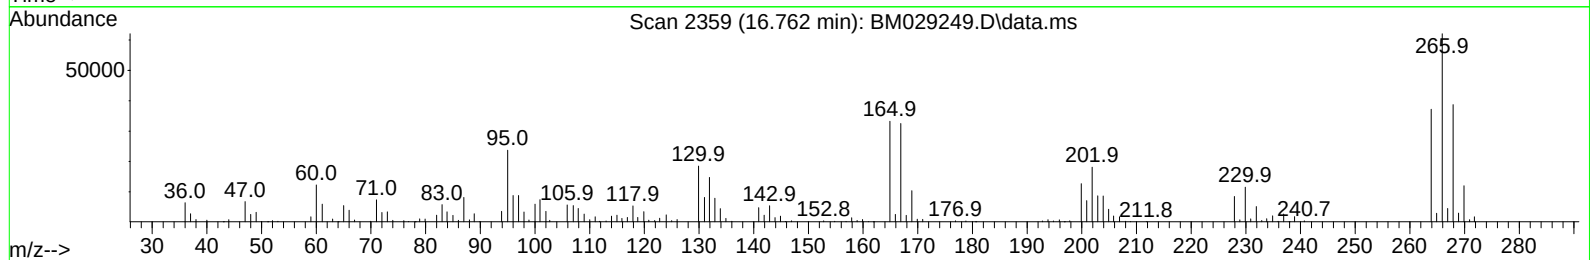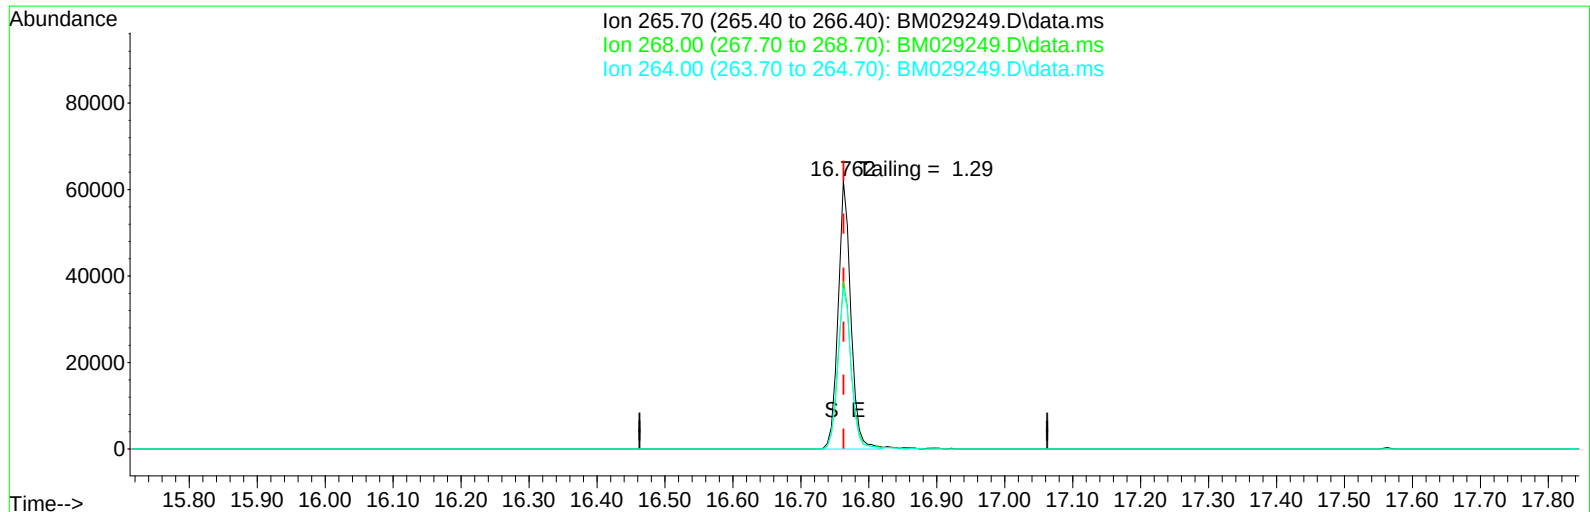

TIC: BM029249.D\data.ms

(70) Pentachlorophenol (C)

16.762min (-0.000) 0.00 ng

response 80981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.43
264.00	63.60	59.90
0.00	0.00	0.00