
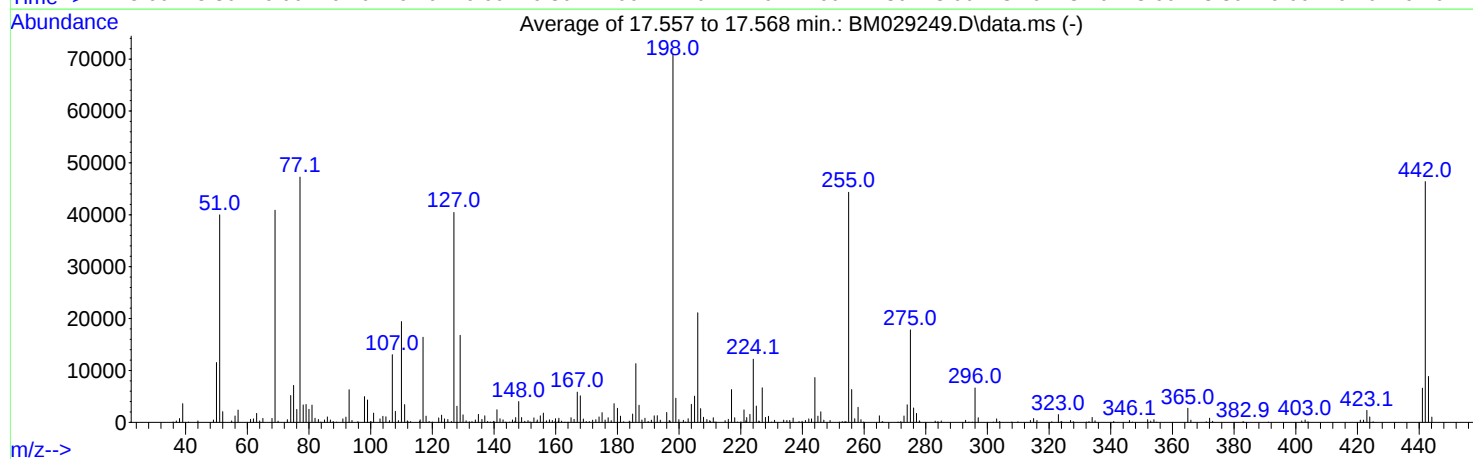


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
 Data File : BM029249.D
 Acq On : 29 Mar 2021 17:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 29 11:14:33 2021

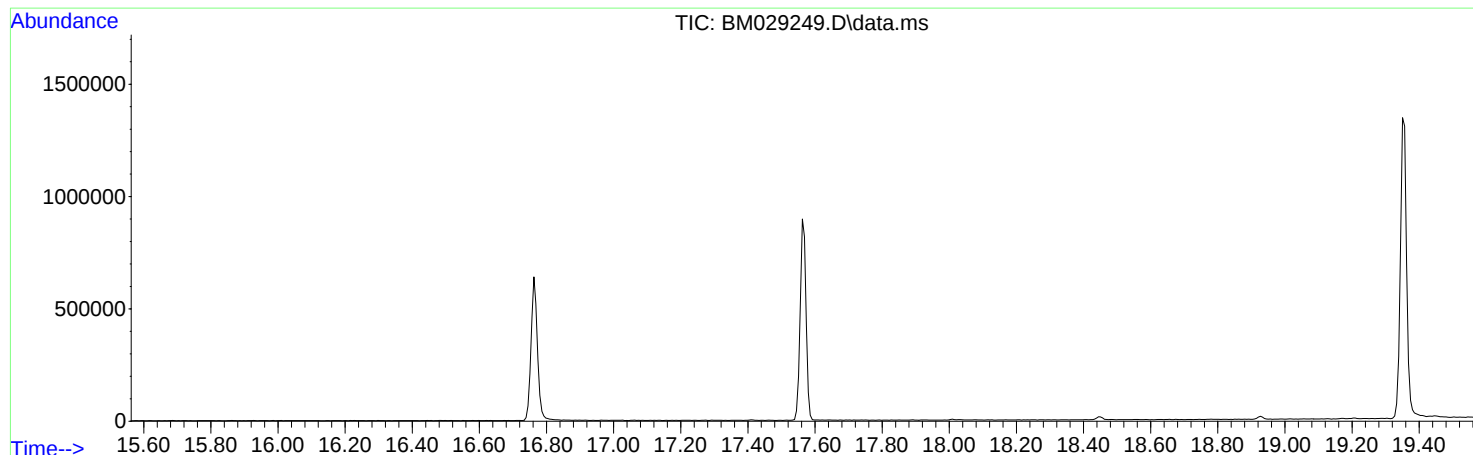




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.4	39997	PASS
68	69	0.00	2	1.9	786	PASS
69	198	0.00	100	57.7	40891	PASS
70	69	0.00	2	0.6	241	PASS
127	198	10	80	57.1	40461	PASS
197	198	0.00	2	0.5	383	PASS
198	198	100	100	100.0	70883	PASS
199	198	5	9	6.6	4645	PASS
275	198	10	60	25.1	17820	PASS
365	198	1	100	3.8	2711	PASS
441	198	0.01	100	9.3	6611	PASS
442	442	50	100	100.0	46397	PASS
443	442	15	24	19.1	8856	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
 Data File : BM029249.D
 Acq On : 29 Mar 2021 17:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 18:54:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 29 11:14:33 2021
 Response via : Initial Calibration

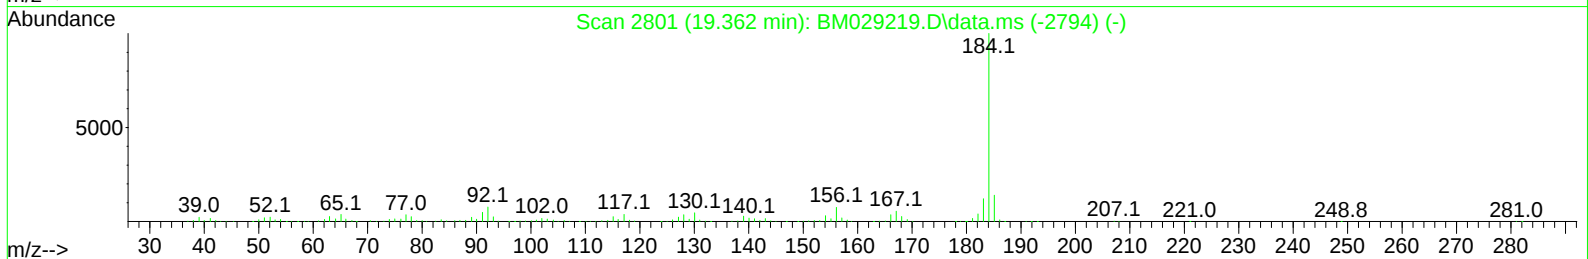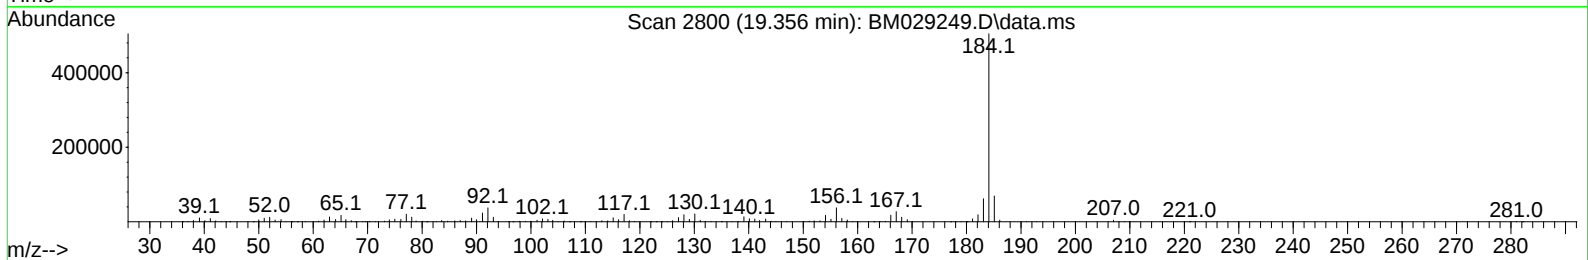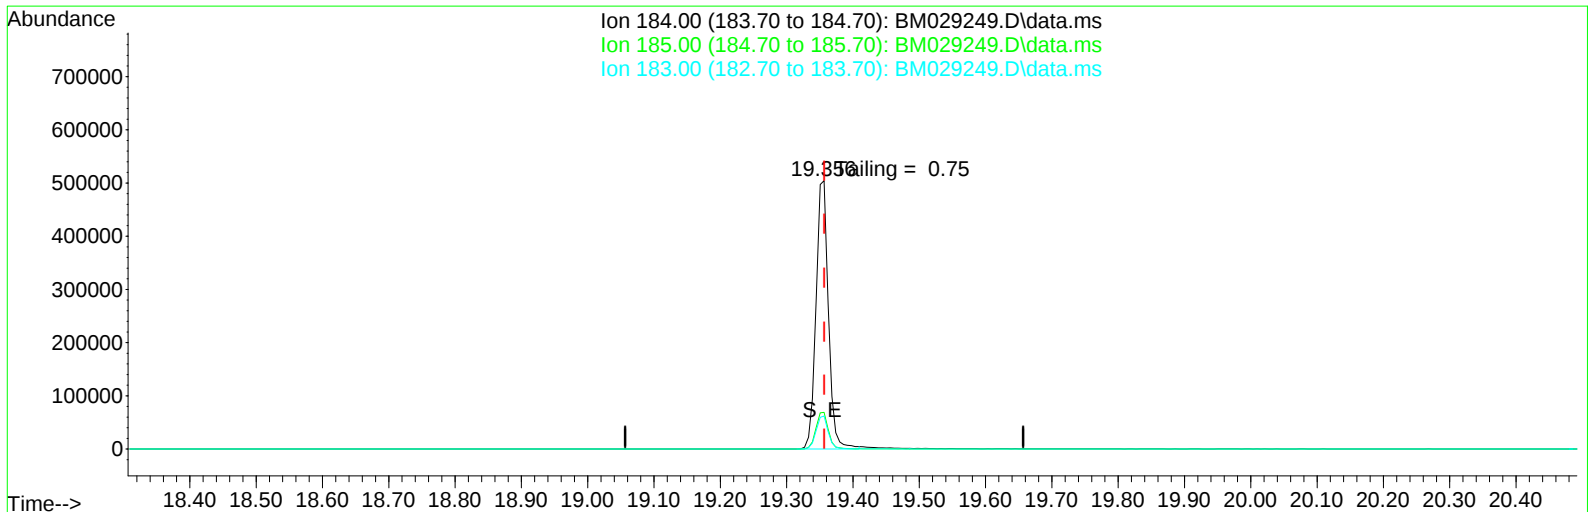

TIC: BM029249.D\data.ms

(77) Benzidine

19.356min (-0.000) 0.00 ng




response 664830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.70
183.00	12.20	12.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032921\
Data File : BM029249.D
Acq On : 29 Mar 2021 17:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 29 18:54:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 29 11:14:33 2021
Response via : Initial Calibration

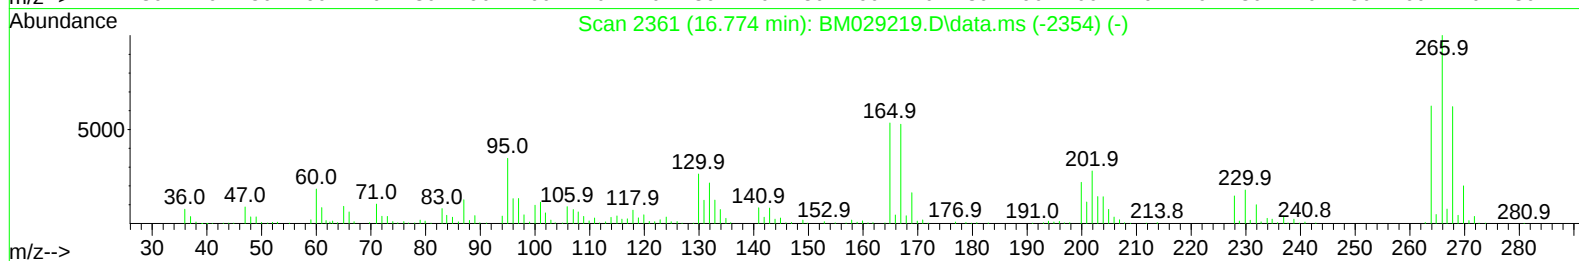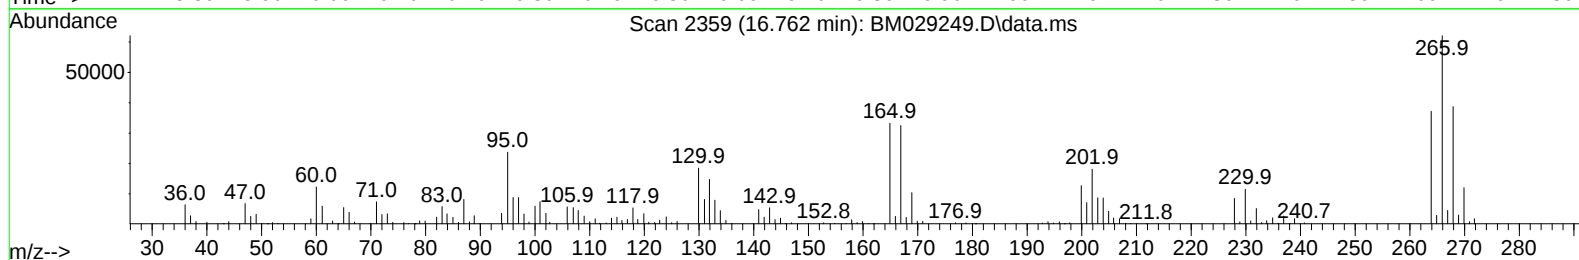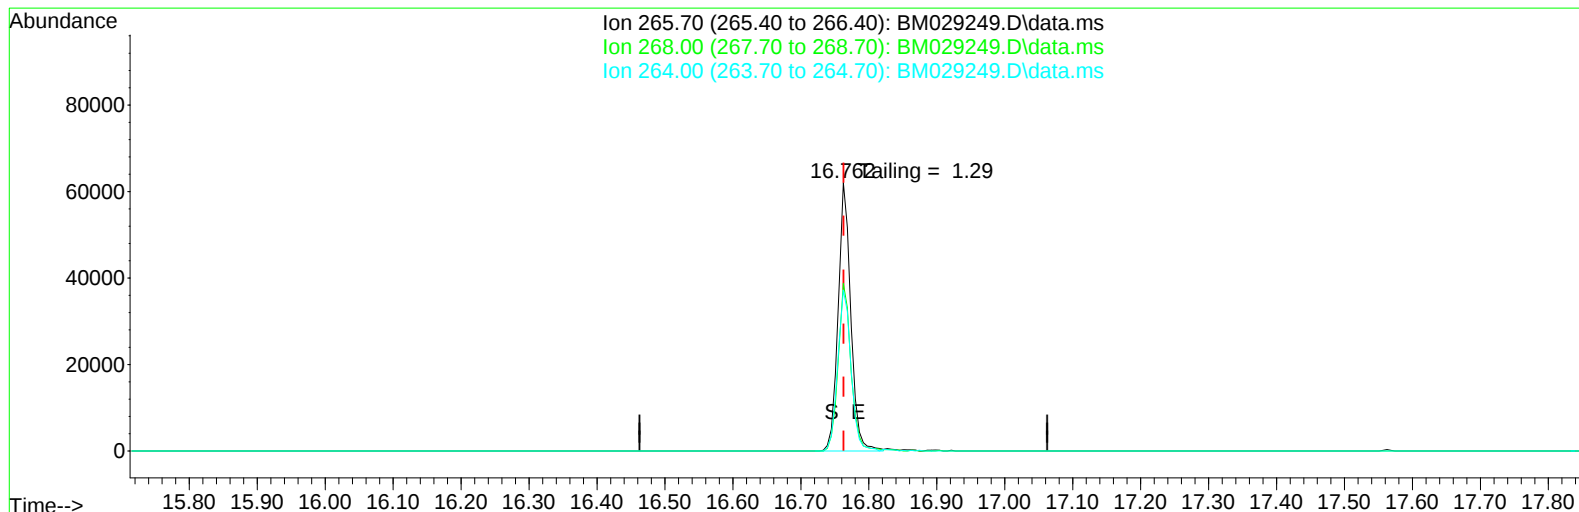

TIC: BM029249.D\data.ms

(70) Pentachlorophenol (C)

16.762min (-0.000) 0.00 ng

response 80981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.43
264.00	63.60	59.90
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/29/2021	BNA_M	<u>BM029249.D</u>
Compound Name	Response	Retention Time
DDT	285520	20.58
DDD	1945	20.15
DDE	331	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2276	287796	0.79

Instrument :
BNA_M
ClientSampleId :
DFTPP